


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051021\
 Data File : BF123881.D
 Acq On : 10 May 2021 11:13
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 10 16:46:01 2021

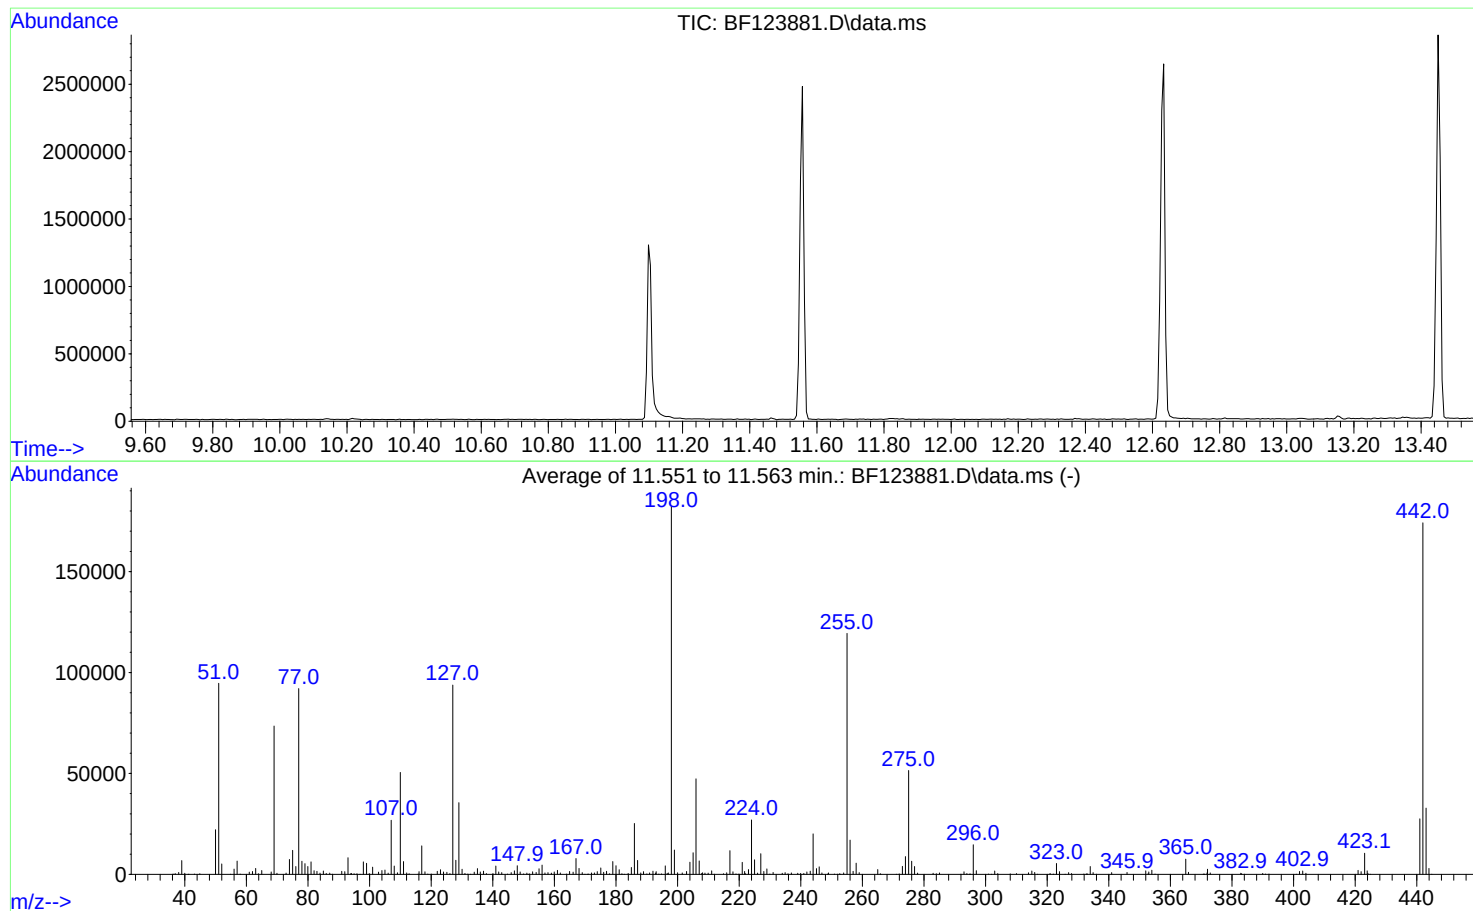




AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1604

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.9	94630	PASS
68	69	0.00	2	1.6	1205	PASS
69	198	0.00	100	40.3	73461	PASS
70	69	0.00	2	0.7	534	PASS
127	198	10	80	51.5	93787	PASS
197	198	0.00	2	0.4	747	PASS
198	198	100	100	100.0	182248	PASS
199	198	5	9	6.6	12035	PASS
275	198	10	60	28.3	51493	PASS
365	198	1	100	4.1	7523	PASS
441	198	0.01	100	15.1	27540	PASS
442	442	50	100	100.0	174152	PASS
443	442	15	24	18.8	32811	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051021\
Data File : BF123881.D
Acq On : 10 May 2021 11:13
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 10 12:16:07 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 07 13:43:24 2021
Response via : Initial Calibration

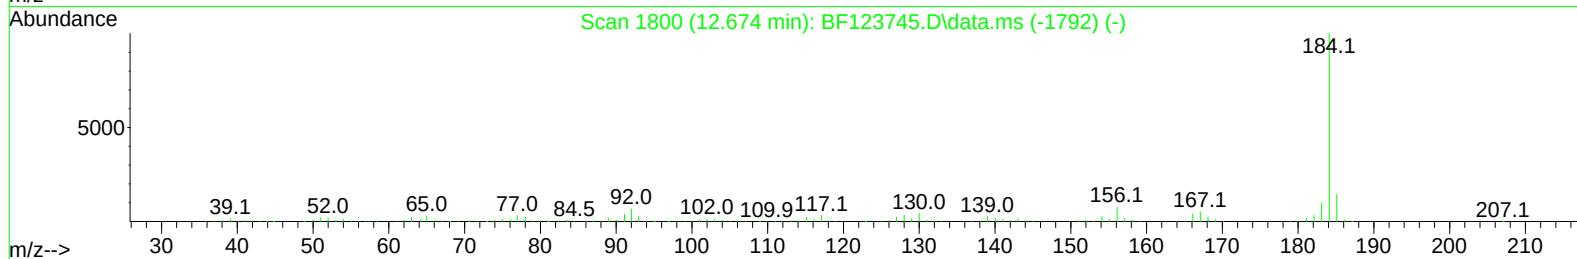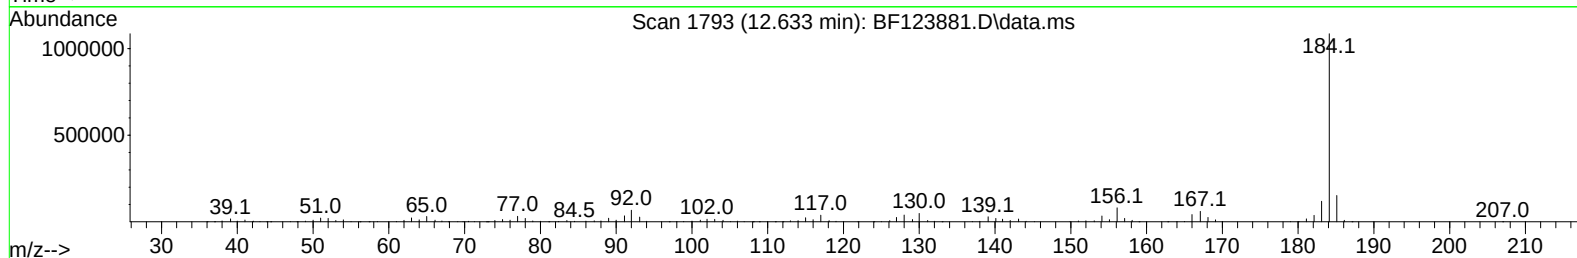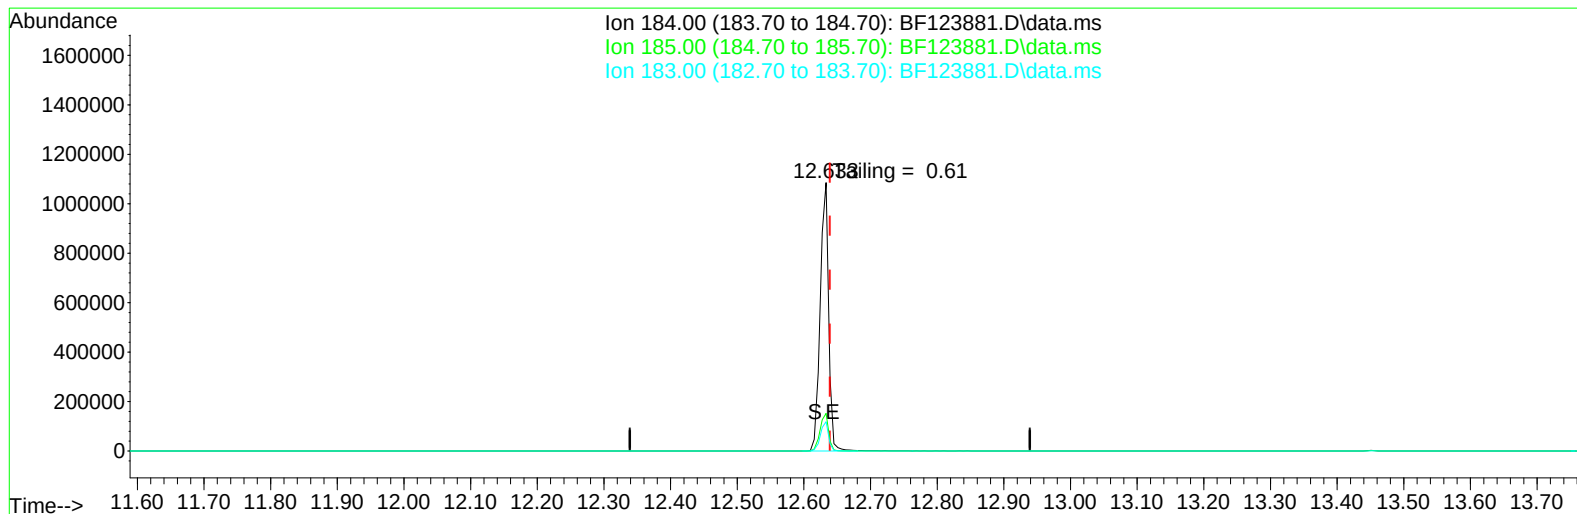

TIC: BF123881.D\data.ms

(77) Benzidine

12.633min (-0.006) 0.00 ng




response 955899

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.00
183.00	9.80	10.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051021\
Data File : BF123881.D
Acq On : 10 May 2021 11:13
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 10 12:16:07 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF042721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 07 13:43:24 2021
Response via : Initial Calibration

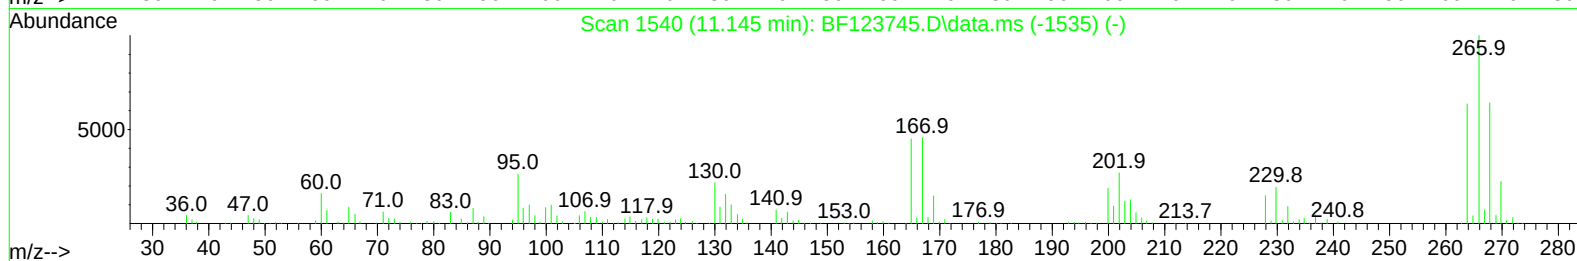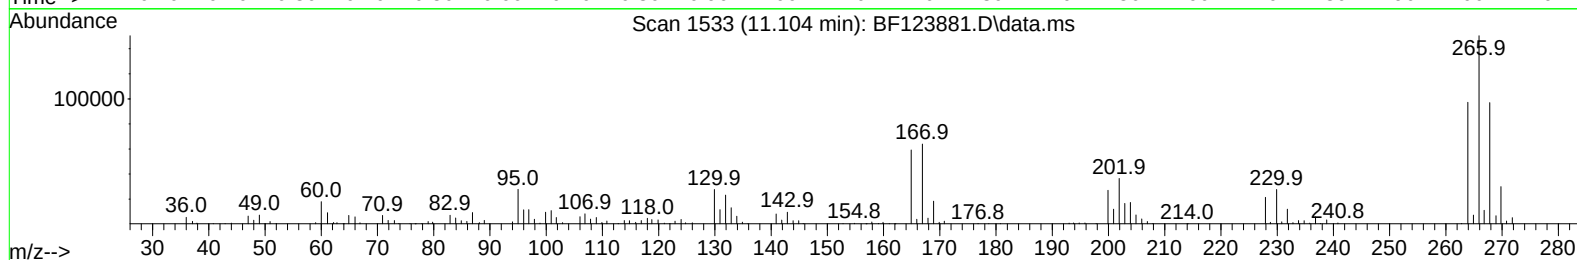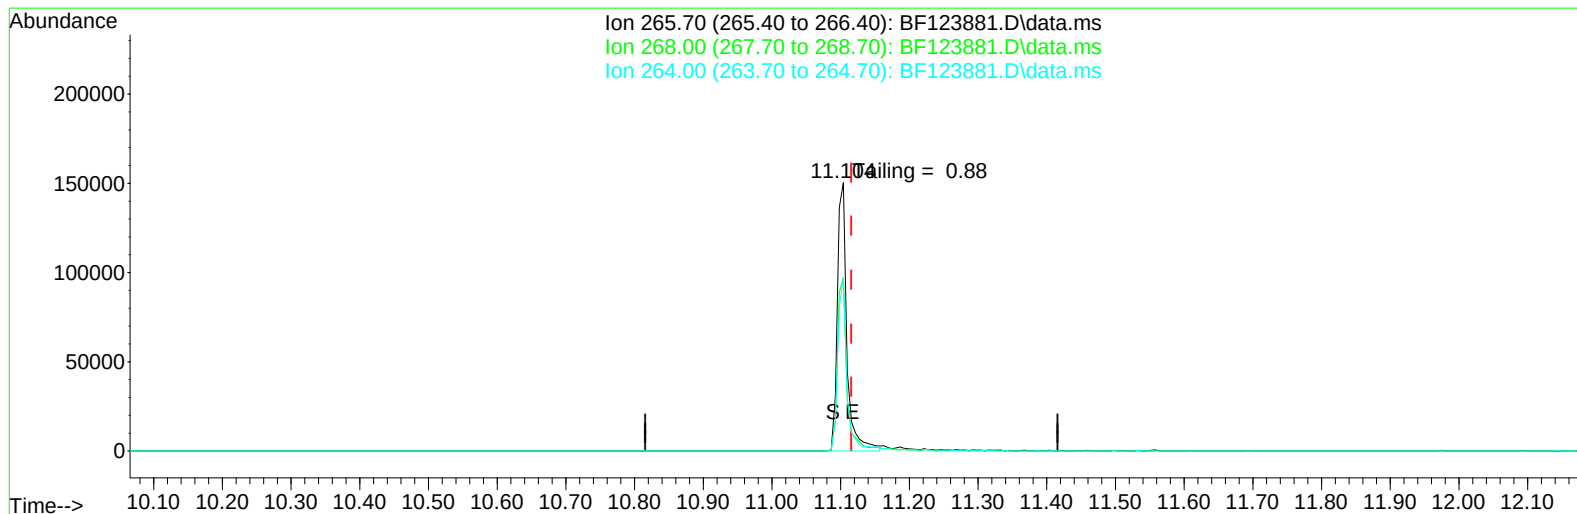

TIC: BF123881.D\data.ms

(70) Pentachlorophenol (C)

11.104min (-0.012) 30336.09 ng

response 148443

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.51
264.00	65.70	64.63
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/10/2021	BNA_F	<u>BF123881.D</u>
Compound Name	Response	Retention Time
DDT	436988	13.45
DDD	4080	13.15
DDE	1076	12.81
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5156	442144	1.17