
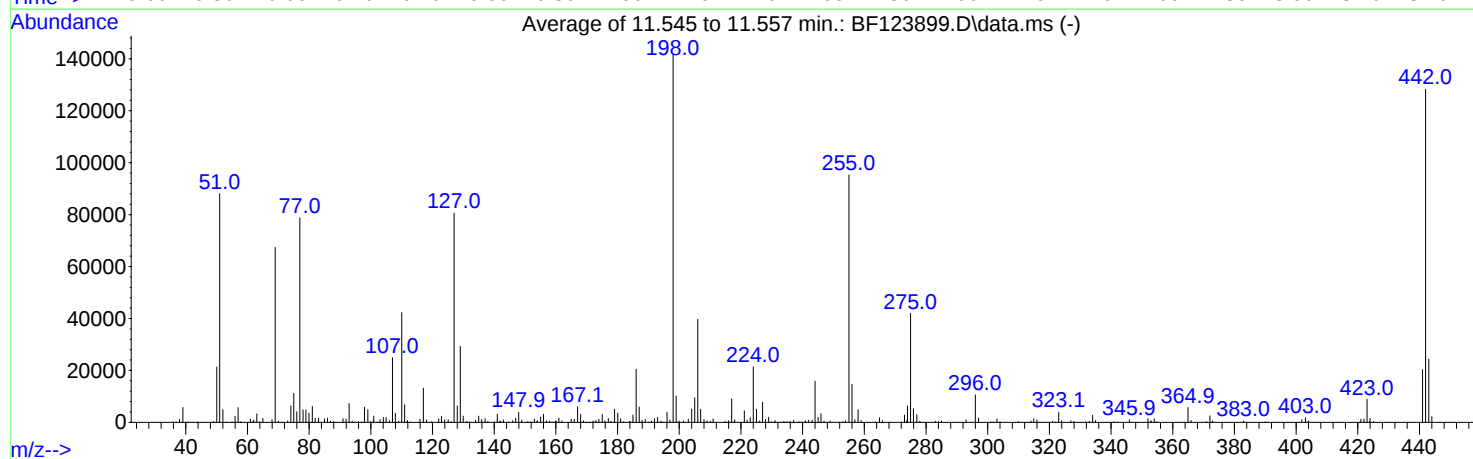


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051021\
 Data File : BF123899.D
 Acq On : 11 May 2021 00:13
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 10 16:46:01 2021

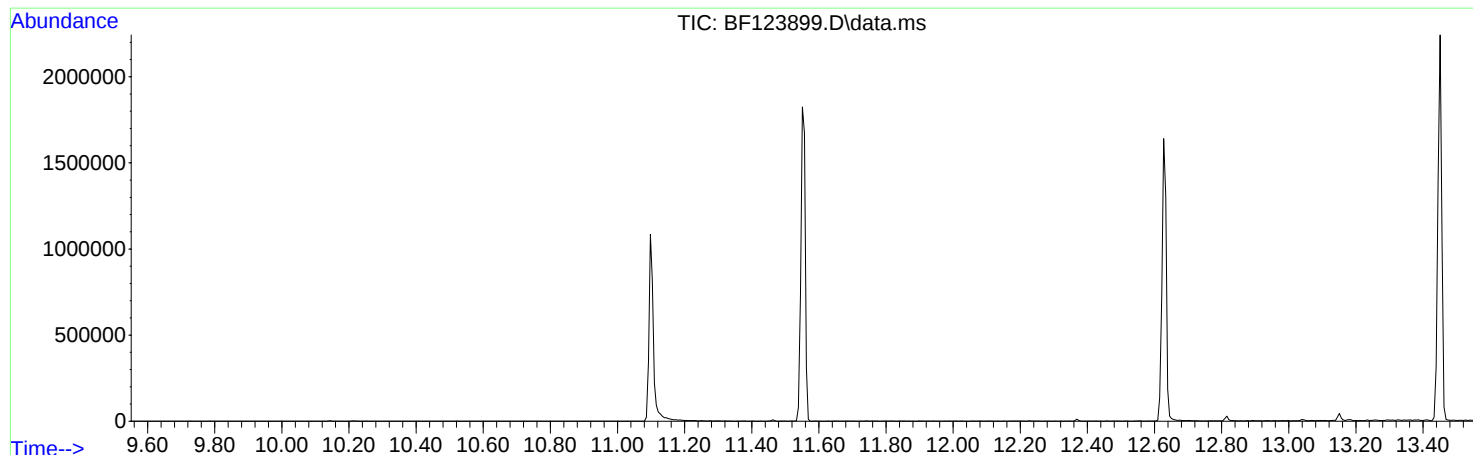




AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	62.2	88072	PASS
68	69	0.00	2	1.6	1052	PASS
69	198	0.00	100	47.6	67429	PASS
70	69	0.00	2	0.7	473	PASS
127	198	10	80	56.9	80584	PASS
197	198	0.00	2	0.6	855	PASS
198	198	100	100	100.0	141648	PASS
199	198	5	9	7.2	10144	PASS
275	198	10	60	29.6	41939	PASS
365	198	1	100	4.0	5718	PASS
441	198	0.01	100	14.4	20358	PASS
442	442	50	100	100.0	128221	PASS
443	442	15	24	19.0	24328	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051021\
 Data File : BF123899.D
 Acq On : 11 May 2021 00:13
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 11 05:34:15 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 10 16:46:01 2021
 Response via : Initial Calibration

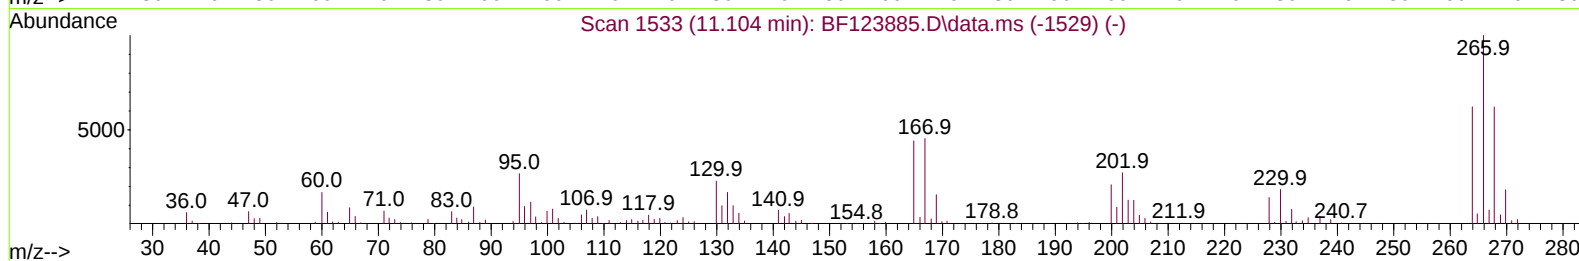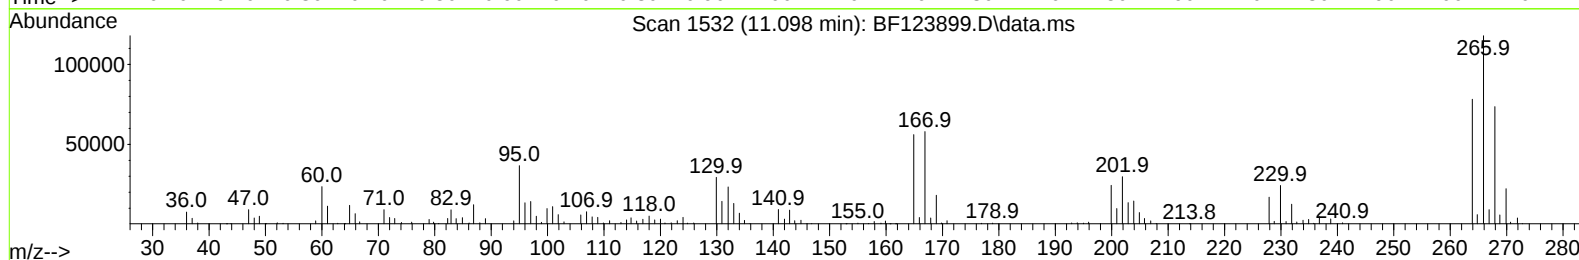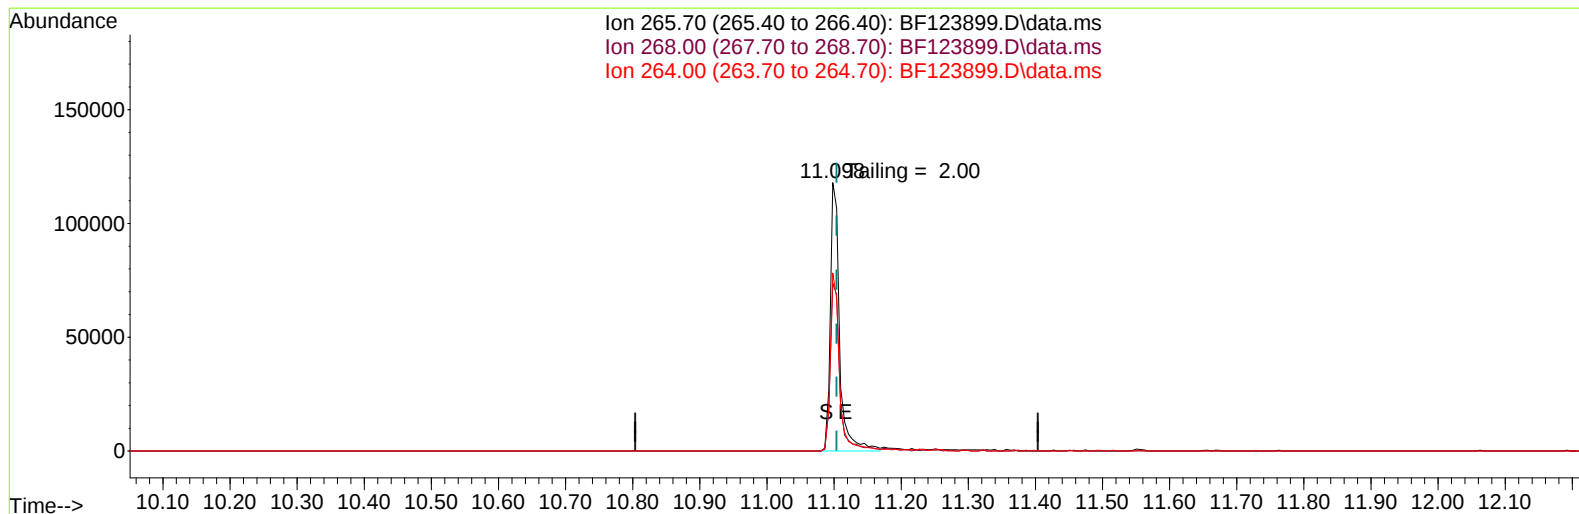

TIC: BF123899.D\data.ms

(70) Pentachlorophenol (C)

11.098min (-0.006) 27460.95 ng




response 116708

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	62.43
264.00	65.70	66.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051021\
Data File : BF123899.D
Acq On : 11 May 2021 00:13
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 11 05:34:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 10 16:46:01 2021
Response via : Initial Calibration

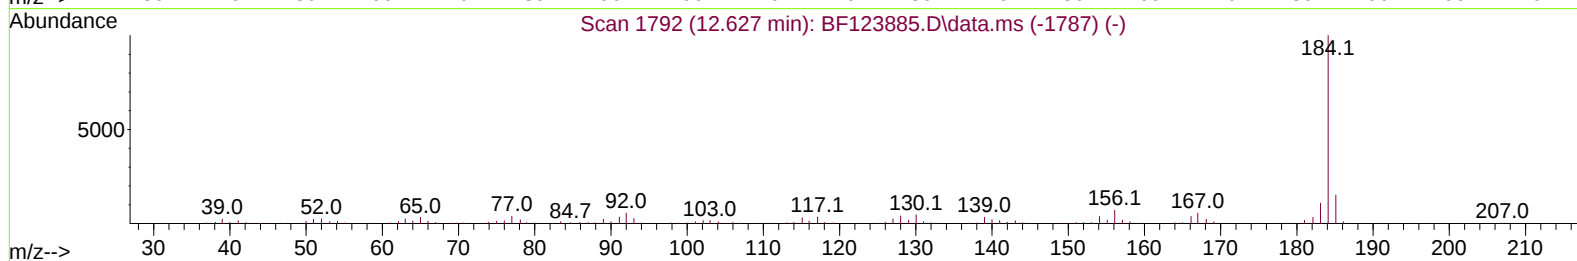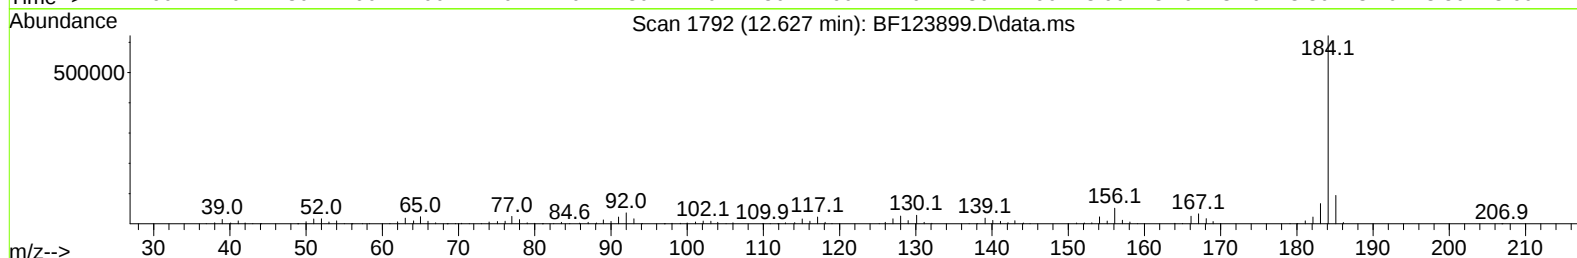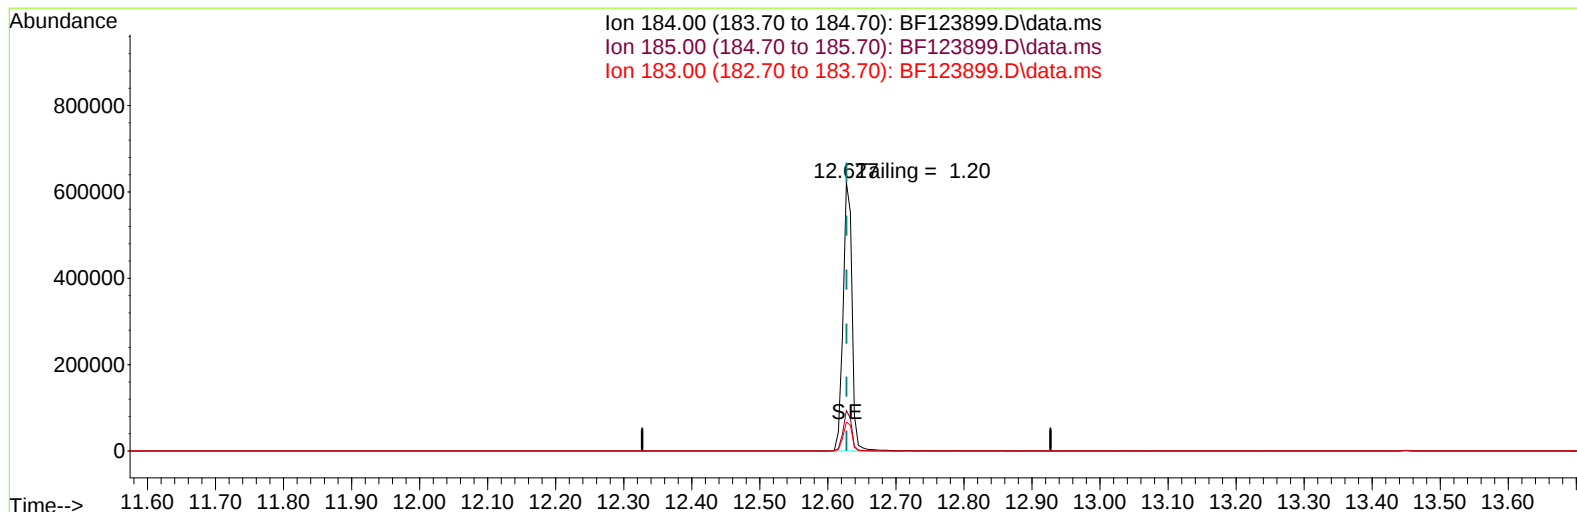

TIC: BF123899.D\data.ms

(77) Benzidine

12.627min (+ 0.000) 0.00 ng

response 567305

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	15.09
183.00	9.80	10.78
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/10/2021	BNA_F	<u>BF123899.D</u>
Compound Name	Response	Retention Time
DDT	331692	13.451
DDD	7789	13.151
DDE	2560	12.816
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10349	342041	3.03