

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051022\
 Data File : BF128161.D
 Acq On : 10 May 2022 15:32
 Operator : CG\JU
 Sample : PB144630BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB144630BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128161.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.528	546	551	554	rBV	2919215	3054697	76.45%	12.786%
2	6.522	714	720	723	rBV	2691148	3136163	78.49%	13.127%
3	6.892	779	783	786	rBV	693990	627718	15.71%	2.627%
4	7.457	873	879	882	rBV	1879331	2136220	53.46%	8.941%
5	8.175	996	1001	1004	rBV	838593	855858	21.42%	3.582%
6	9.251	1177	1184	1187	rBV	3485493	3768297	94.31%	15.773%
7	9.933	1294	1300	1303	rBV	1059944	985903	24.67%	4.127%
8	10.728	1428	1435	1438	rBV	2576955	2453105	61.39%	10.268%
9	11.422	1547	1553	1557	rBV	1161013	1037316	25.96%	4.342%
10	13.016	1818	1824	1827	rBV	4097068	3995685	100.00%	16.724%
11	14.068	1999	2003	2007	rBV	1043320	889316	22.26%	3.722%
12	15.563	2252	2257	2268	rVB	573207	749177	18.75%	3.136%
13	17.374	2552	2565	2581	rBV2	42012	201964	5.05%	0.845%




Sum of corrected areas: 23891419

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051022\
Data File : BF128161.D
Acq On : 10 May 2022 15:32
Operator : CG\JU
Sample : PB144630BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144630BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

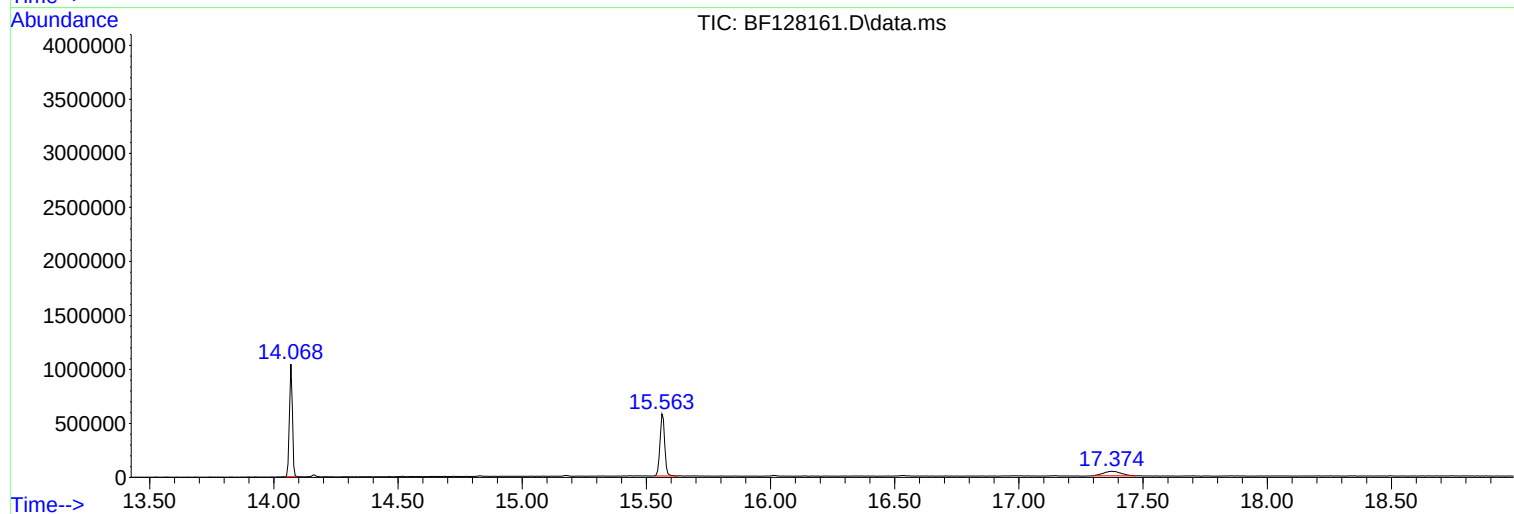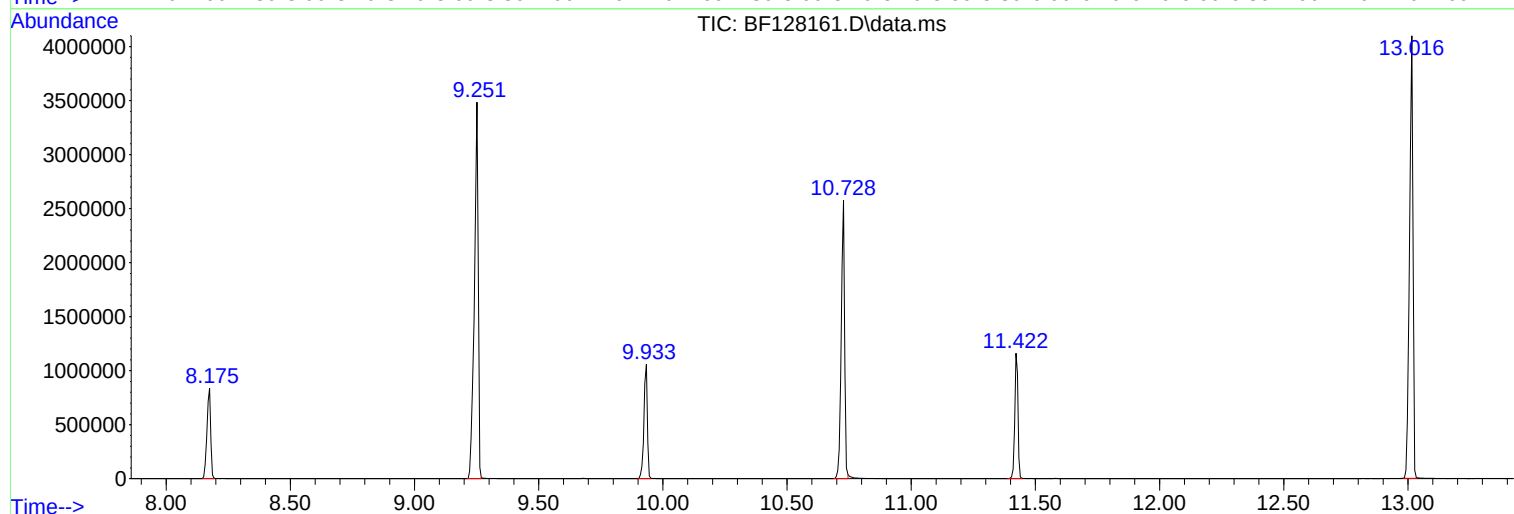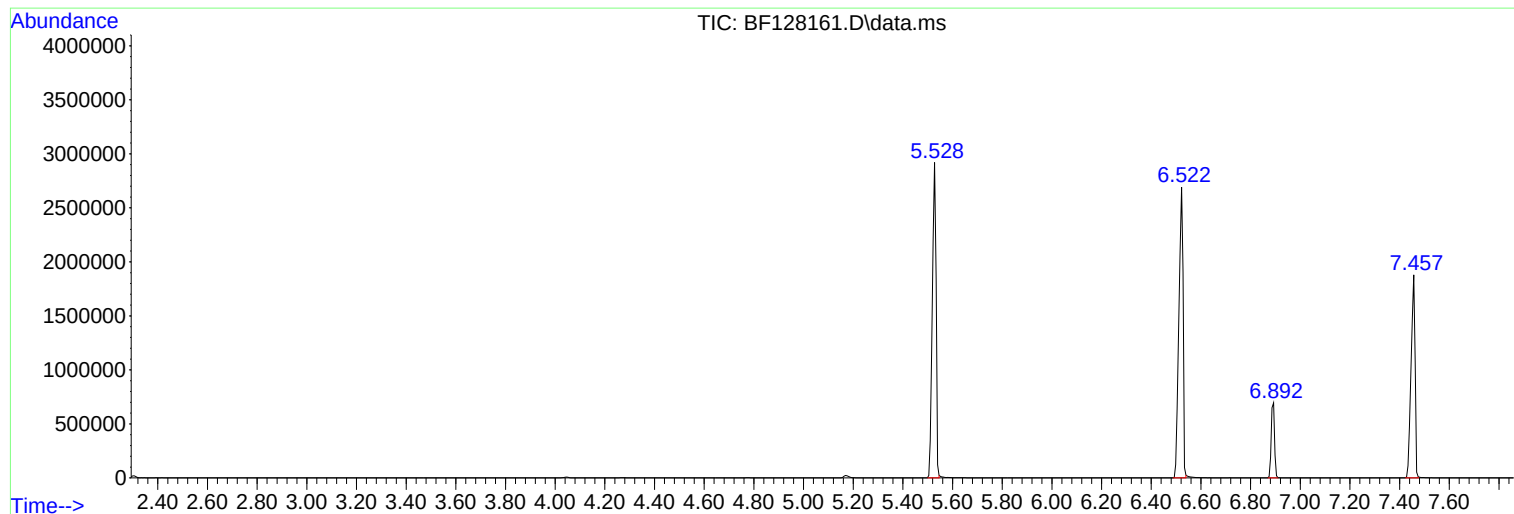

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051022\
Data File : BF128161.D
Acq On : 10 May 2022 15:32
Operator : CG\JU
Sample : PB144630BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144630BL









Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (1,1'-Biphenyl)-4,4'-diamin... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
17.374	5.39 ng	201964	Perylene-d12	15.563

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			(1,1'-Biphenyl)-4,4'-diamine, N,...	360	C26H20N2	006311-48-4	91
2			1,10-Phenanthroline, 2,9-dimethy...	360	C26H20N2	004733-39-5	47
3			Benzaldehyde, 4-hydroxy-3,5-dime...	360	C18H20N2O6	014414-32-5	47
4			N,N'-di-2-Naphthyl-p-phenylenedi...	360	C26H20N2	000093-46-9	46
5			1,3,2-Dioxaborolane, bis(spiro[4...	360	C20H13B06	1000150-23-7	43

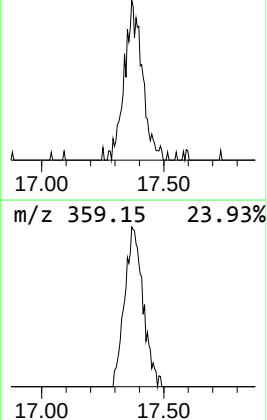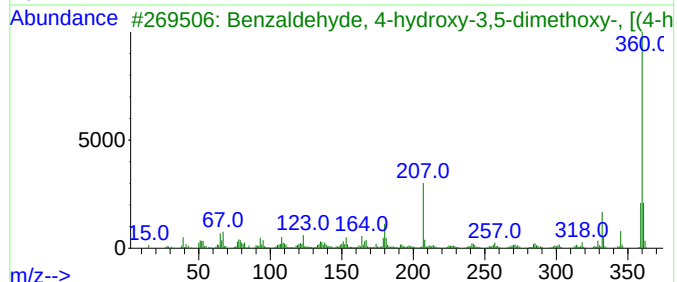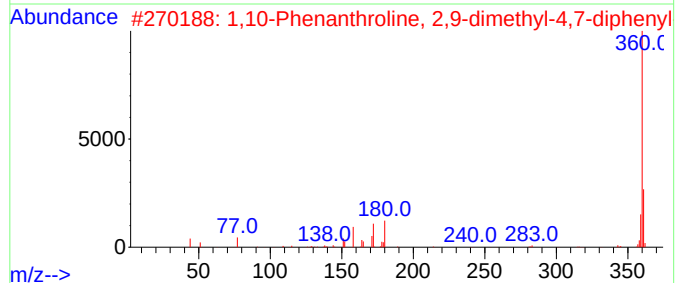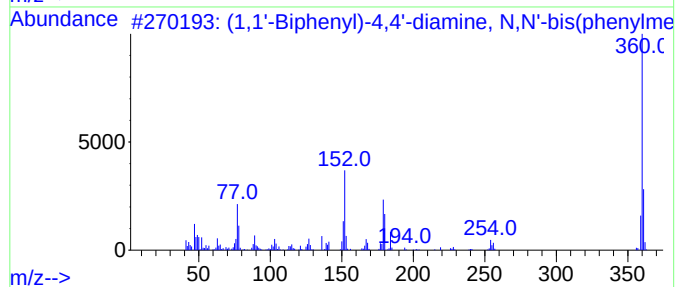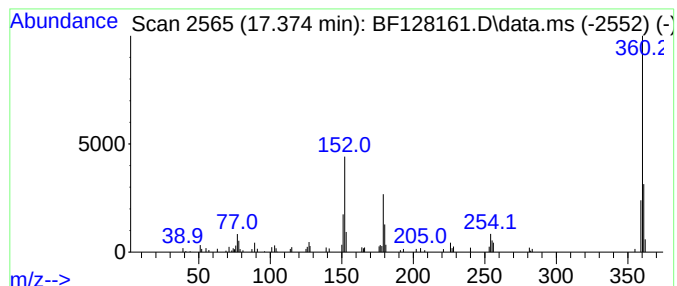

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051022\
Data File : BF128161.D
Acq On : 10 May 2022 15:32
Operator : CG\JU
Sample : PB144630BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144630BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(1,1'-Biphenyl)...	17.374	5.4	ng	201964	6	15.563	749177	20.0