


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051022\
 Data File : BF128155.D
 Acq On : 10 May 2022 09:55
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 09 15:30:11 2022

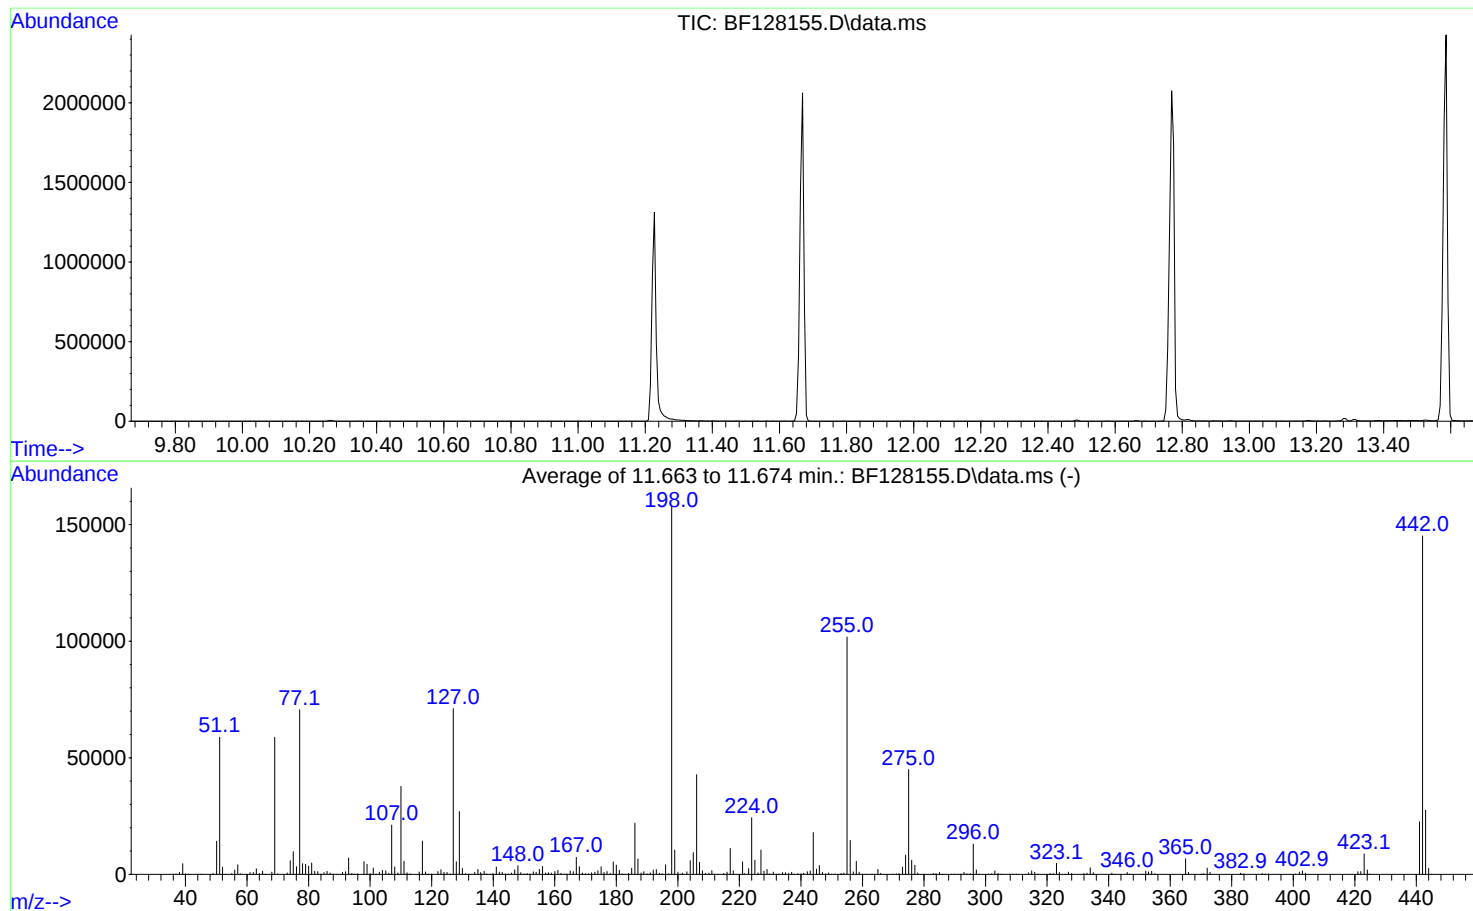




AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	58806	PASS
68	69	0.00	2	1.6	943	PASS
69	198	0.00	100	37.3	58837	PASS
70	69	0.00	2	0.5	306	PASS
127	198	10	80	45.1	71123	PASS
197	198	0.00	2	0.2	245	PASS
198	198	100	100	100.0	157795	PASS
199	198	5	9	6.6	10432	PASS
275	198	10	60	28.5	44960	PASS
365	198	1	100	4.2	6657	PASS
441	198	0.01	100	14.3	22567	PASS
442	442	50	100	100.0	145195	PASS
443	442	15	24	19.0	27547	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051022\
Data File : BF128155.D
Acq On : 10 May 2022 09:55
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 11 07:18:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 09 15:30:11 2022
Response via : Initial Calibration

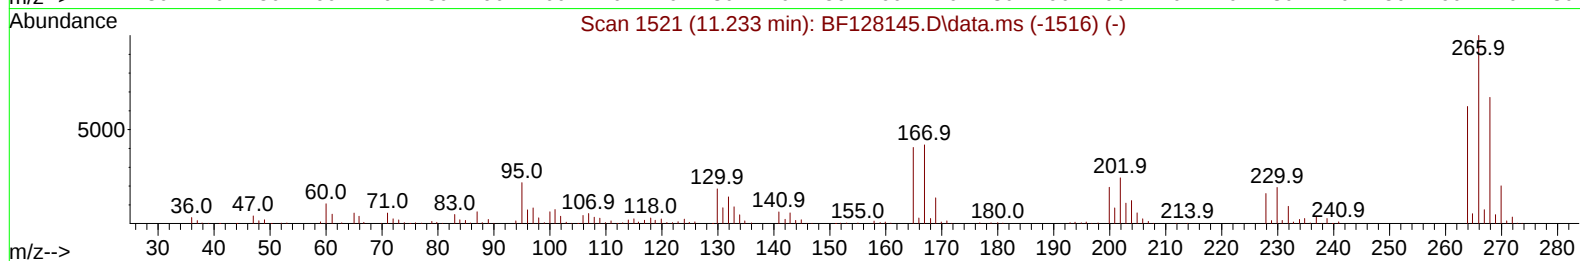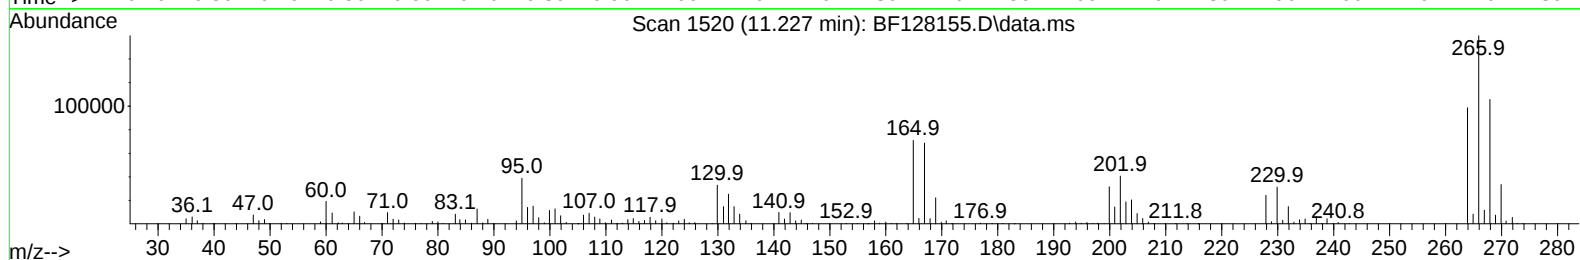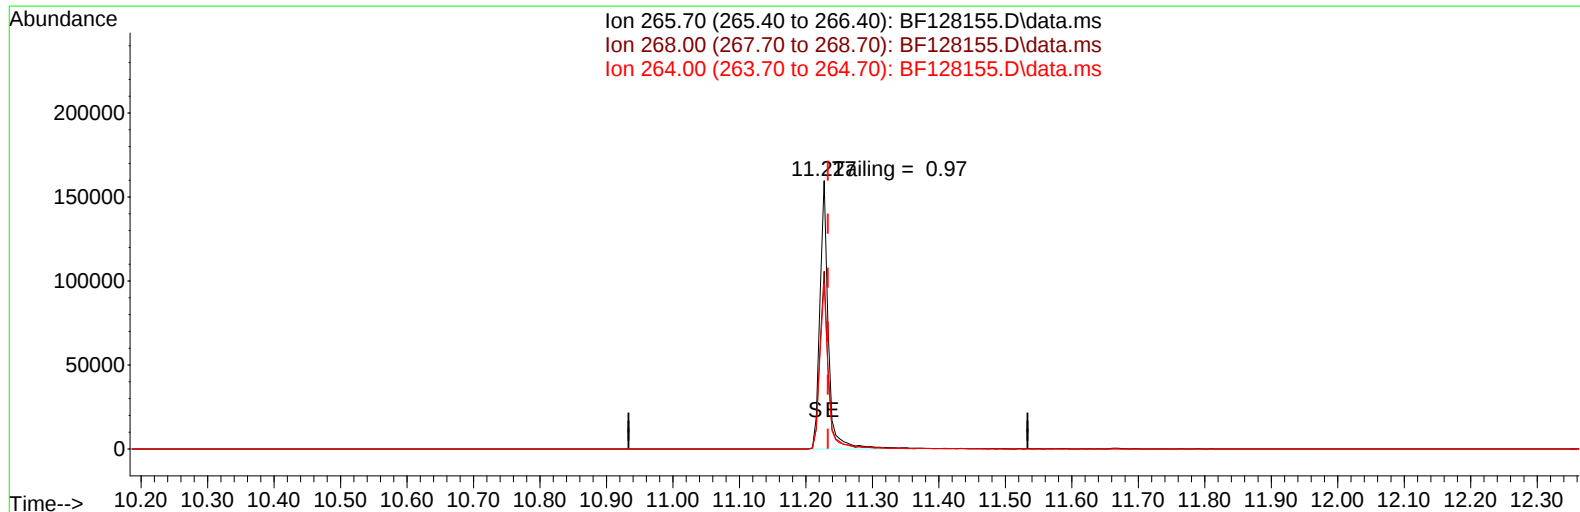

TIC: BF128155.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.006) 37773.38 ng




response 143257

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	66.19
264.00	66.40	61.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051022\
Data File : BF128155.D
Acq On : 10 May 2022 09:55
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 11 07:18:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 09 15:30:11 2022
Response via : Initial Calibration

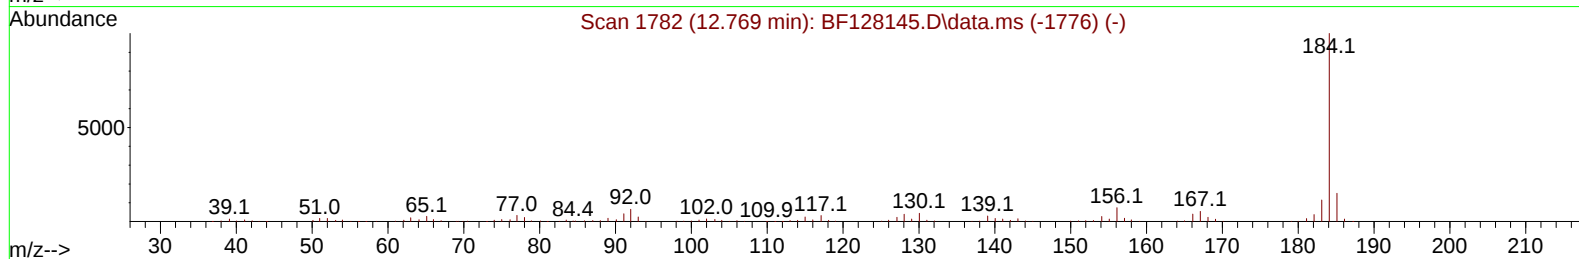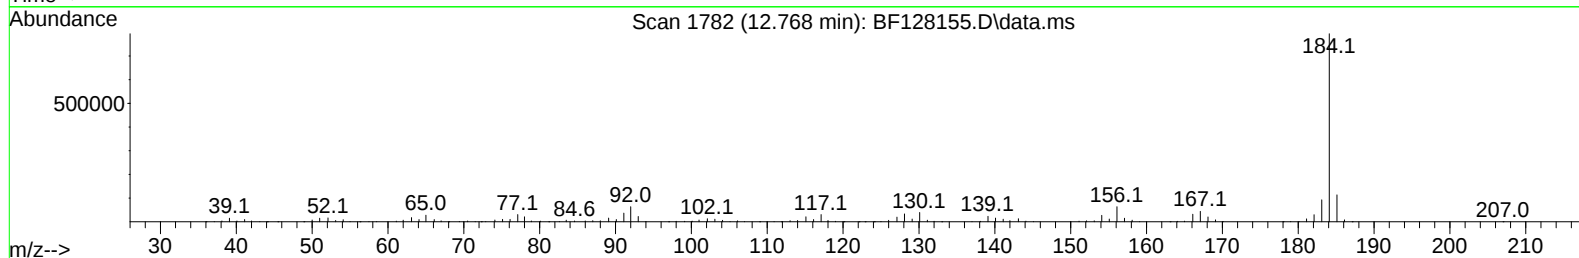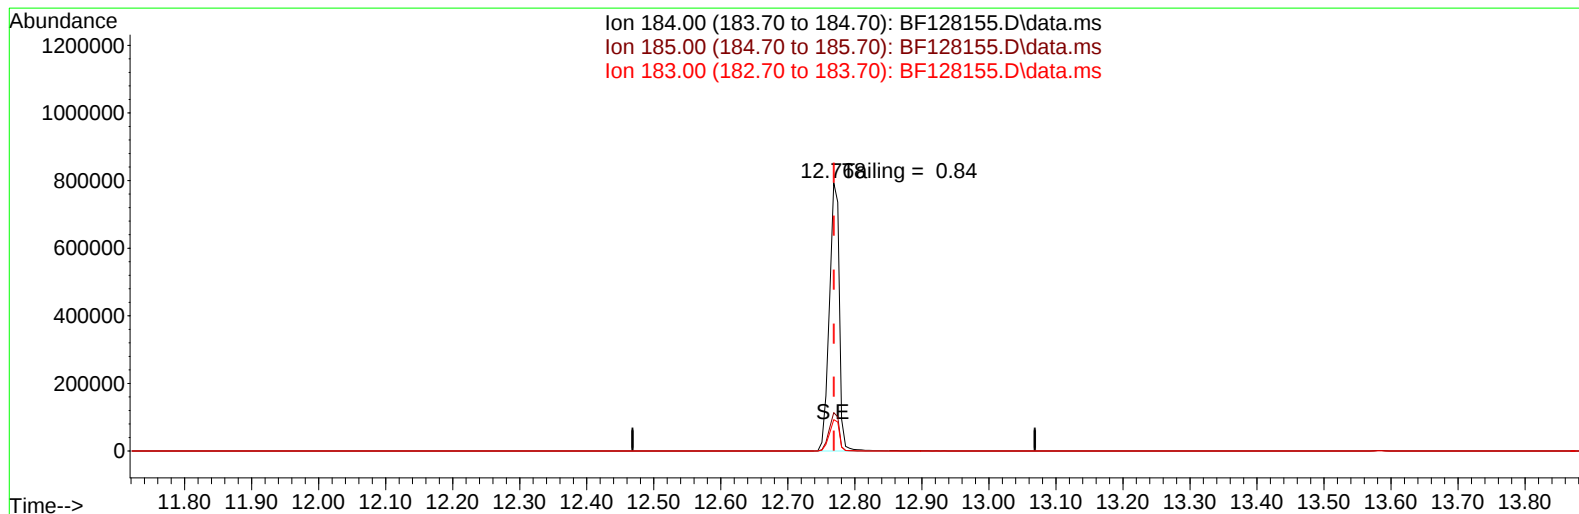

TIC: BF128155.D\data.ms

(77) Benzidine

12.768min (-0.000) 687469.86 ng

response 818919

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.30
183.00	11.20	11.70
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/10/2022	BNA_F	<u>BF128155.D</u>
Compound Name	Response	Retention Time
DDT	410048	13.586
DDD	5515	13.286
DDE	584	12.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6099	416147	1.47

Instrument :
BNA_F
ClientSampleId :
DFTPP