


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051022\
 Data File : BF128159.D
 Acq On : 10 May 2022 14:34
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 09 15:30:11 2022

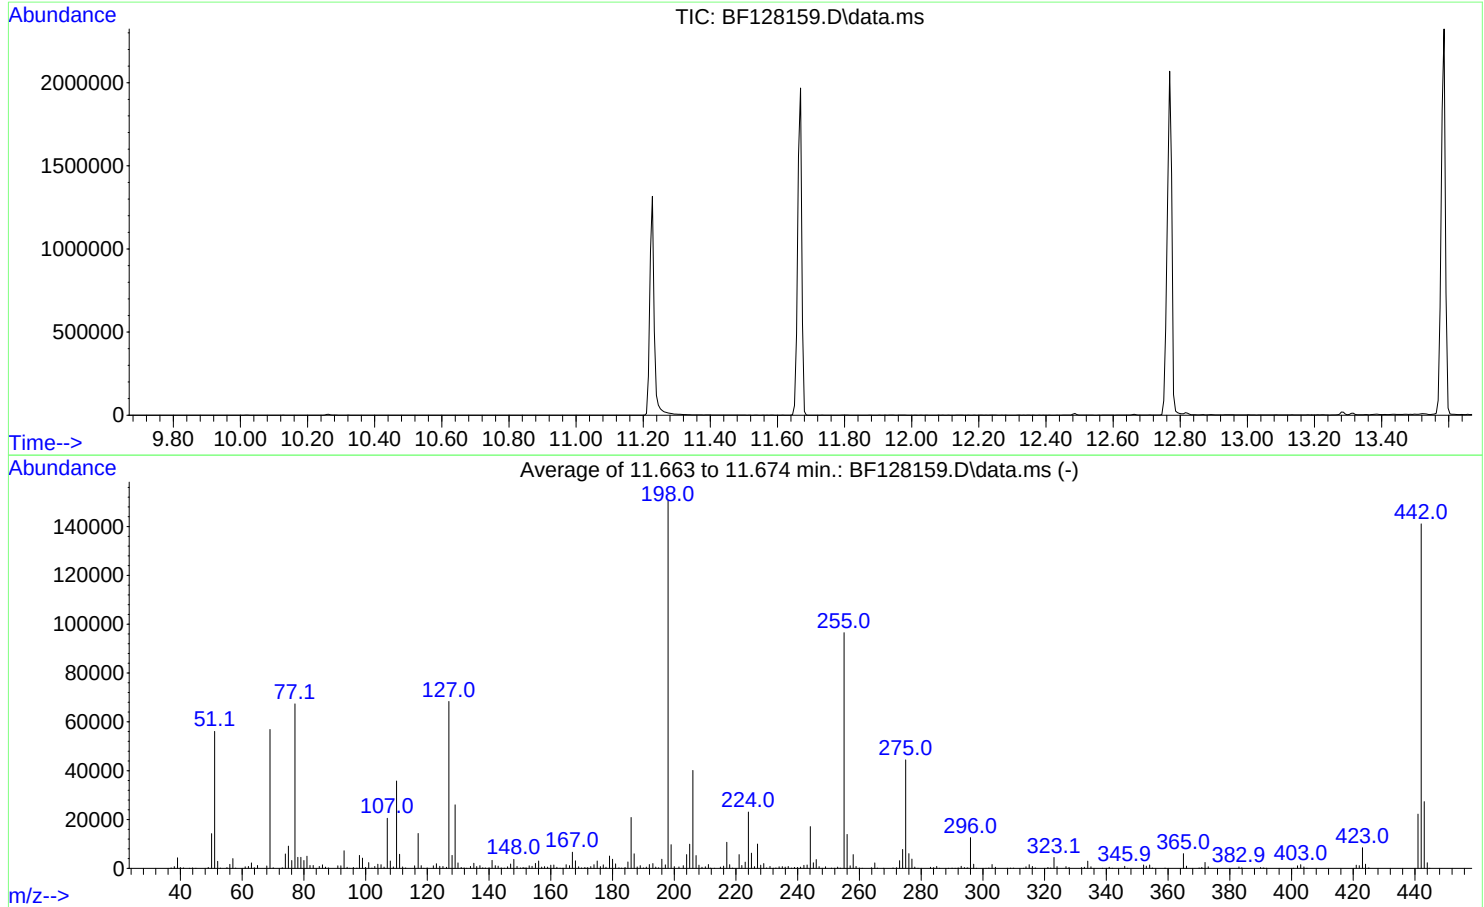




AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	56112	PASS
68	69	0.00	2	1.8	1002	PASS
69	198	0.00	100	37.8	56915	PASS
70	69	0.00	2	0.5	294	PASS
127	198	10	80	45.4	68371	PASS
197	198	0.00	2	1.0	1454	PASS
198	198	100	100	100.0	150651	PASS
199	198	5	9	6.4	9688	PASS
275	198	10	60	29.5	44413	PASS
365	198	1	100	4.0	6055	PASS
441	198	0.01	100	14.8	22250	PASS
442	442	50	100	100.0	141061	PASS
443	442	15	24	19.4	27352	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051022\
Data File : BF128159.D
Acq On : 10 May 2022 14:34
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 11 07:21:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 09 15:30:11 2022
Response via : Initial Calibration

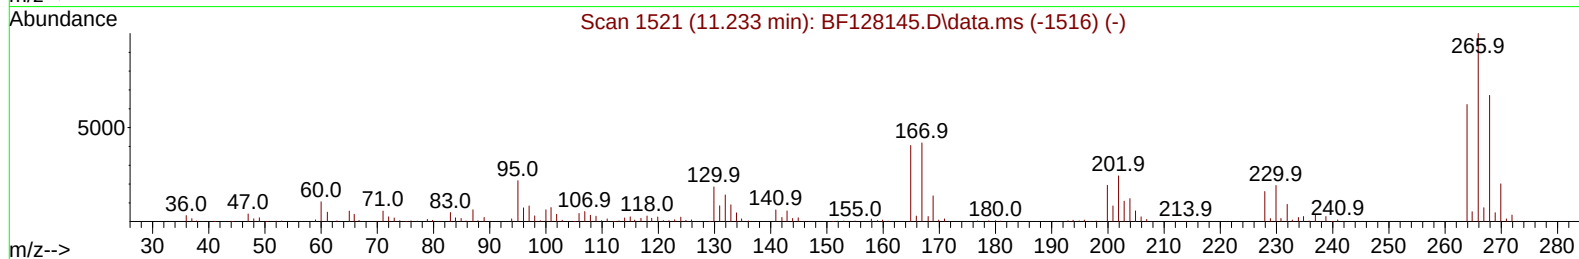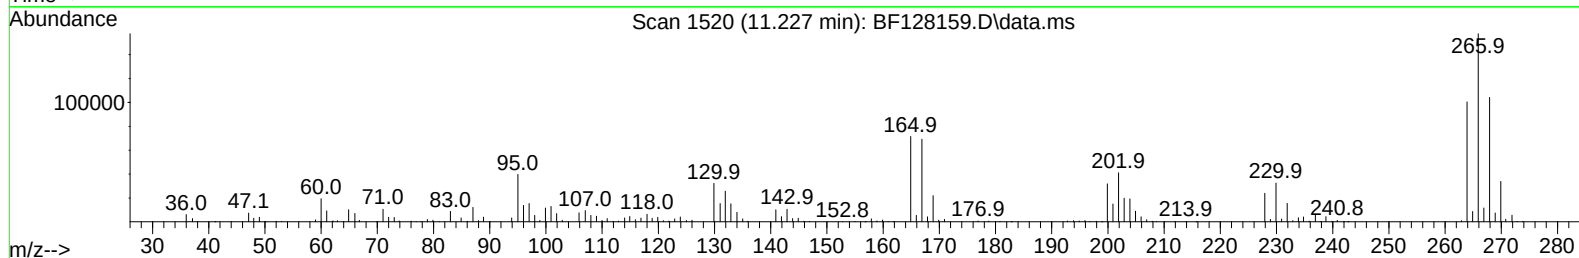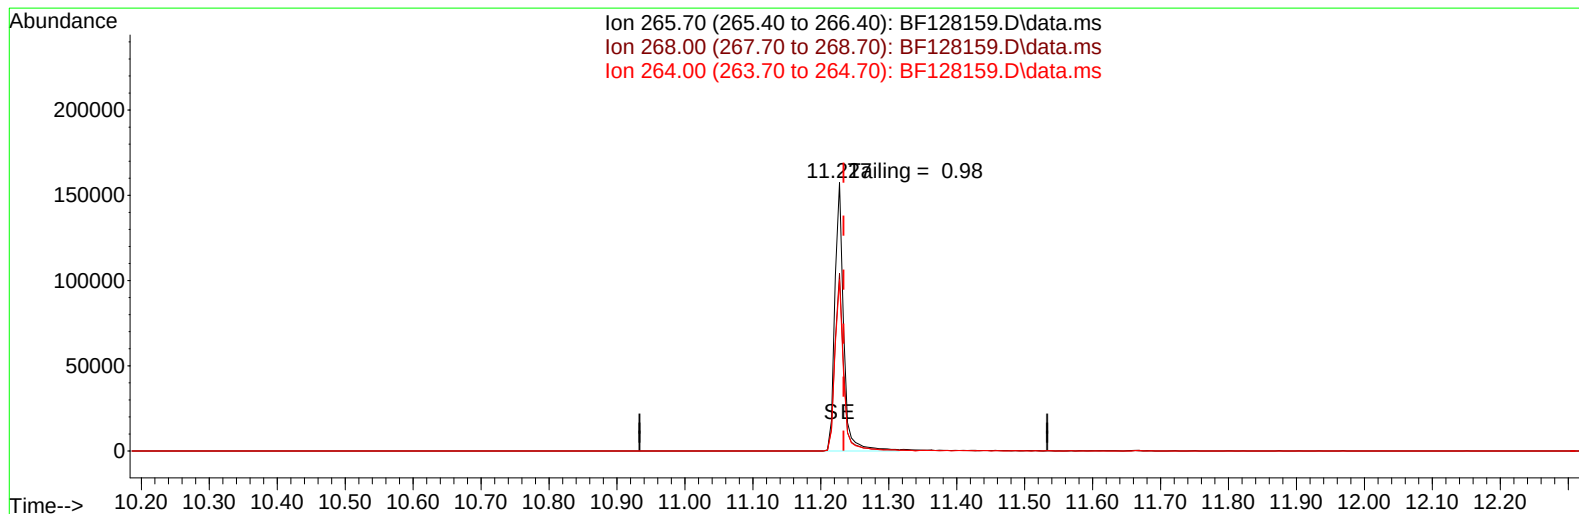

TIC: BF128159.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.006) 32096.30 ng




response 141342

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	66.13
264.00	66.40	63.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051022\
Data File : BF128159.D
Acq On : 10 May 2022 14:34
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 11 07:21:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 09 15:30:11 2022
Response via : Initial Calibration

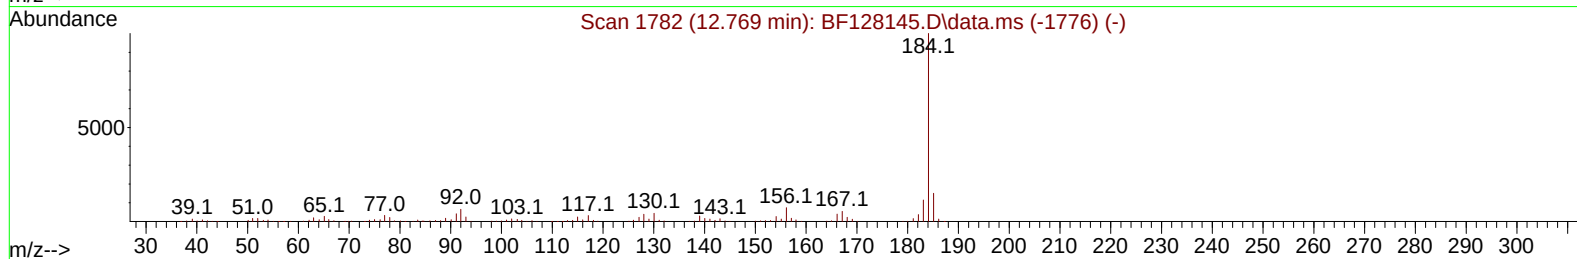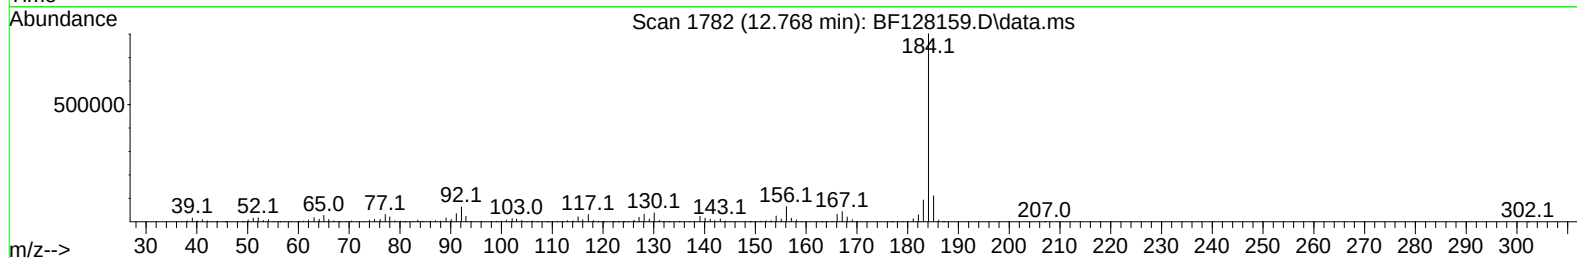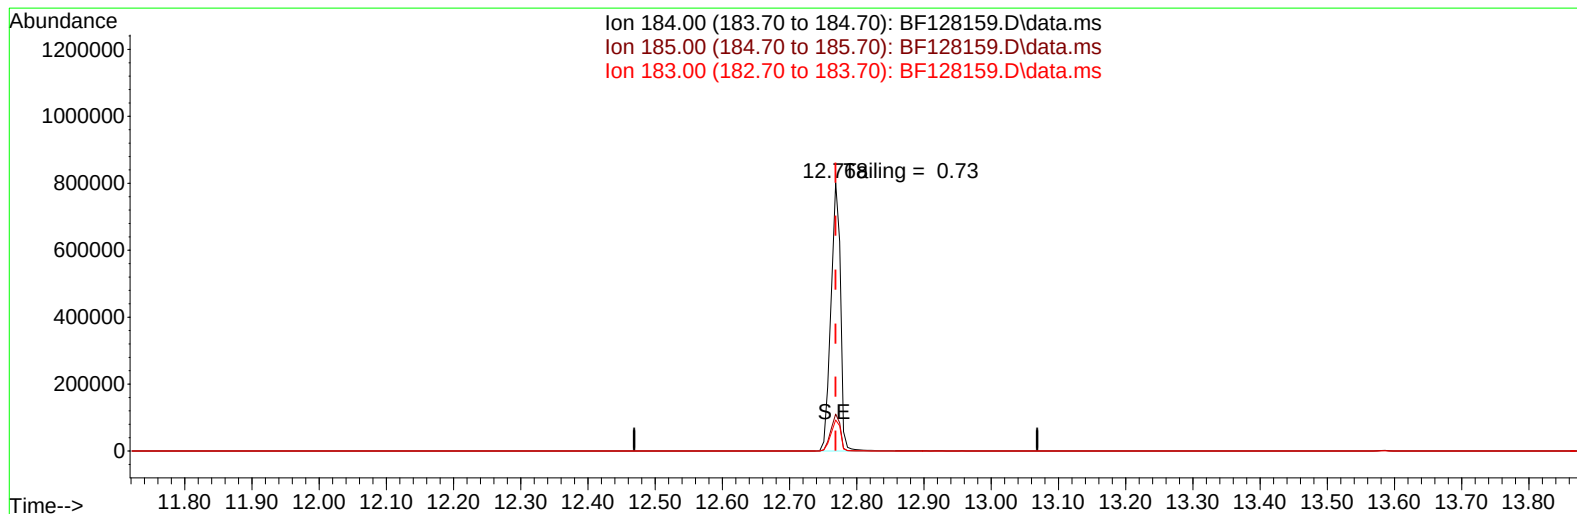

TIC: BF128159.D\data.ms

(77) Benzidine

12.768min (-0.000) 0.00 ng

response 790329

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.82
183.00	11.20	11.61
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/10/2022	BNA_F	<u>BF128159.D</u>
Compound Name	Response	Retention Time
DDT	390715	13.586
DDD	5716	13.28
DDE	401	12.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6117	396832	1.54

Instrument :
BNA_F
ClientSampleId :
DFTPP