
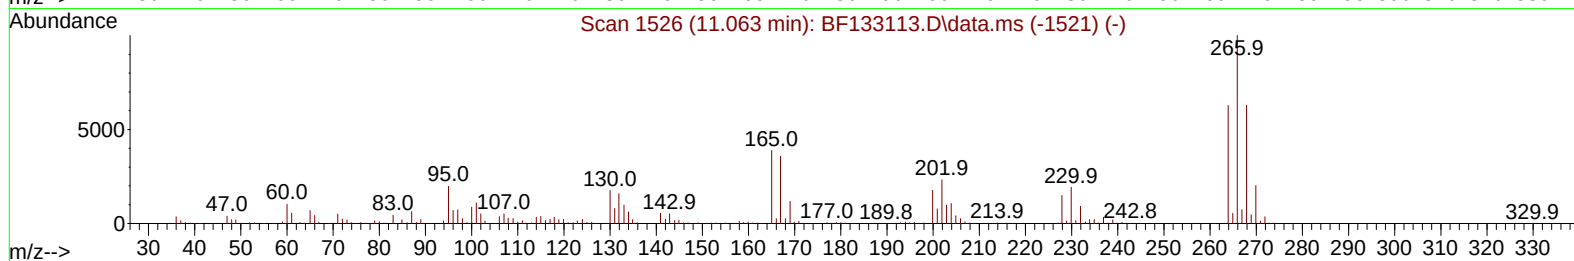
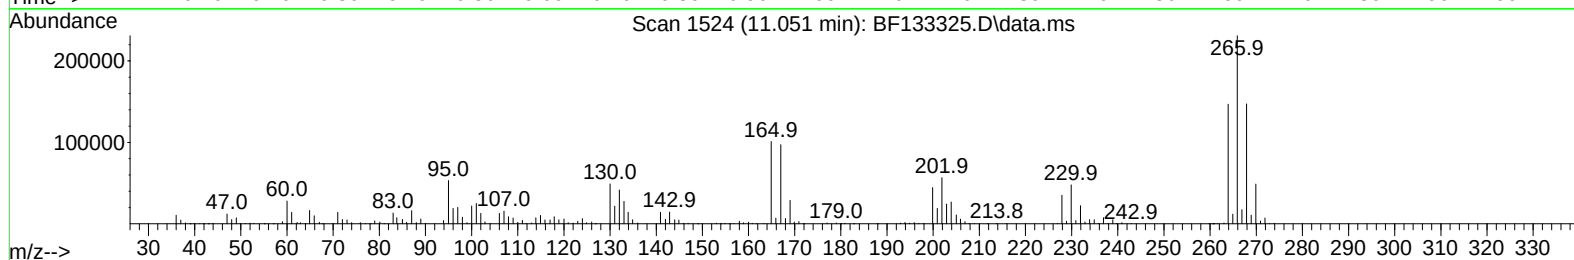


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051023\
Data File : BF133325.D
Acq On : 10 May 2023 12:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 10 14:20:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 09 04:59:36 2023
Response via : Initial Calibration

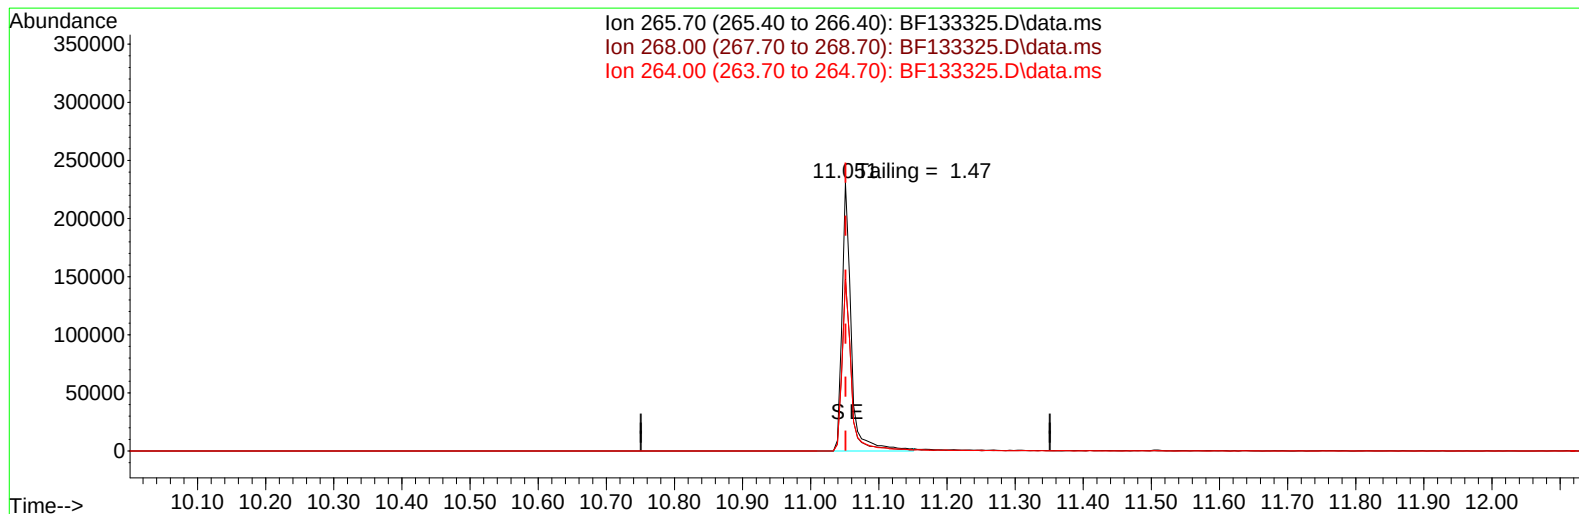

TIC: BF133325.D\data.ms

(70) Pentachlorophenol (C)




11.051min (+ 0.000) 152184.48 ng

response 211995

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	63.80
264.00	63.30	63.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051023\
 Data File : BF133325.D
 Acq On : 10 May 2023 12:14
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 10 14:20:55 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 09 04:59:36 2023
 Response via : Initial Calibration

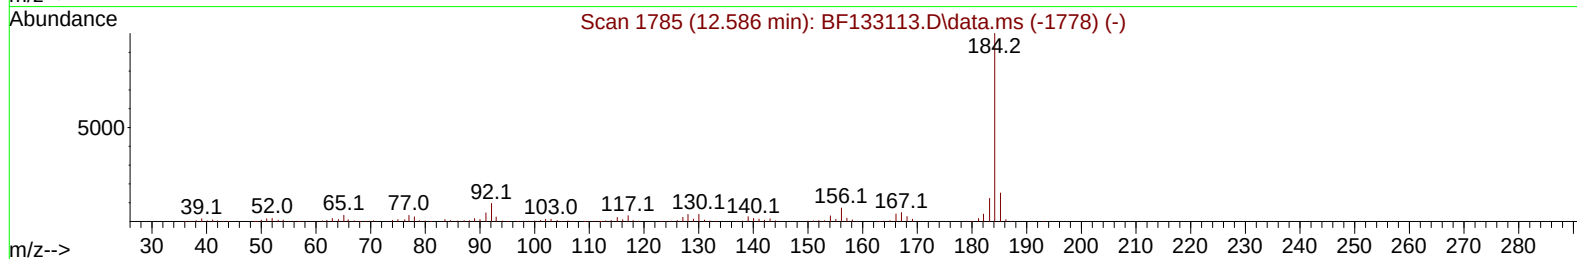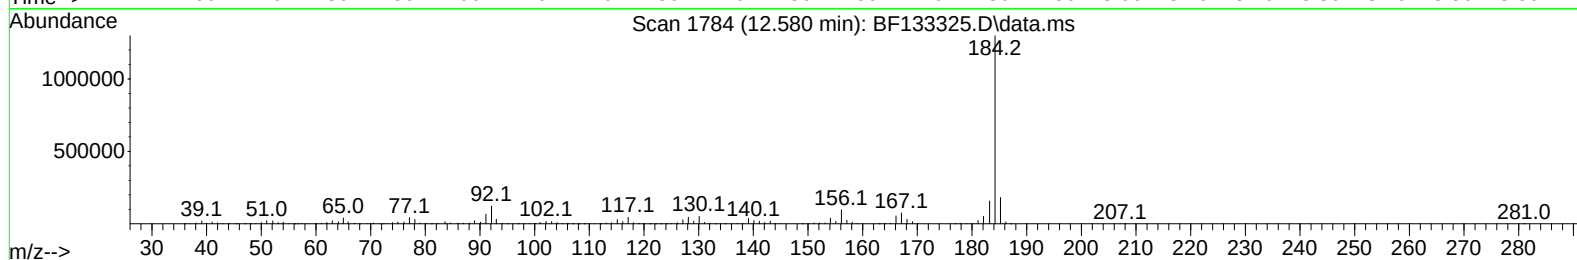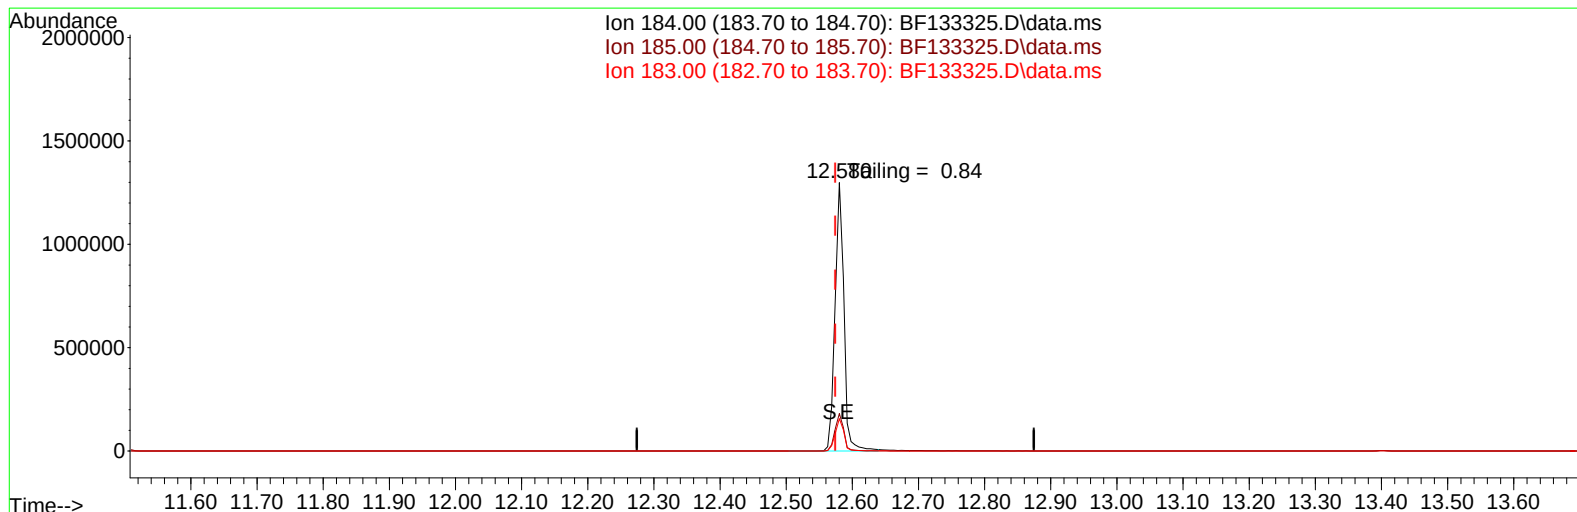

TIC: BF133325.D\data.ms

(77) Benzidine

12.580min (+ 0.006) 8167.51 ng m

response 1224130

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	13.97#
183.00	11.70	12.09
0.00	0.00	0.00