
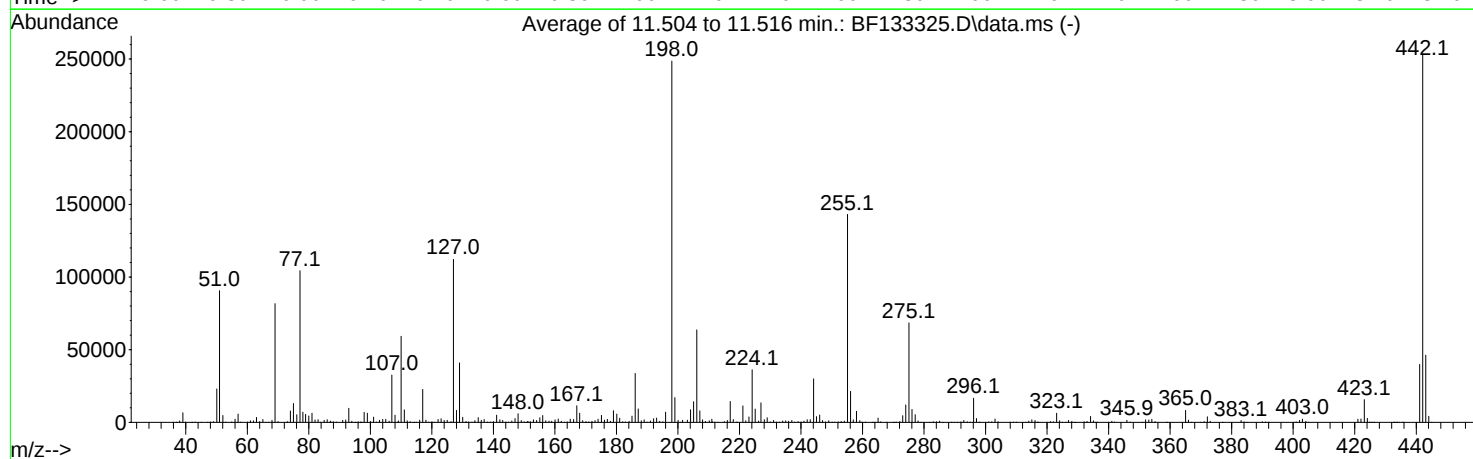


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051023\
 Data File : BF133325.D
 Acq On : 10 May 2023 12:14
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 09 04:59:36 2023

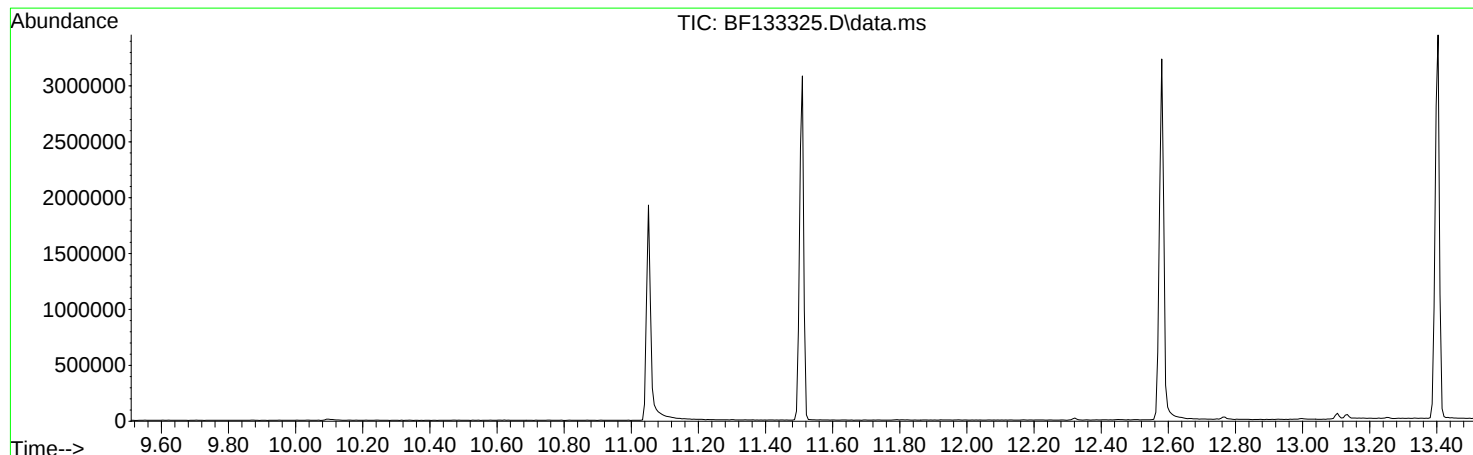

AutoFind: Scans 1601, 1602, 1603; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	90577	PASS
68	69	0.00	2	1.8	1468	PASS
69	198	0.00	100	32.9	81757	PASS
70	69	0.00	2	0.6	527	PASS
127	198	10	80	45.1	112216	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	248621	PASS
199	198	5	9	6.9	17068	PASS
275	198	10	60	27.5	68464	PASS
365	198	1	100	3.3	8302	PASS
441	198	0.01	100	16.0	39819	PASS
442	442	50	100	100.0	253141	PASS
443	442	15	24	18.3	46288	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/10/2023	BNA_F	<u>BF133325.D</u>
Compound Name	Response	Retention Time
DDT	595936	13.404
DDD	15466	13.104
DDE	2906	12.769
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18372	614308	2.99

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051023\
Data File : BF133325.D
Acq On : 10 May 2023 12:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 10 14:20:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 09 04:59:36 2023
Response via : Initial Calibration

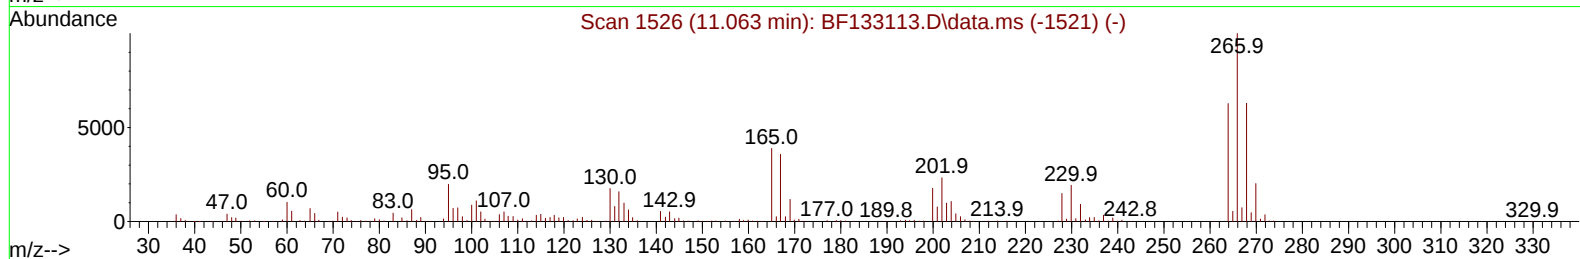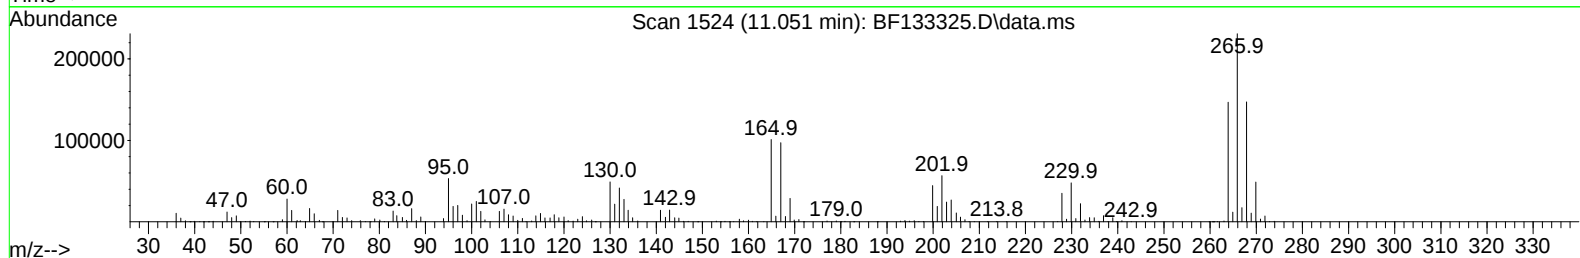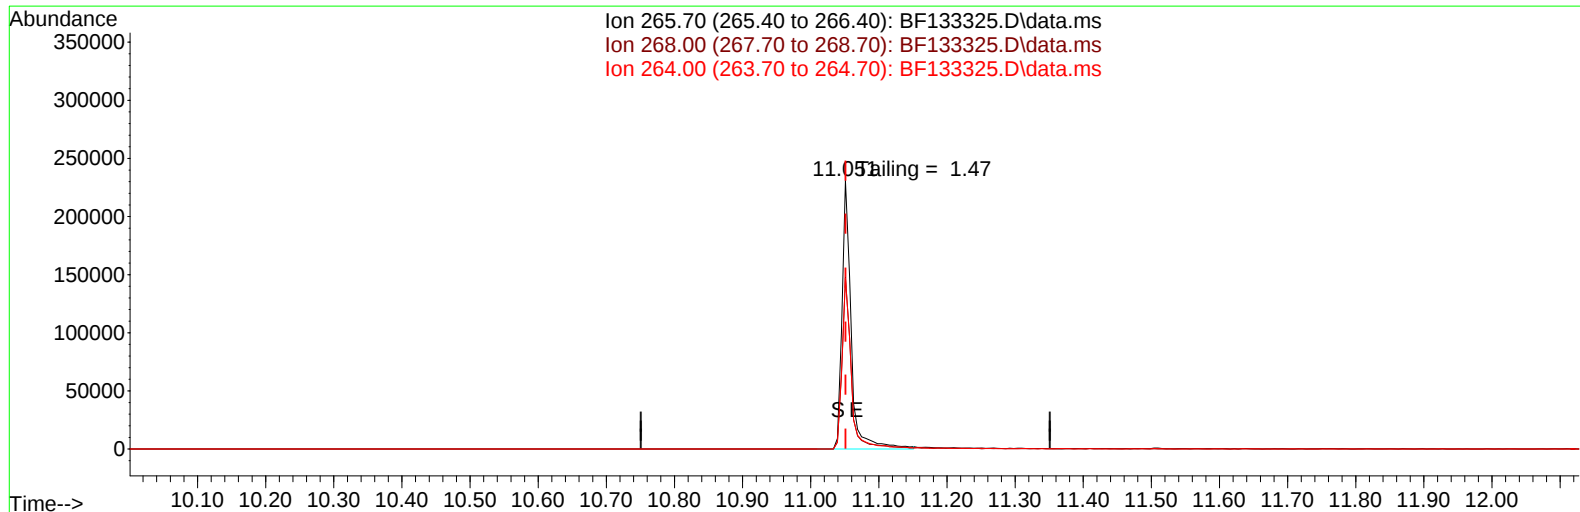

TIC: BF133325.D\data.ms

(70) Pentachlorophenol (C)

11.051min (+ 0.000) 152184.48 ng




response 211995

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	63.80
264.00	63.30	63.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051023\
Data File : BF133325.D
Acq On : 10 May 2023 12:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 10 14:20:55 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 09 04:59:36 2023
Response via : Initial Calibration

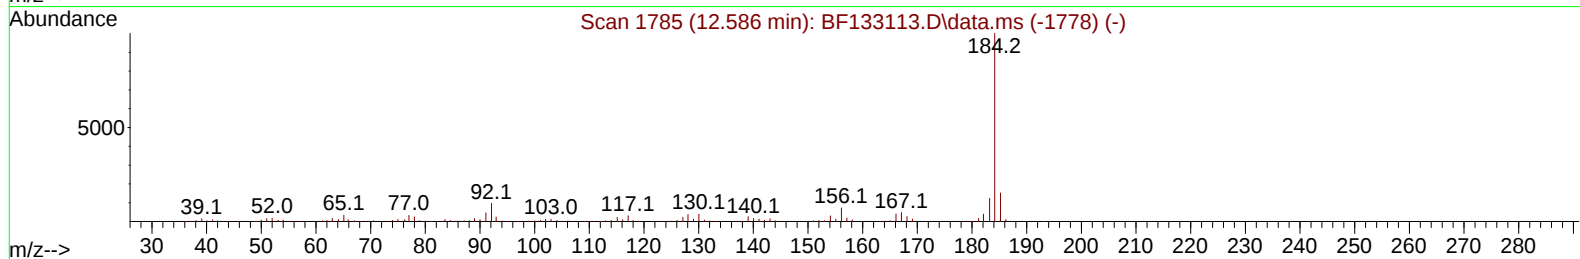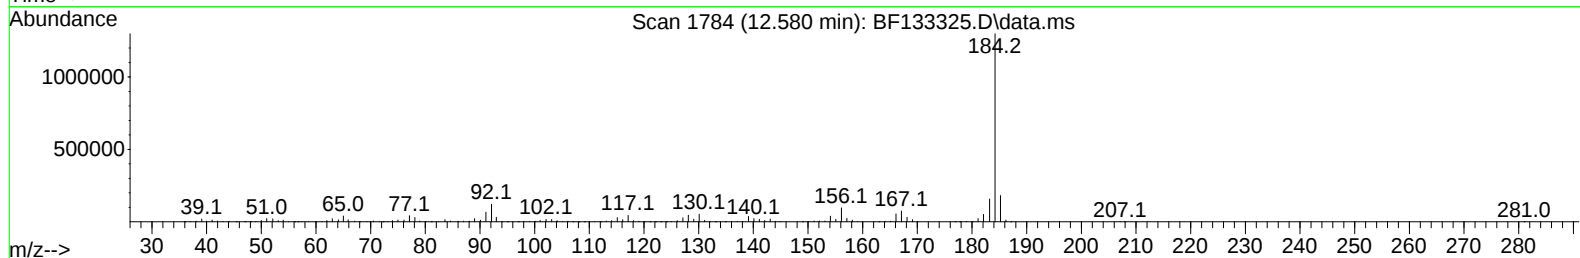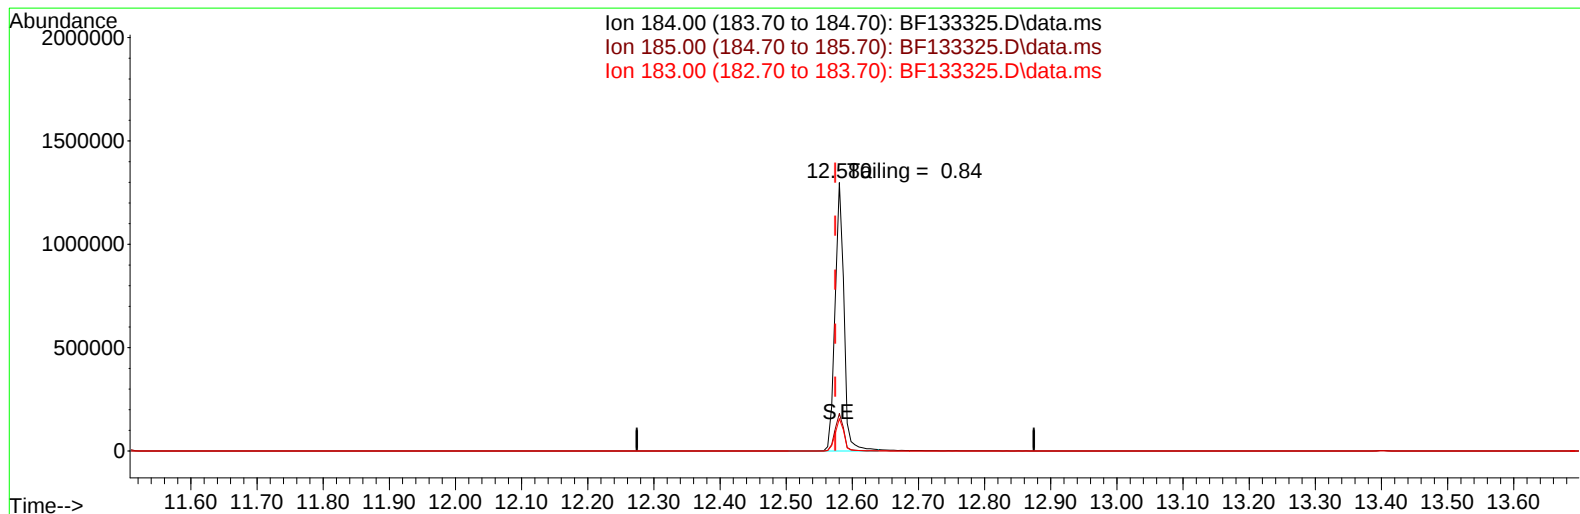

TIC: BF133325.D\data.ms

(77) Benzidine

12.580min (+ 0.006) 8167.51 ng m

response 1224130

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	13.97#
183.00	11.70	12.09
0.00	0.00	0.00