
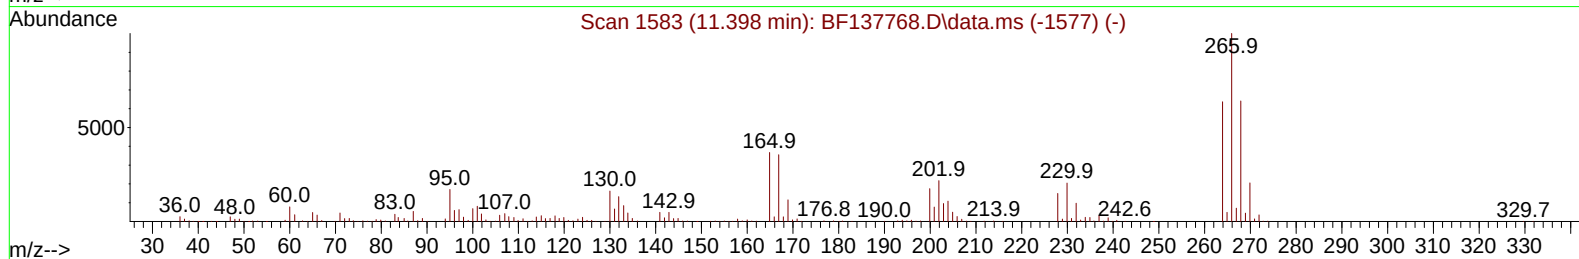
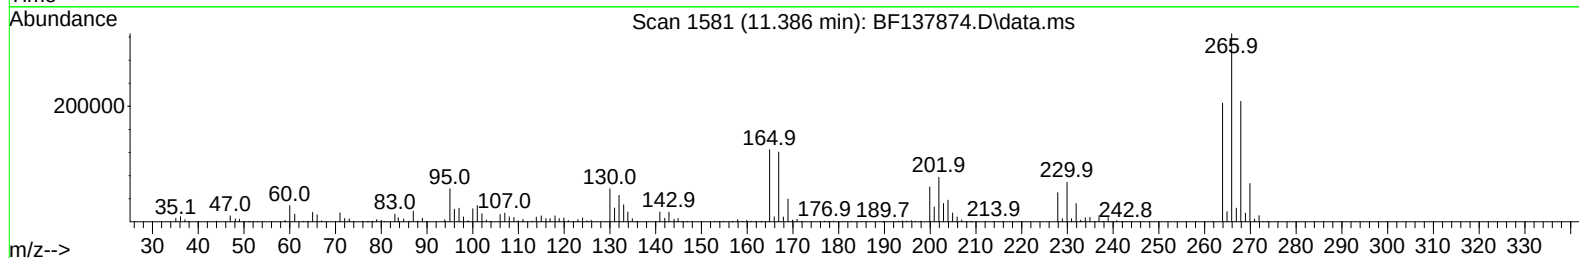


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051024\
Data File : BF137874.D
Acq On : 10 May 2024 11:34
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 00:29:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

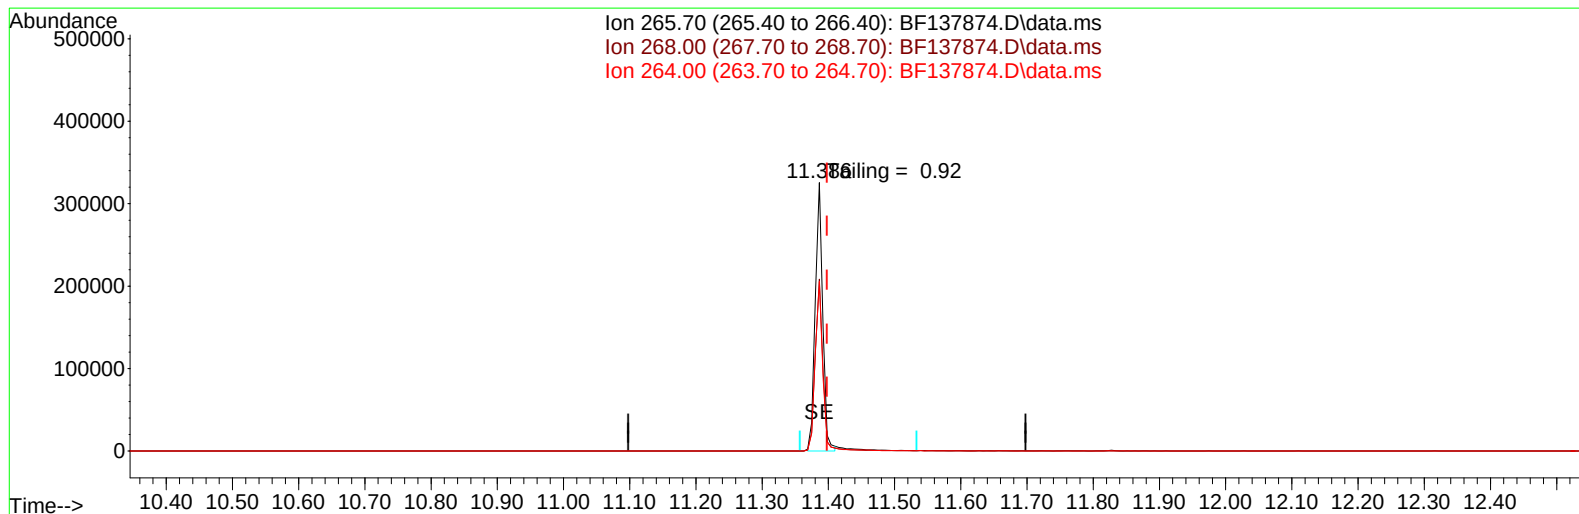

TIC: BF137874.D\data.ms




(70) Pentachlorophenol (C)

11.386min (-0.012) 27537.46 ng

response 269975

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	64.05
264.00	63.70	63.16
0.00	0.00	0.00

Quant Time: May 11 00:29:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 01 03:25:08 2024
Response via : Initial Calibration

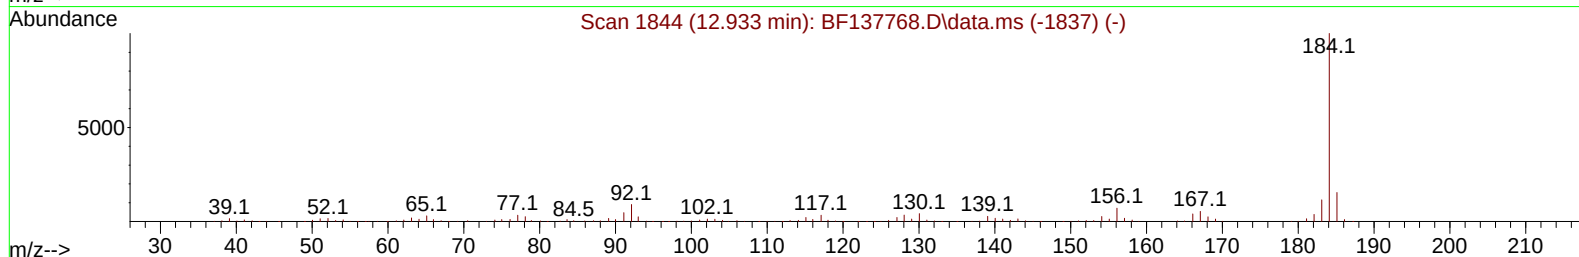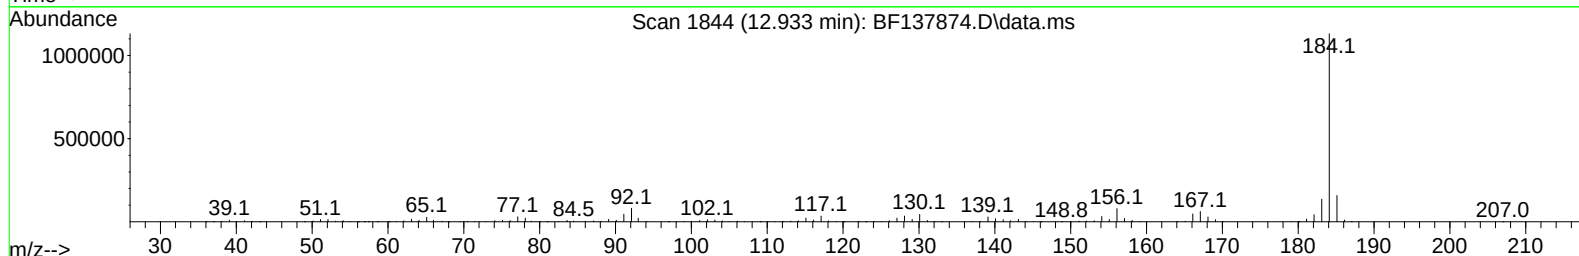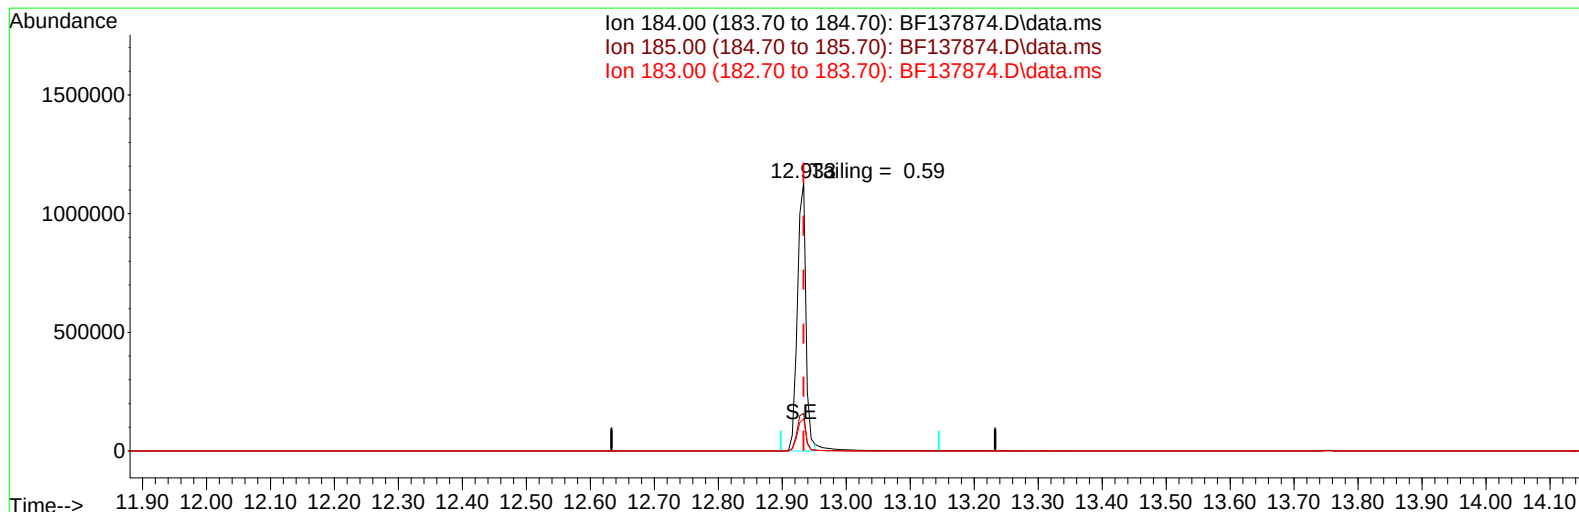

TIC: BF137874.D\data.ms

(77) Benzidine

12.933min (+ 0.000) 0.00 ng

response **1090250**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.01
183.00	11.50	12.02
0.00	0.00	0.00