

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051024\
 Data File : BF137891.D
 Acq On : 10 May 2024 20:21
 Operator : CG\JU
 Sample : P2432-06
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SW-04-011

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF137891.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.199	16	19	24	rVB2	61989	95062	2.98%	0.439%
2	2.416	49	56	62	rVB	1652740	2267000	71.06%	10.462%
3	5.669	604	609	612	rBV	2552889	2315239	72.57%	10.685%
4	6.657	772	777	780	rBV	2362699	2293532	71.89%	10.585%
5	7.045	840	843	847	rVB	1069643	887159	27.81%	4.094%
6	7.610	934	939	942	rBV	1641301	1495782	46.89%	6.903%
7	8.334	1058	1062	1065	rBV	1426397	1185291	37.15%	5.470%
8	9.404	1240	1244	1248	rBV	3529564	3190296	100.00%	14.723%
9	10.092	1357	1361	1365	rBV	1656932	1355306	42.48%	6.255%
10	10.175	1372	1375	1382	rVB3	29222	41003	1.29%	0.189%
11	10.881	1492	1495	1510	rBV	1720652	1567147	49.12%	7.232%
12	11.586	1612	1615	1619	rBV	1287934	1134837	35.57%	5.237%
13	12.092	1698	1701	1712	rBV3	83324	97831	3.07%	0.451%
14	13.033	1855	1861	1868	rVB2	38709	45967	1.44%	0.212%
15	13.174	1881	1885	1888	rBV	2649922	2241311	70.25%	10.344%
16	14.239	2062	2066	2079	rVB	841528	790479	24.78%	3.648%
17	15.804	2327	2332	2341	rBV	469107	665186	20.85%	3.070%




Sum of corrected areas: 21668428

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051024\
Data File : BF137891.D
Acq On : 10 May 2024 20:21
Operator : CG\JU
Sample : P2432-06
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SW-04-011

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

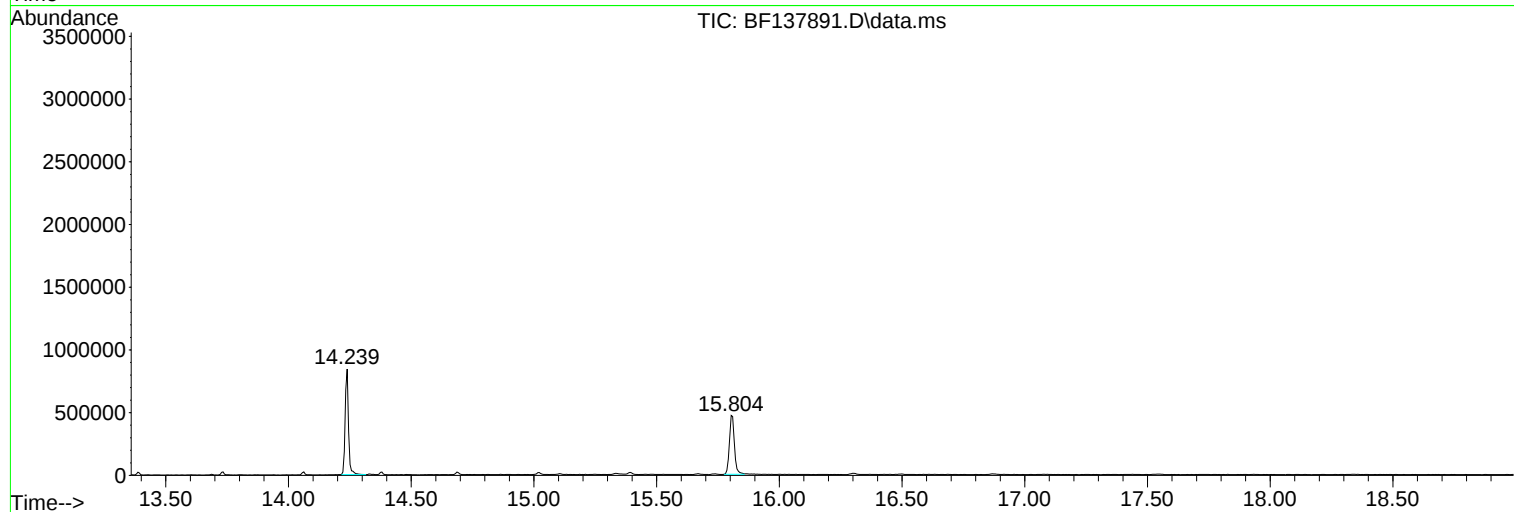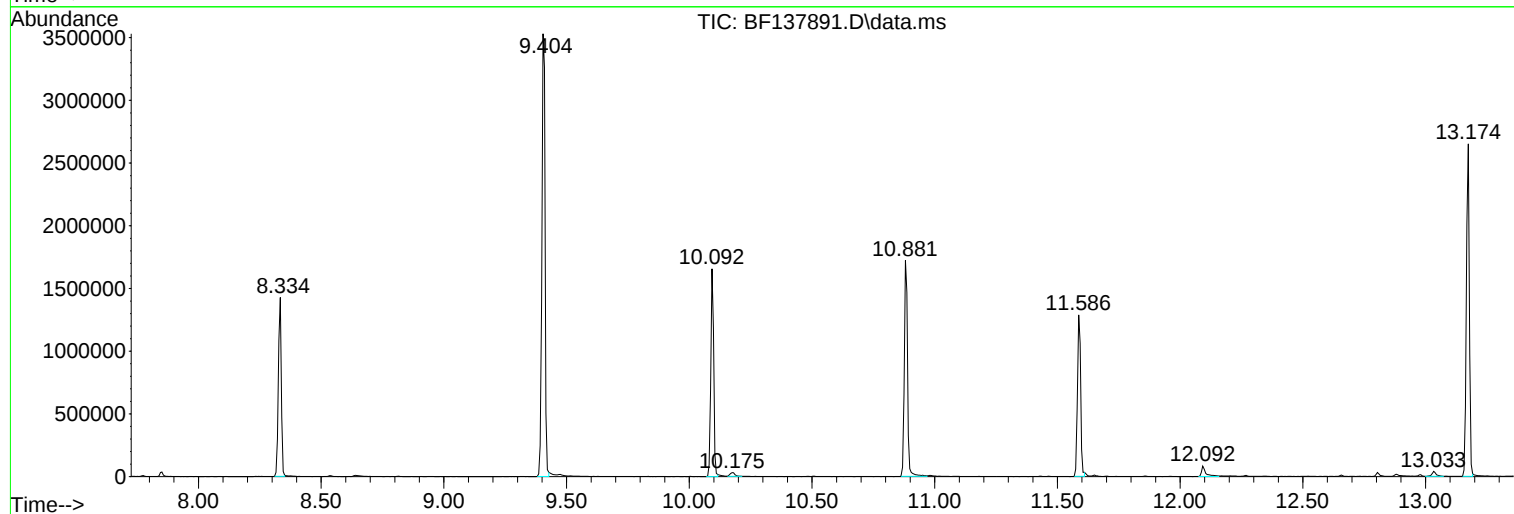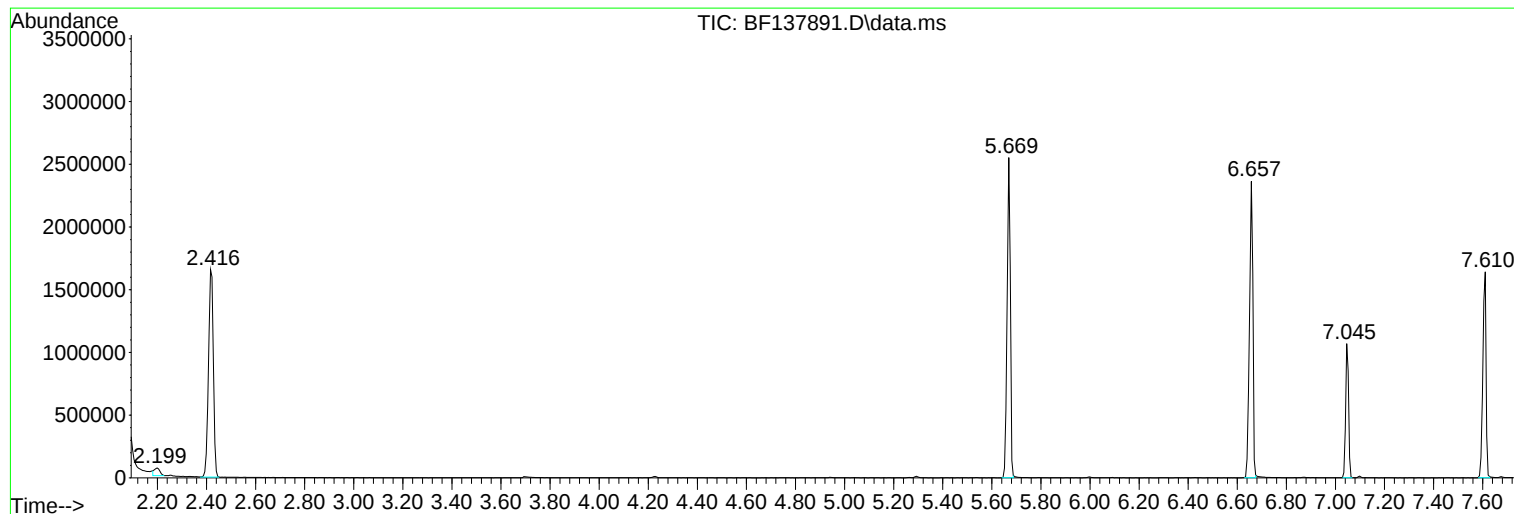

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051024\
Data File : BF137891.D
Acq On : 10 May 2024 20:21
Operator : CG\JU
Sample : P2432-06
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SW-04-011










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.416	51.11 ng	2267000	1,4-Dichlorobenzene-d4	7.045

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			1-(2-Methoxyethoxy)-2-methyl-2-p...	162	C8H18O3	1000364-24-4	25
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9

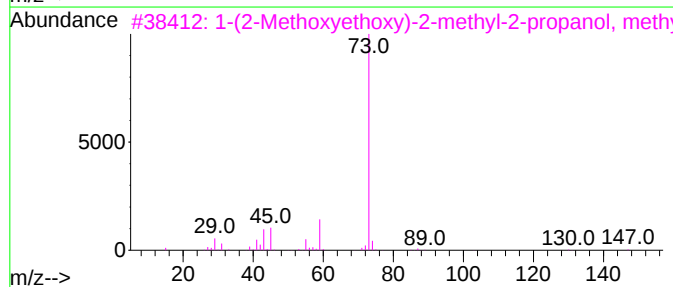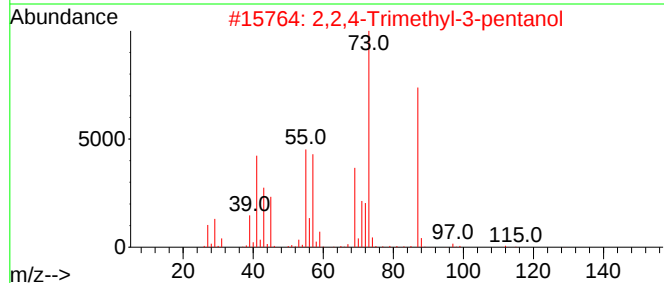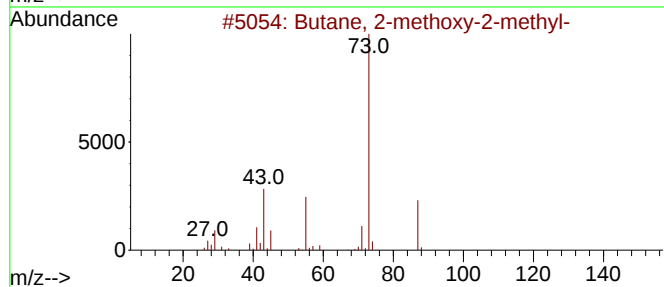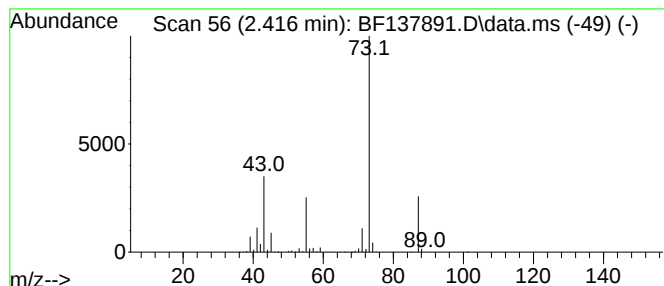

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051024\
Data File : BF137891.D
Acq On : 10 May 2024 20:21
Operator : CG\JU
Sample : P2432-06
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SW-04-011

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.416	51.1	ng	2267000	1	7.045	887159	20.0