


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051024\
Data File : BF137874.D
Acq On : 10 May 2024 11:34
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 01 03:25:08 2024

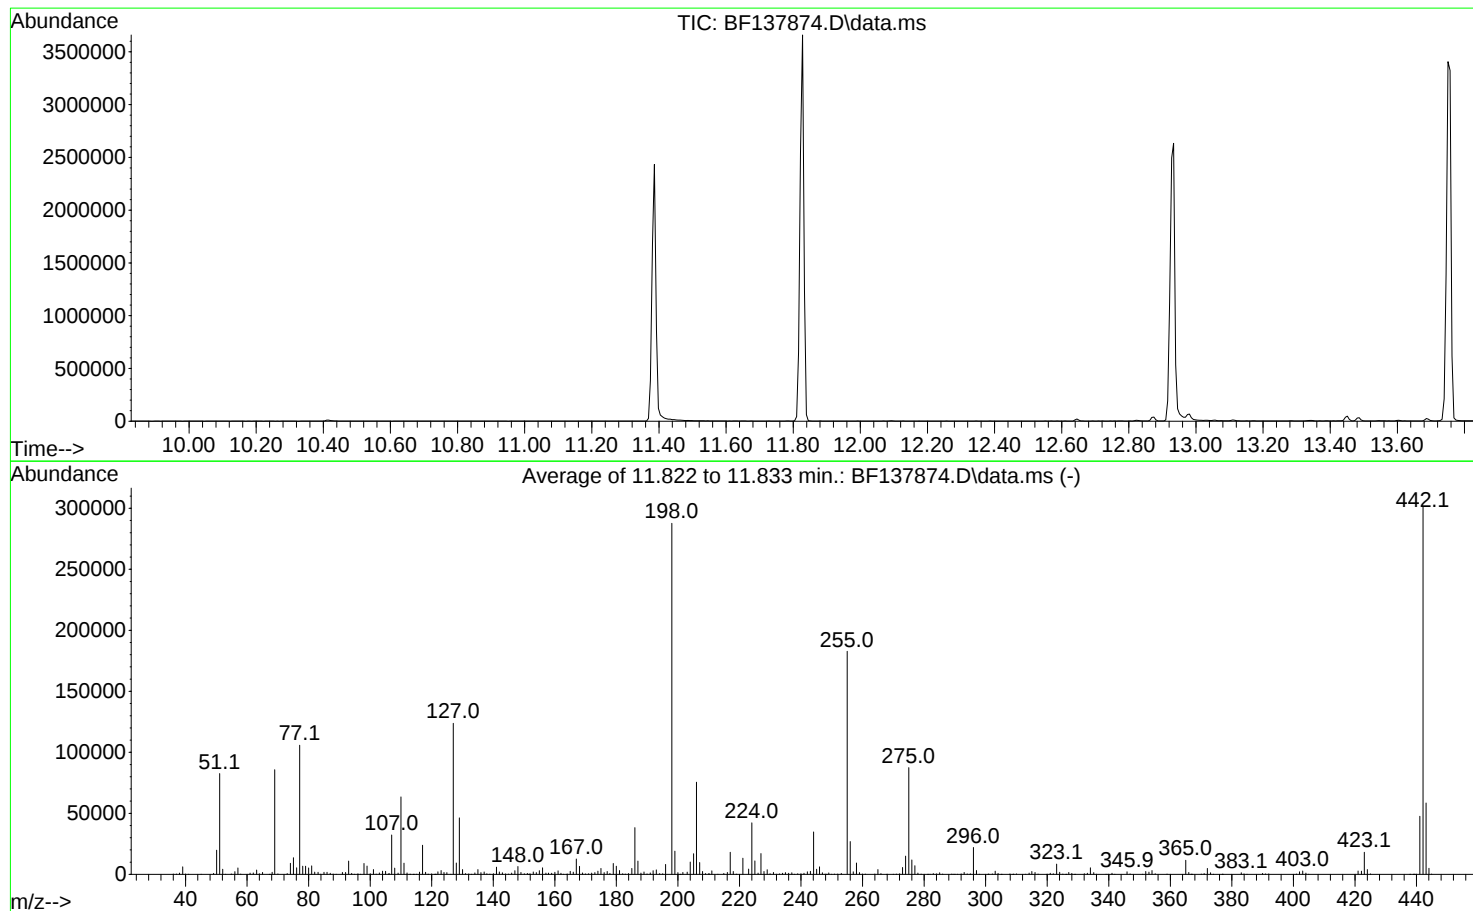

AutoFind: Scans 1655, 1656, 1657; Background Corrected with Scan 1650

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	28.7	82600	PASS
68	69	0.00	2	2.0	1674	PASS
69	198	0.00	100	29.8	85763	PASS
70	69	0.00	2	0.5	388	PASS
127	198	10	80	43.0	123800	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	287699	PASS
199	198	5	9	6.6	19081	PASS
275	198	10	60	30.4	87451	PASS
365	198	1	100	4.0	11526	PASS
441	198	0.01	100	16.5	47555	PASS
442	442	50	100	100.0	301440	PASS
443	442	15	24	19.4	58472	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/10/2024	BNA_F	<u>BF137874.D</u>
Compound Name	Response	Retention Time
DDT	655814	13.757
DDD	13946	13.451
DDE	1209	13.11
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15155	670969	2.26

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051024\
 Data File : BF137874.D
 Acq On : 10 May 2024 11:34
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 11 00:29:32 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF043024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 01 03:25:08 2024
 Response via : Initial Calibration

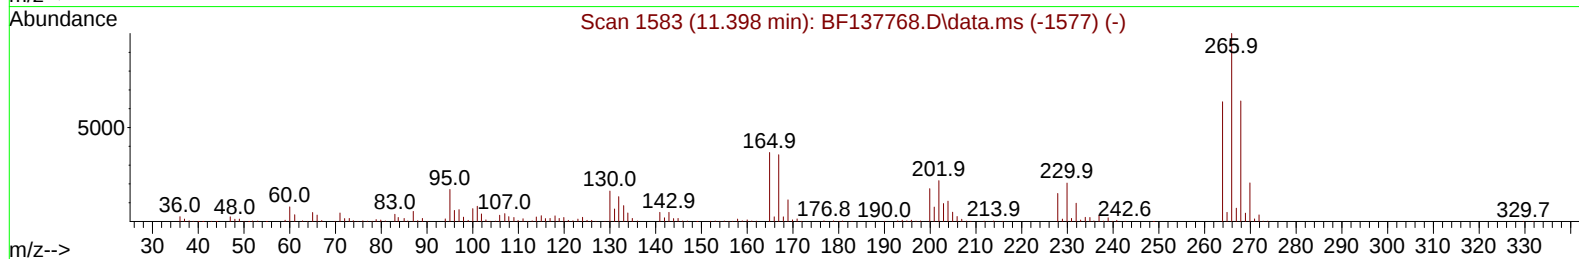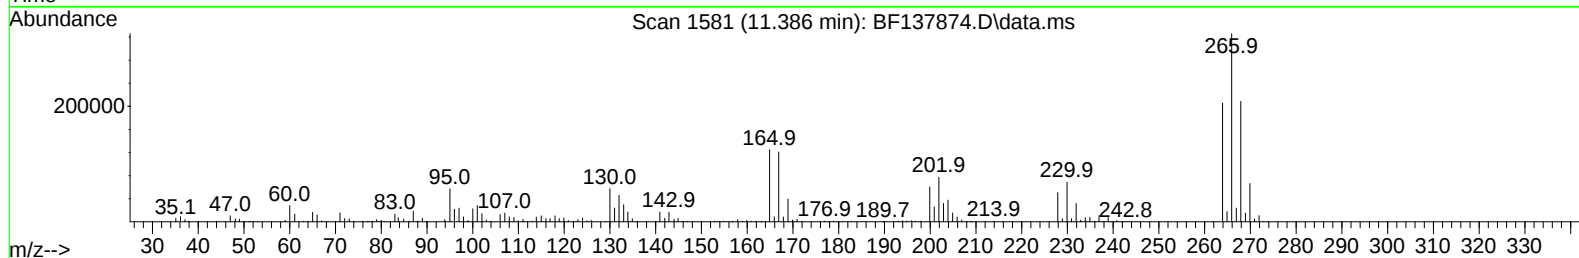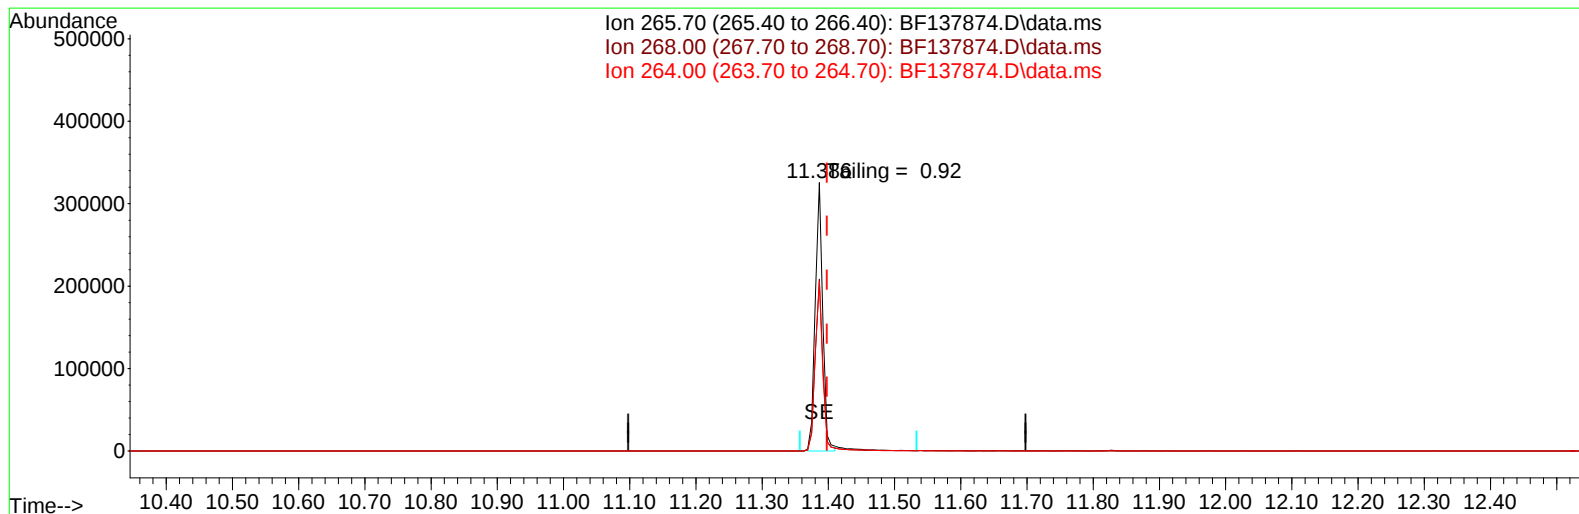

TIC: BF137874.D\data.ms

(70) Pentachlorophenol (C)

11.386min (-0.012) 27537.46 ng

response 269975

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	64.05
264.00	63.70	63.16
0.00	0.00	0.00

