


Data Path : Z:\HPCHEM1\BNA F\Data\BF051115\
Data File : BF079133.D
Acq On : 12 May 2015 00:56
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Apr 30 19:07:47 2015

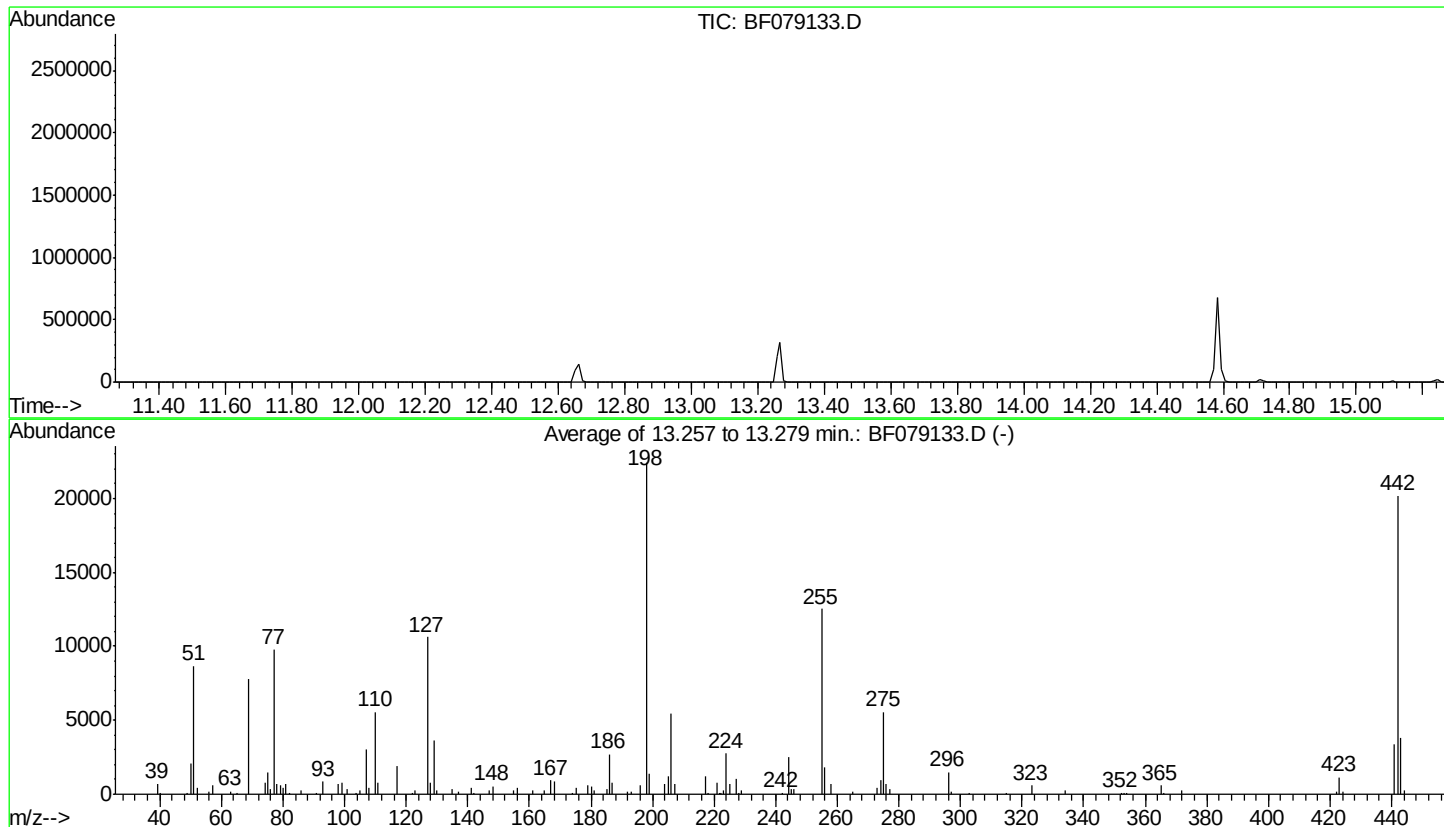

AutoFind: Scans 1056, 1057, 1058; Background Corrected with Scan 1052

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	8692	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.6	7762	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.5	10643	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	22422	PASS
199	198	5	9	6.3	1422	PASS
275	198	10	60	24.9	5577	PASS
365	198	1	100	2.6	585	PASS
441	442	0.01	24	16.8	3391	PASS
442	198	50	100	90.0	20185	PASS
443	442	15	24	18.8	3797	PASS