


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF051116\  
Data File : BF086918.D  
Acq On : 12 May 2016 6:33  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050916.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Thu May 12 15:26:18 2016

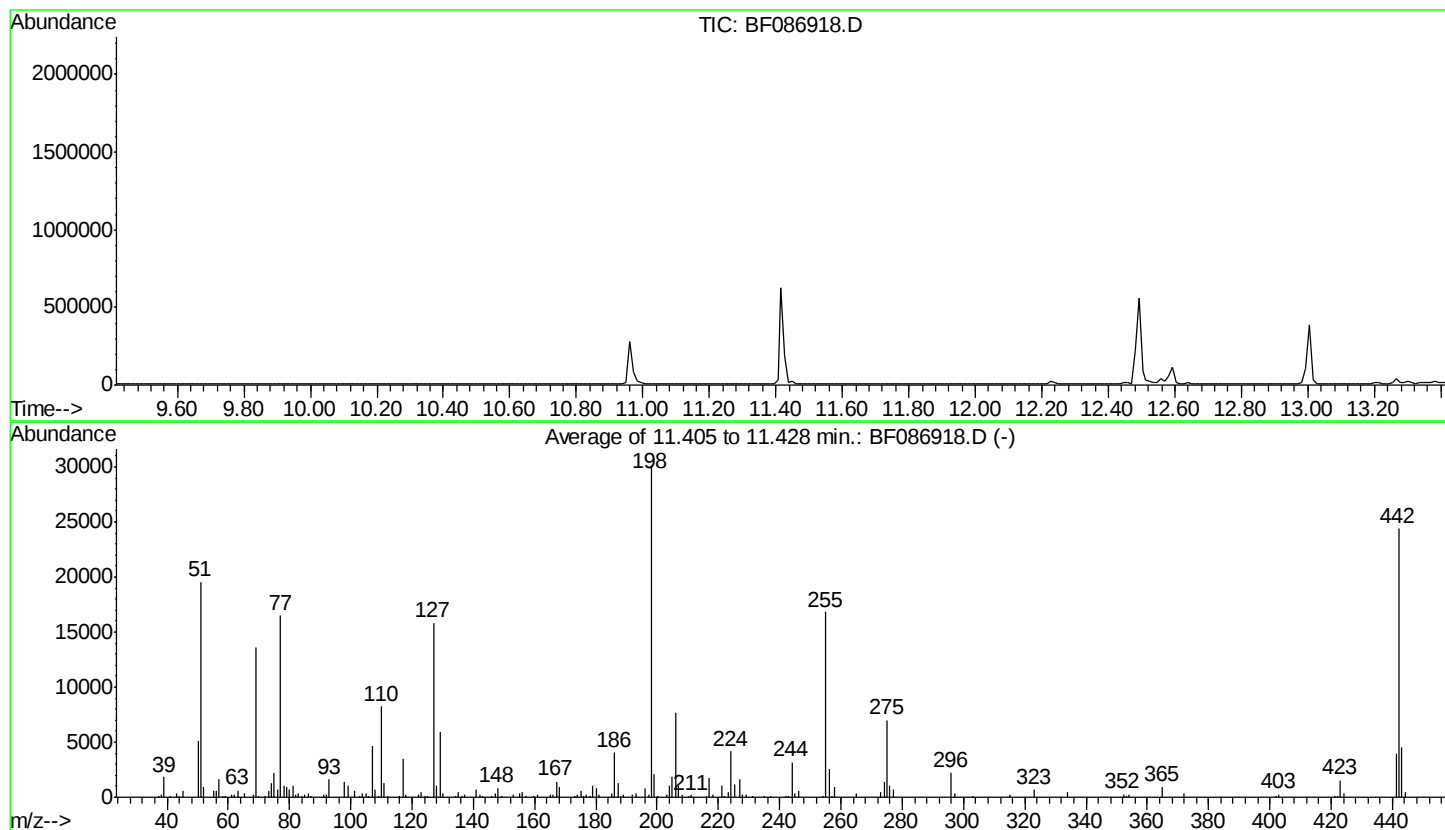

AutoFind: Scans 859, 860, 861; Background Corrected with Scan 856

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 65.0         | 19569      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.8          | 242        | PASS                |
| 69             | 198             | 0.00            | 100             | 45.4         | 13657      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.8          | 105        | PASS                |
| 127            | 198             | 10              | 80              | 52.6         | 15835      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.7          | 206        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 30114      | PASS                |
| 199            | 198             | 5               | 9               | 7.0          | 2099       | PASS                |
| 275            | 198             | 10              | 60              | 23.2         | 6992       | PASS                |
| 365            | 198             | 1               | 100             | 3.2          | 962        | PASS                |
| 441            | 442             | 0.01            | 24              | 16.3         | 3979       | PASS                |
| 442            | 198             | 50              | 100             | 81.0         | 24397      | PASS                |
| 443            | 442             | 15              | 24              | 18.7         | 4566       | PASS                |