
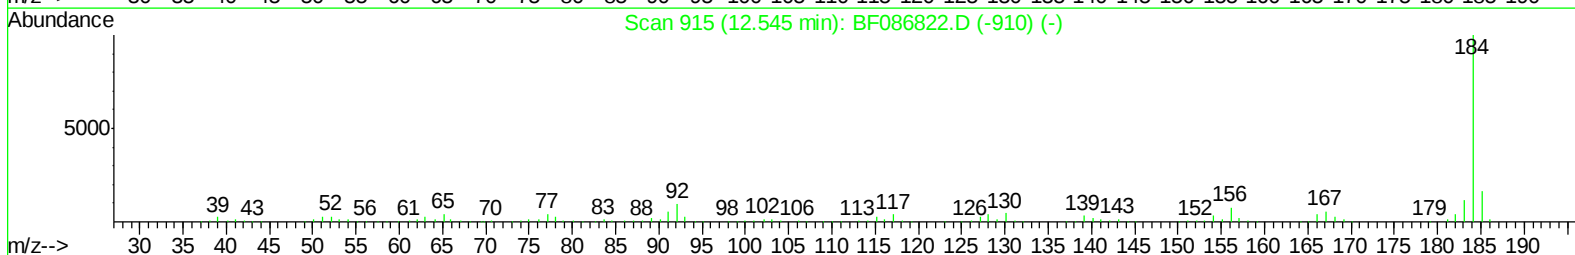
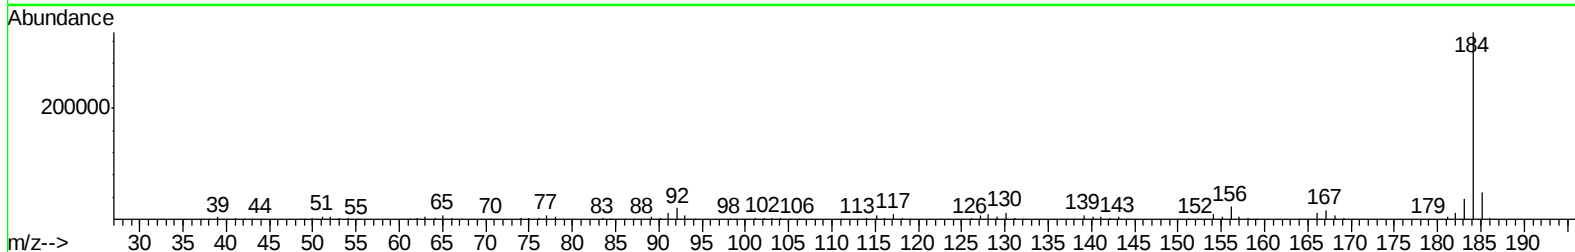


Data Path : Z:\HPCHEM1\BNA_F\Data\BF051116\
Data File : BF086895.D
Acq On : 11 May 2016 17:45
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 09:11:41 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 12 01:06:48 2016
Response via : Initial Calibration

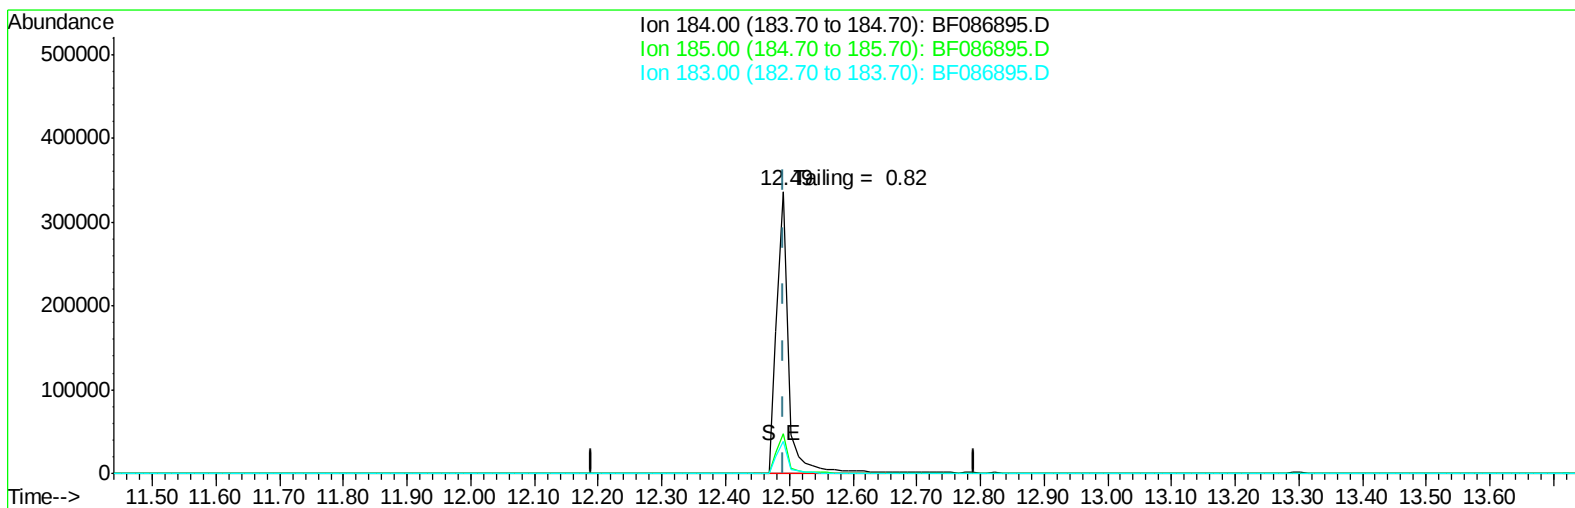

TIC: BF086895.D

(76) Benzidine




12.491min (+0.000) 0.00ng

response 438144

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	14.19
183.00	12.20	11.24
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF051116\
Data File : BF086895.D
Acq On : 11 May 2016 17:45
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 09:11:41 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 12 01:06:48 2016
Response via : Initial Calibration

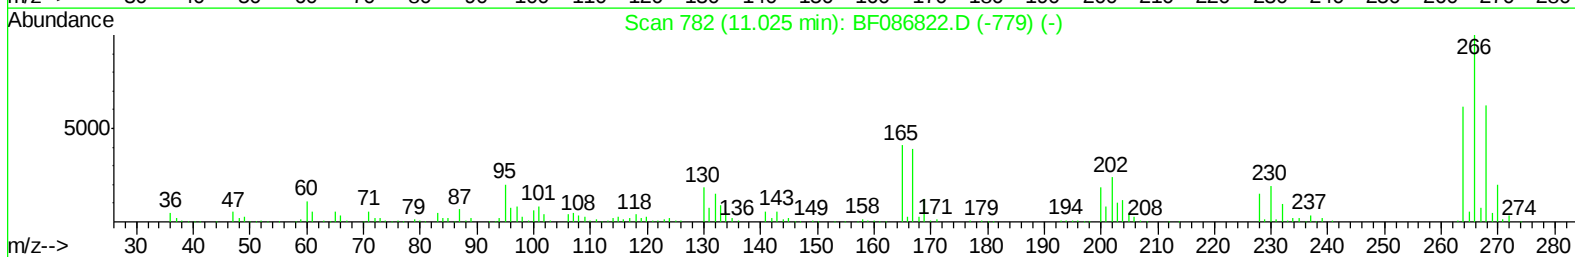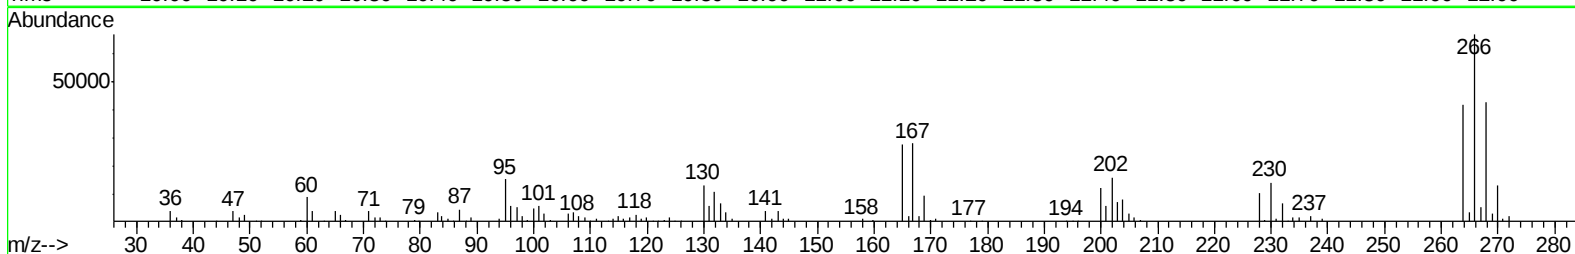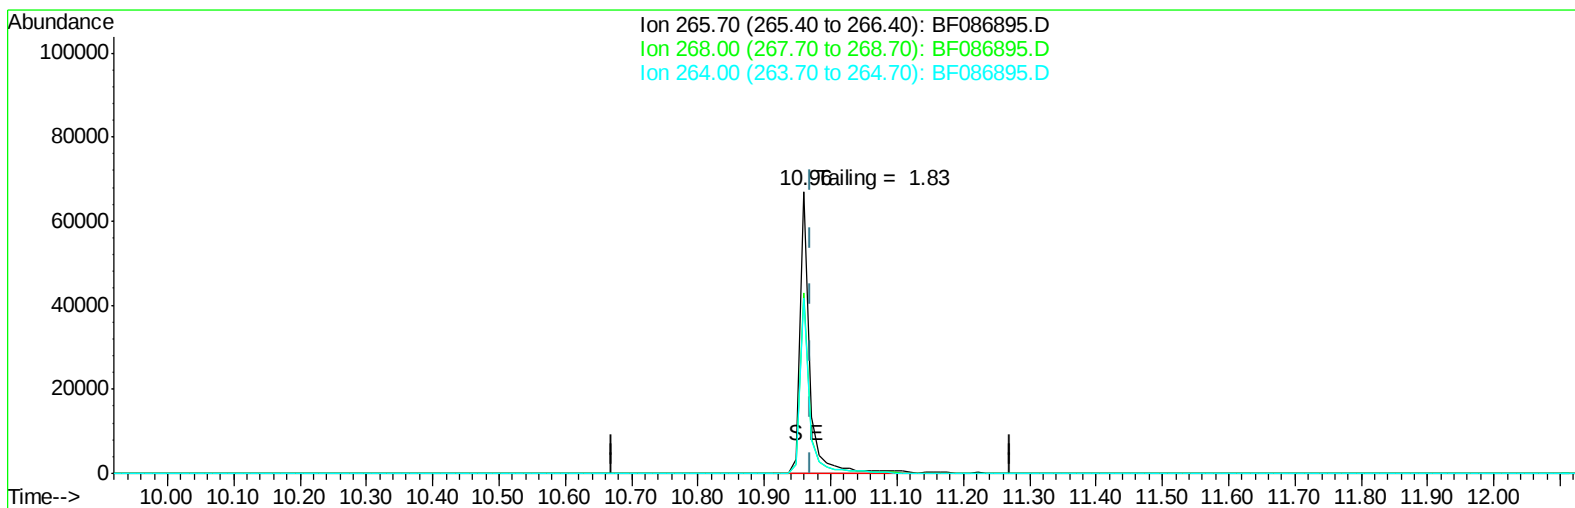

TIC: BF086895.D

(69) Pentachlorophenol (C)

10.959min (-0.011) 0.00ng

response 68455

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	64.16
264.00	66.10	62.47
0.00	0.00	0.00