


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051116\
 Data File : BF086918.D
 Acq On : 12 May 2016 6:33
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon May 09 16:04:56 2016

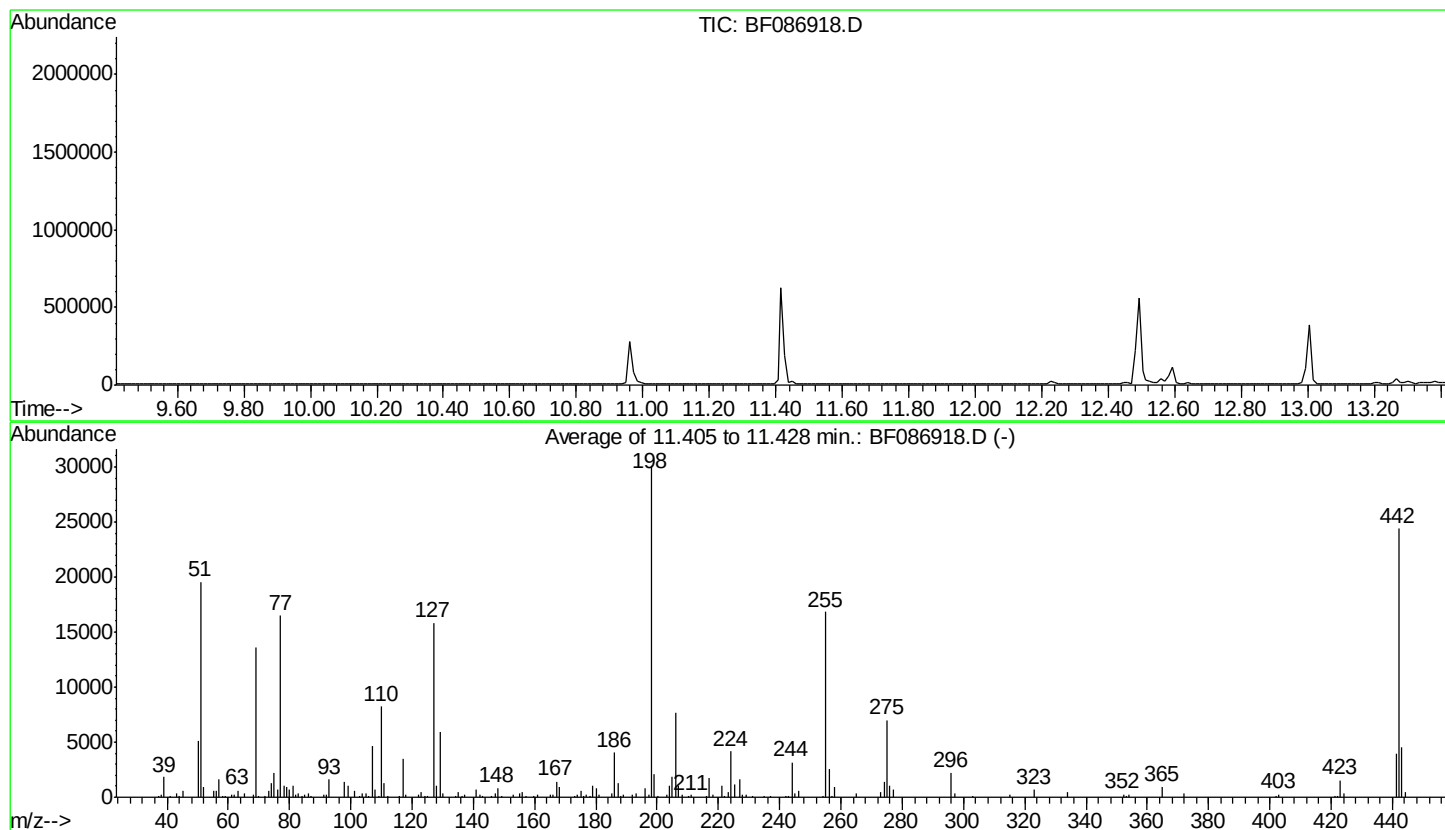

AutoFind: Scans 859, 860, 861; Background Corrected with Scan 856

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	65.0	19569	PASS
68	69	0.00	2	1.8	242	PASS
69	198	0.00	100	45.4	13657	PASS
70	69	0.00	2	0.8	105	PASS
127	198	10	80	52.6	15835	PASS
197	198	0.00	2	0.7	206	PASS
198	198	100	100	100.0	30114	PASS
199	198	5	9	7.0	2099	PASS
275	198	10	60	23.2	6992	PASS
365	198	1	100	3.2	962	PASS
441	442	0.01	24	16.3	3979	PASS
442	198	50	100	81.0	24397	PASS
443	442	15	24	18.7	4566	PASS