
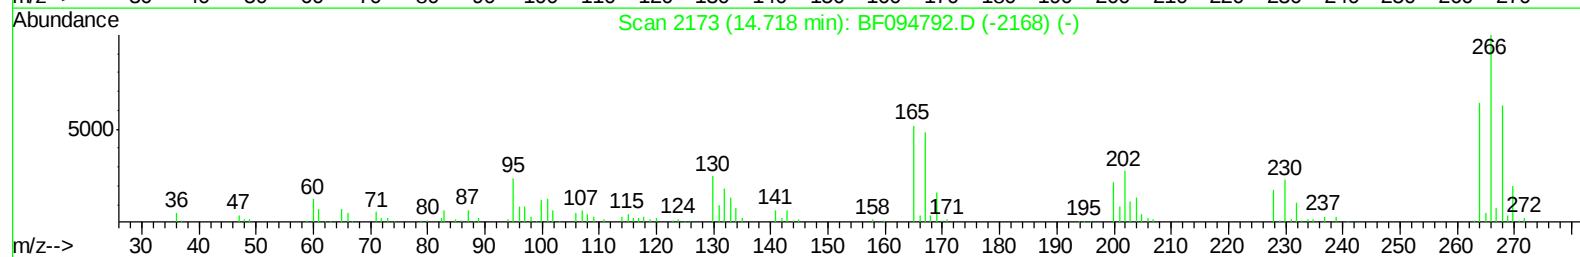
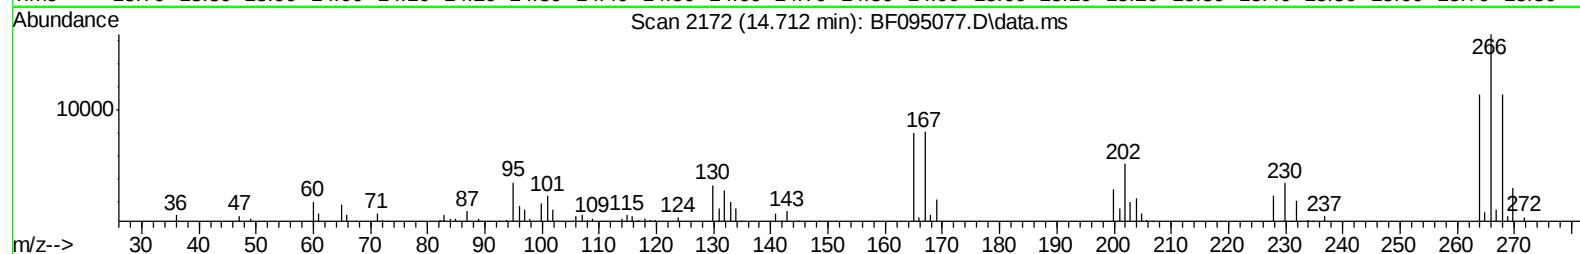


Data Path : Z:\HPCHEM1\BNA F\Data\BF051117\  
Data File : BF095077.D  
Acq On : 11 May 2017 12:55  
Operator : SJ/MA  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 19:03:44 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed May 03 17:24:51 2017  
Response via : Initial Calibration

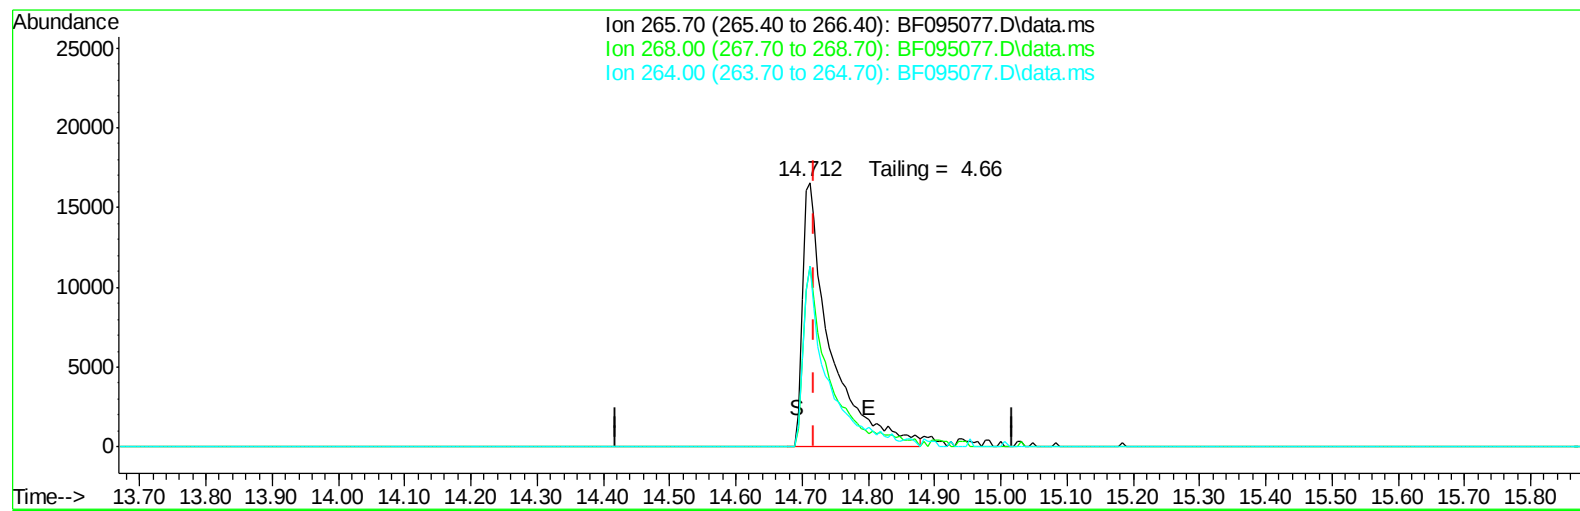

TIC: BF095077.D\data.ms

(69) Pentachlorophenol (C)




14.712min (-0.006) 0.00ng

response 47862

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 68.59 |
| 264.00 | 64.60 | 68.25 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA F\Data\BF051117\  
Data File : BF095077.D  
Acq On : 11 May 2017 12:55  
Operator : SJ/MA  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 19:03:44 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed May 03 17:24:51 2017  
Response via : Initial Calibration

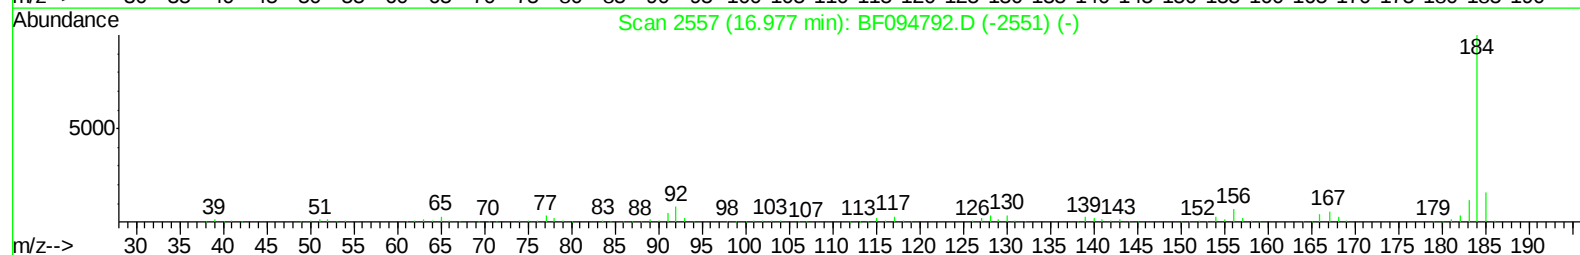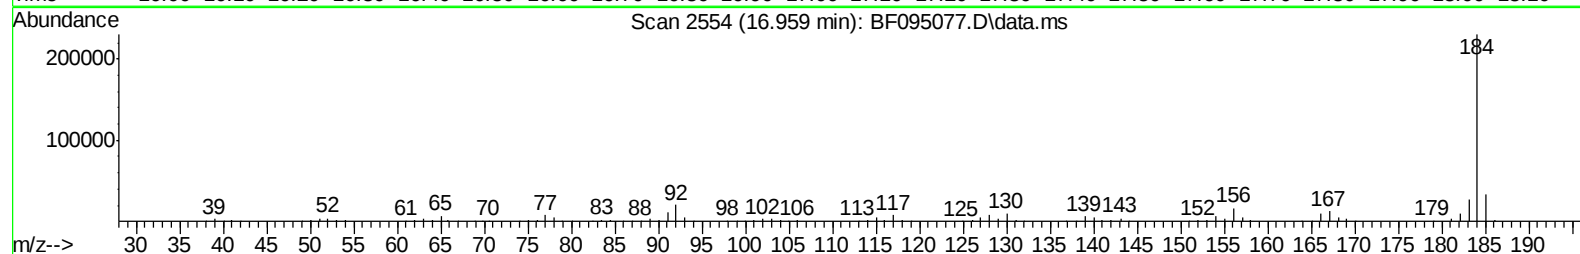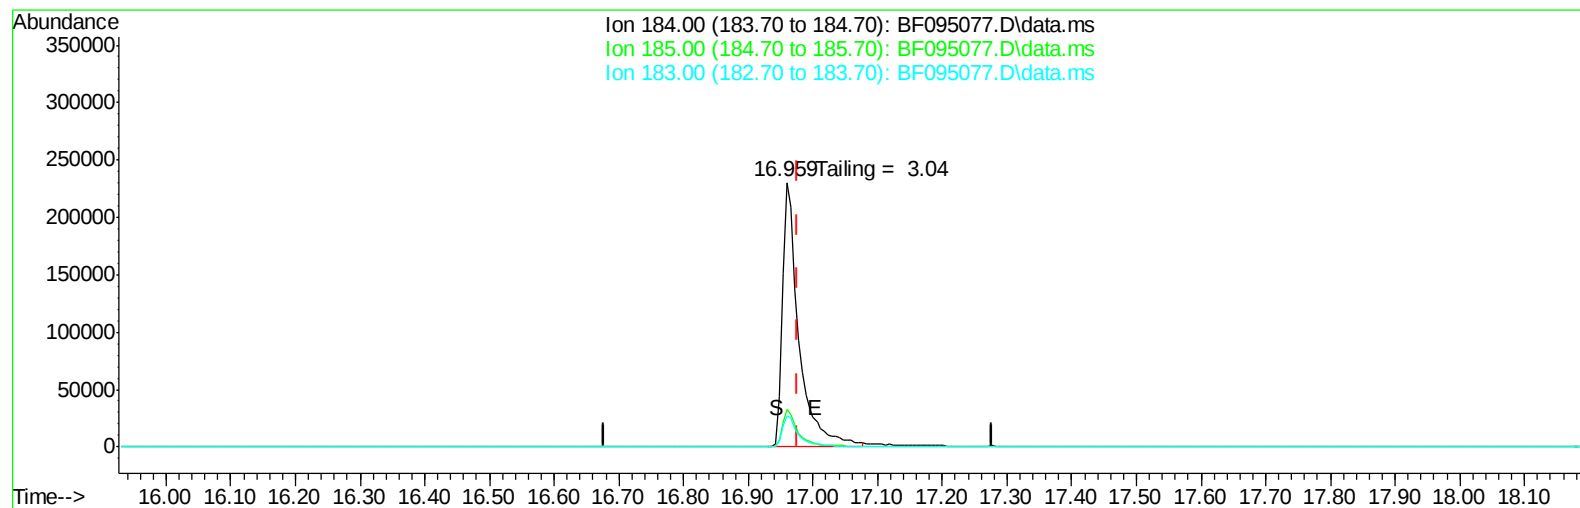

TIC: BF095077.D\data.ms

(76) Benzidine

16.959min (-0.018) 0.00ng

response 419740

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 184.00 | 100   | 100    |
| 185.00 | 19.40 | 14.28# |
| 183.00 | 12.20 | 11.62  |
| 0.00   | 0.00  | 0.00   |