
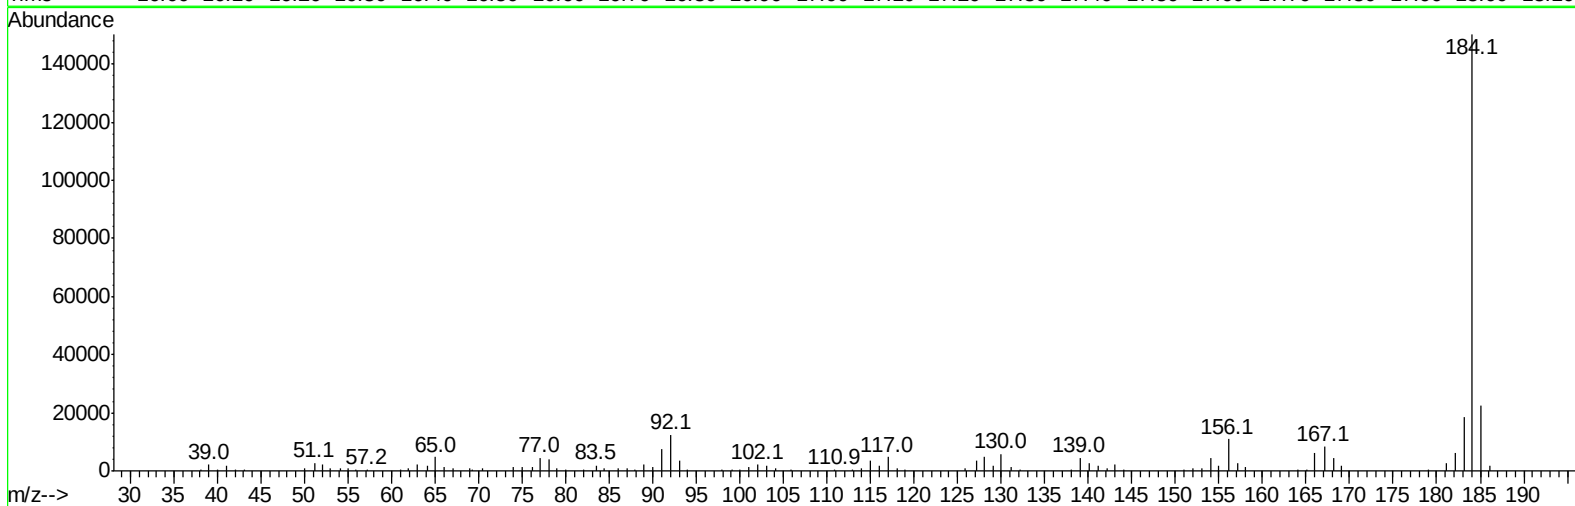


Data Path : Z:\HPCHEM1\BNA F\DATA\BF051117\
Data File : BF095099.D
Acq On : 12 May 2017 2:01
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 06:39:50 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

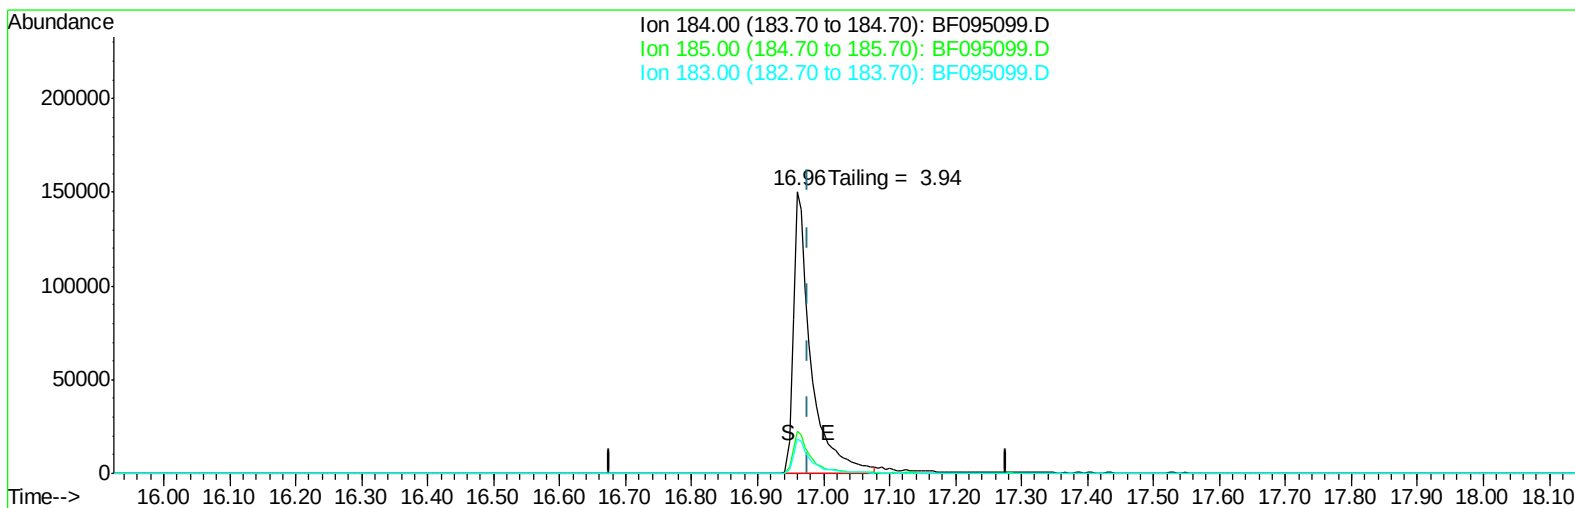

TIC: BF095099.D

(76) Benzidine



16.959min (-0.018) 0.00ng

response 285702

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	15.01#
183.00	12.20	12.24
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051117\
Data File : BF095099.D
Acq On : 12 May 2017 2:01
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 06:39:50 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 03 17:24:51 2017
Response via : Initial Calibration

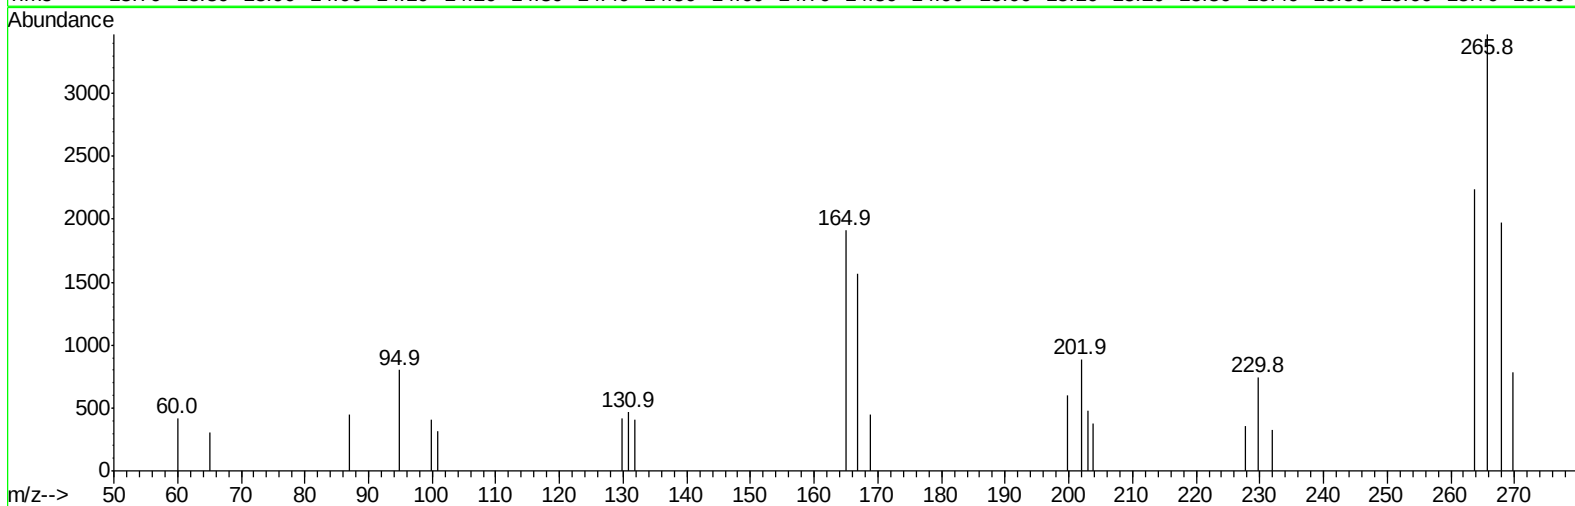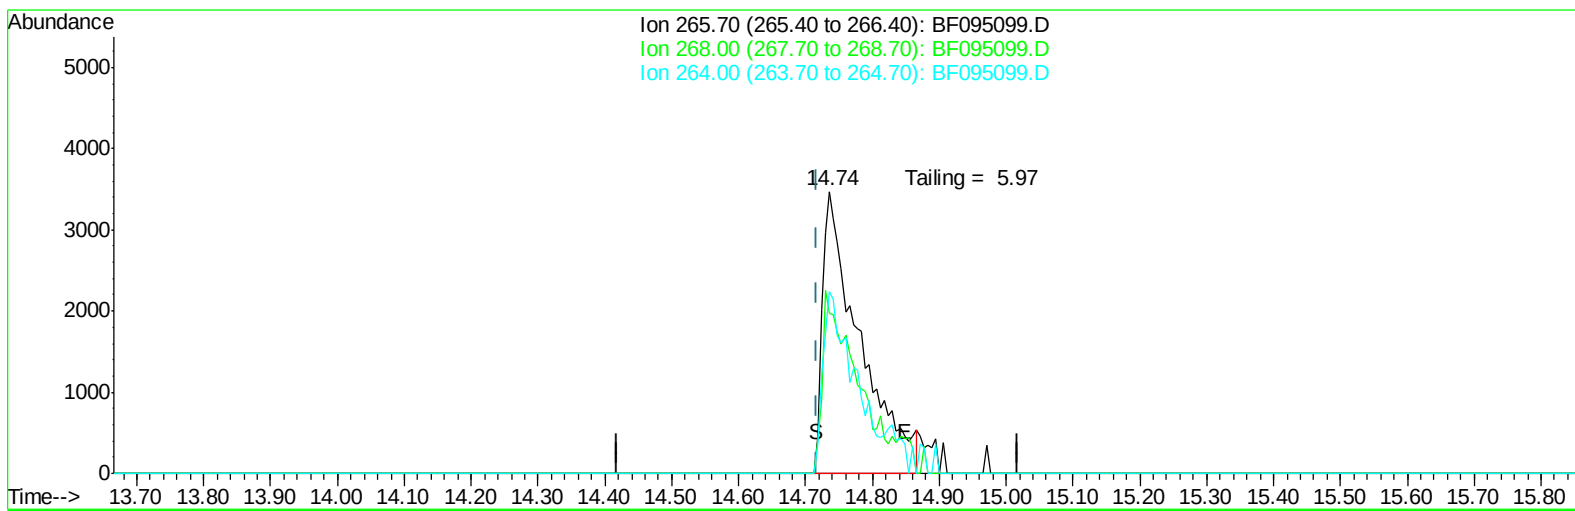

TIC: BF095099.D

(69) Pentachlorophenol (C)

14.736min (+0.018) 0.00ng

response 12917

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	57.04
264.00	64.60	64.56
0.00	0.00	0.00