


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051121\
 Data File : BF123908.D
 Acq On : 11 May 2021 13:39
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 11 18:02:17 2021

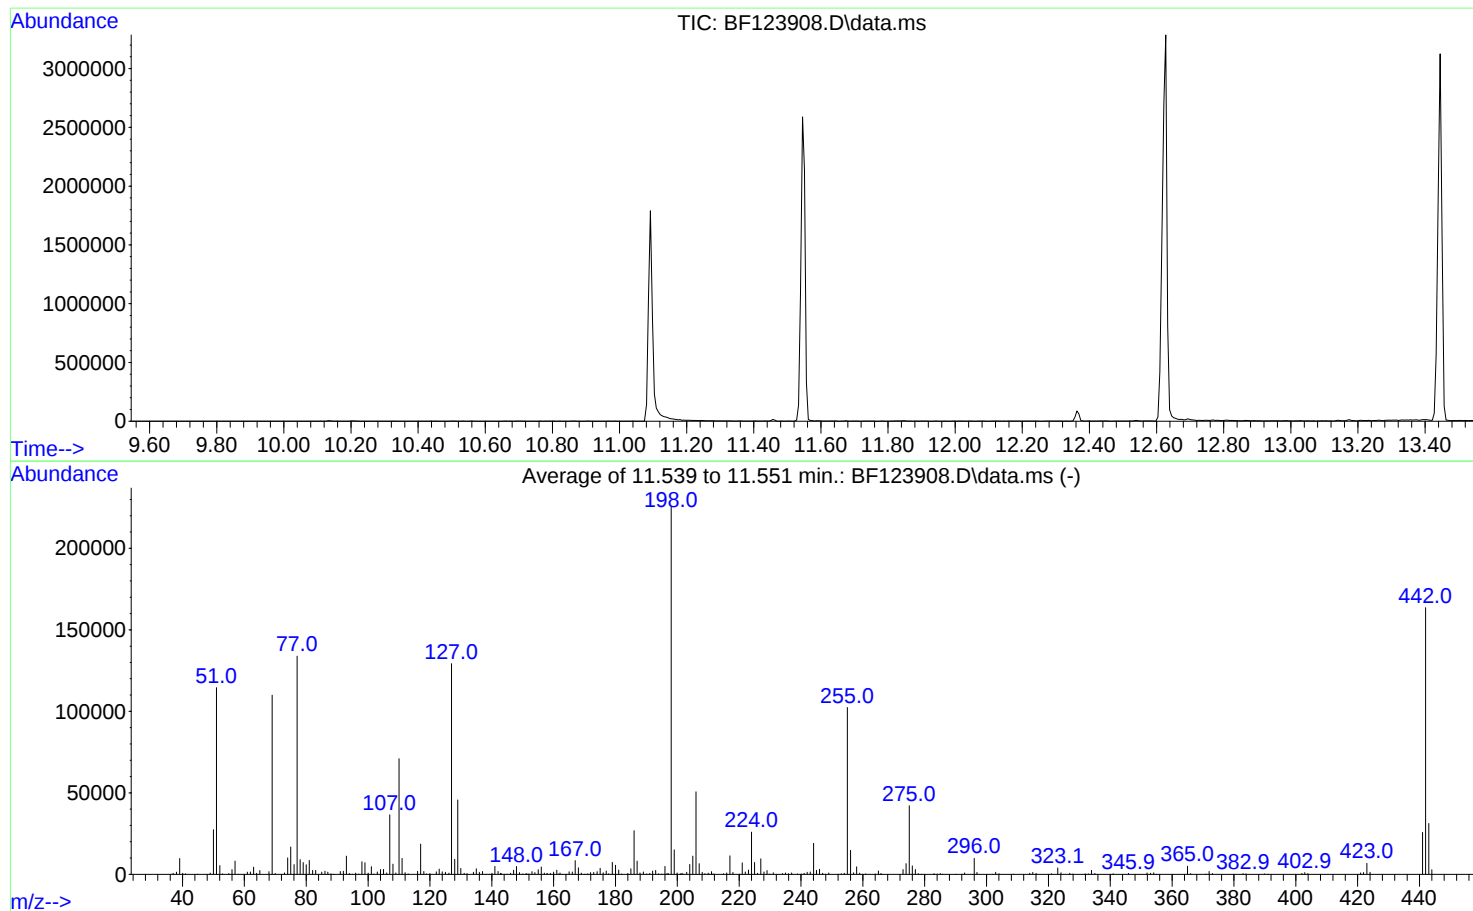




AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.8	114579	PASS
68	69	0.00	2	1.6	1716	PASS
69	198	0.00	100	48.7	109893	PASS
70	69	0.00	2	0.5	568	PASS
127	198	10	80	57.3	129267	PASS
197	198	0.00	2	0.3	580	PASS
198	198	100	100	100.0	225659	PASS
199	198	5	9	6.6	14985	PASS
275	198	10	60	18.6	42077	PASS
365	198	1	100	2.2	4973	PASS
441	198	0.01	100	11.4	25735	PASS
442	442	50	100	100.0	163656	PASS
443	442	15	24	19.0	31168	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051121\
 Data File : BF123908.D
 Acq On : 11 May 2021 13:39
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 11 14:28:13 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 11 14:22:25 2021
 Response via : Initial Calibration

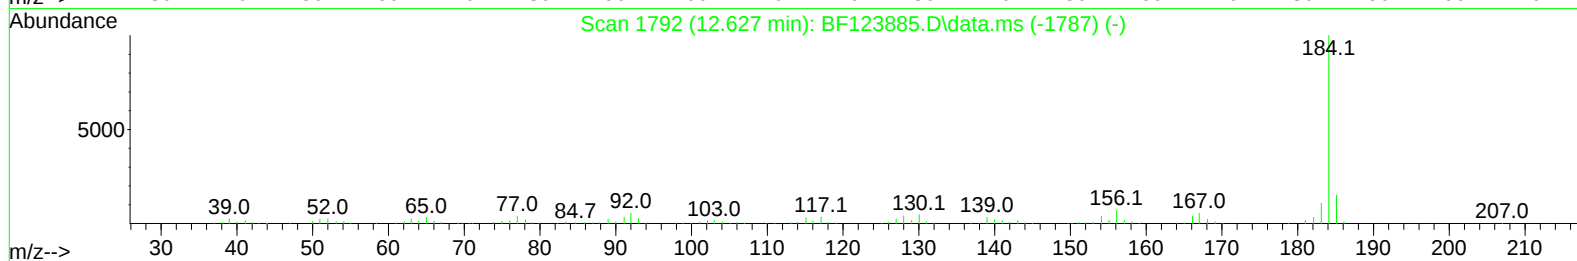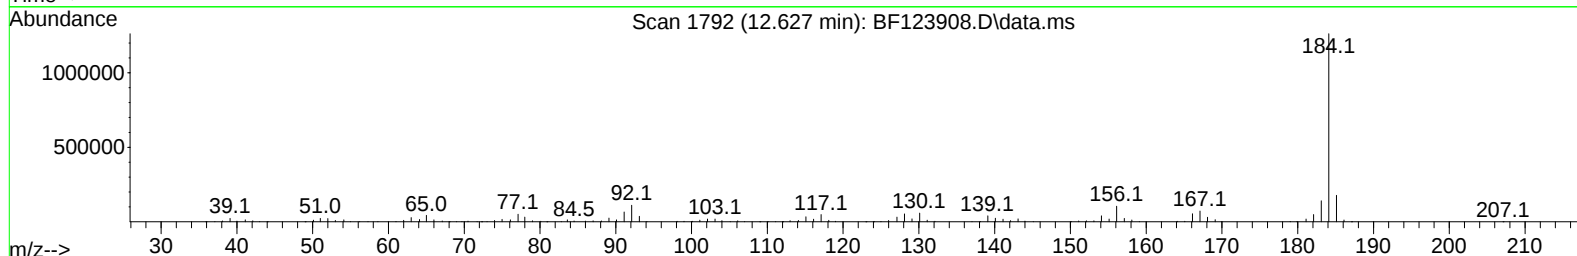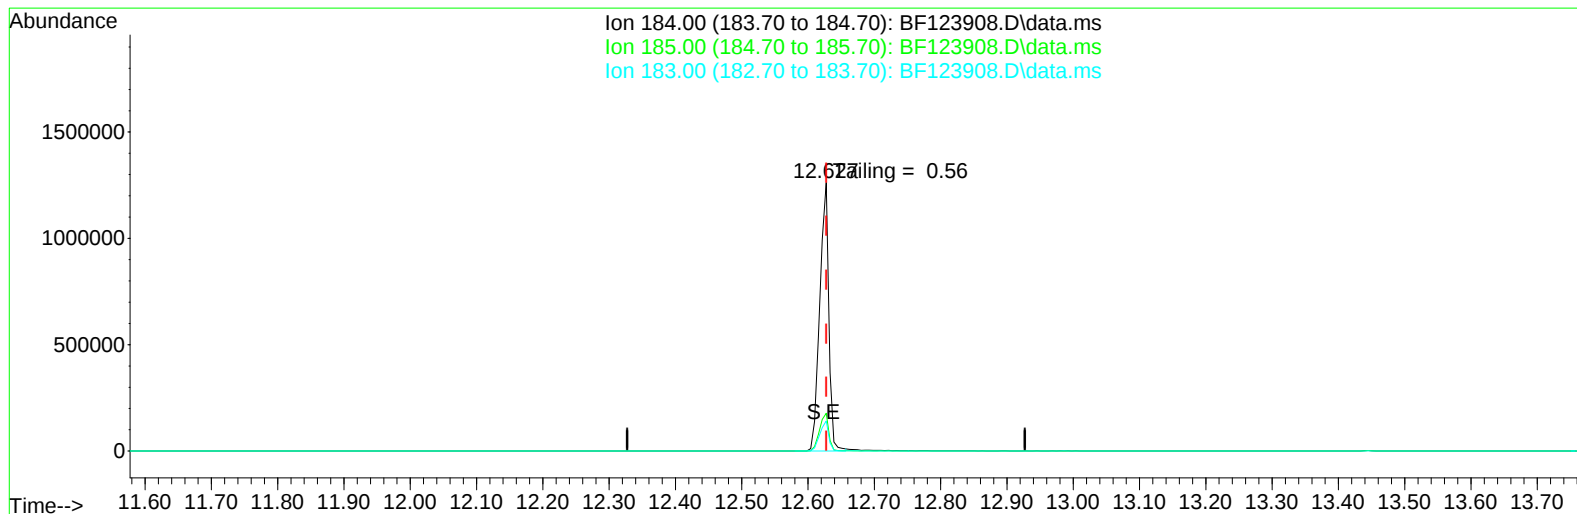

TIC: BF123908.D\data.ms

(77) Benzidine

12.627min (+ 0.000) 0.00 ng




response 1219928

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.09
183.00	9.80	11.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051121\
 Data File : BF123908.D
 Acq On : 11 May 2021 13:39
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 11 14:28:13 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 11 14:22:25 2021
 Response via : Initial Calibration

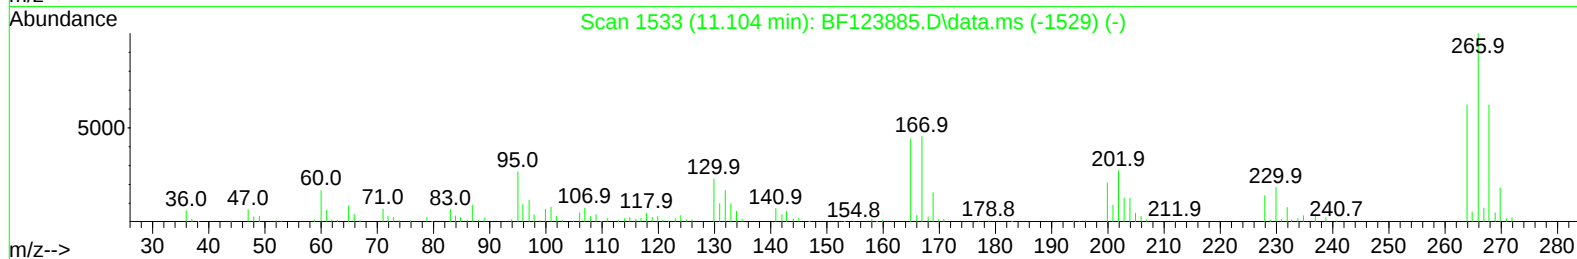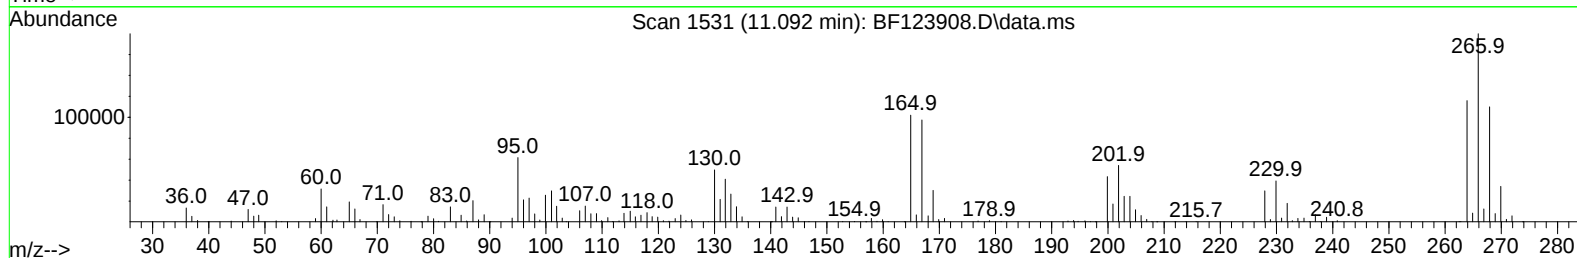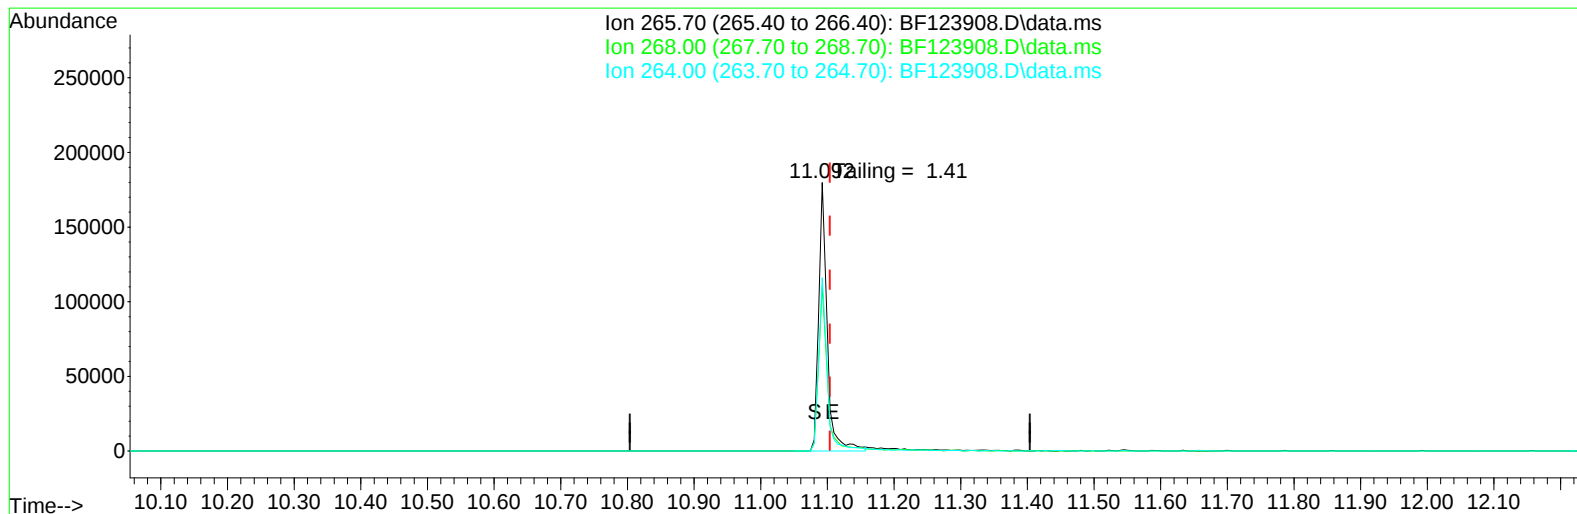

TIC: BF123908.D\data.ms

(70) Pentachlorophenol (C)

11.092min (-0.012) 31384.16 ng

response 166287

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	61.18
264.00	65.70	64.50
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/11/2021	BNA_F	<u>BF123908.D</u>
Compound Name	Response	Retention Time
DDT	468705	13.44
DDD	951	13.14
DDE	513	12.81
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1464	470169	0.31