
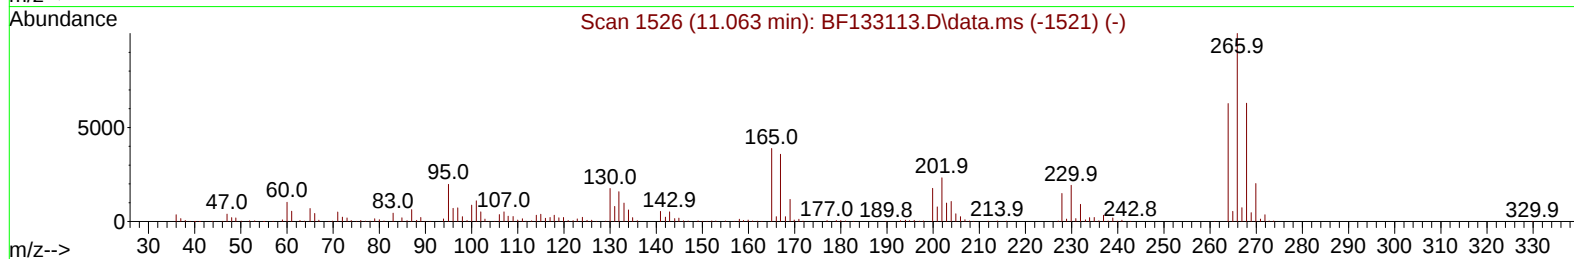
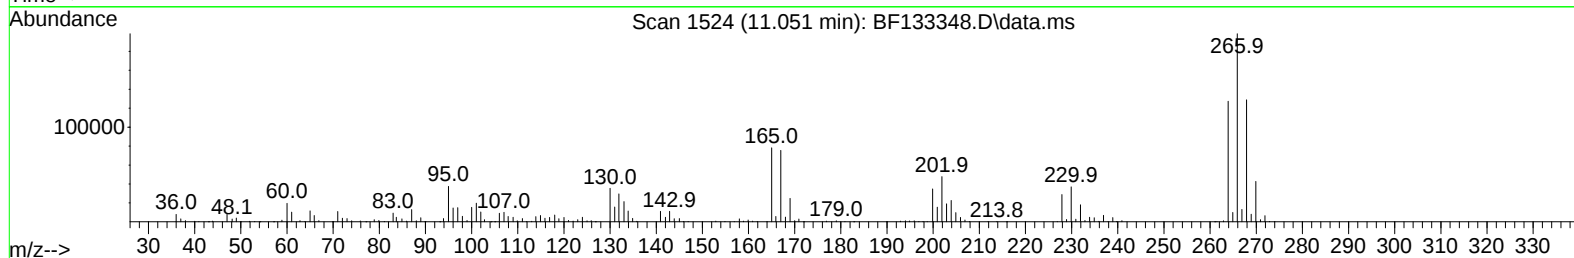


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051123\
Data File : BF133348.D
Acq On : 11 May 2023 11:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 12:32:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 09 04:59:36 2023
Response via : Initial Calibration

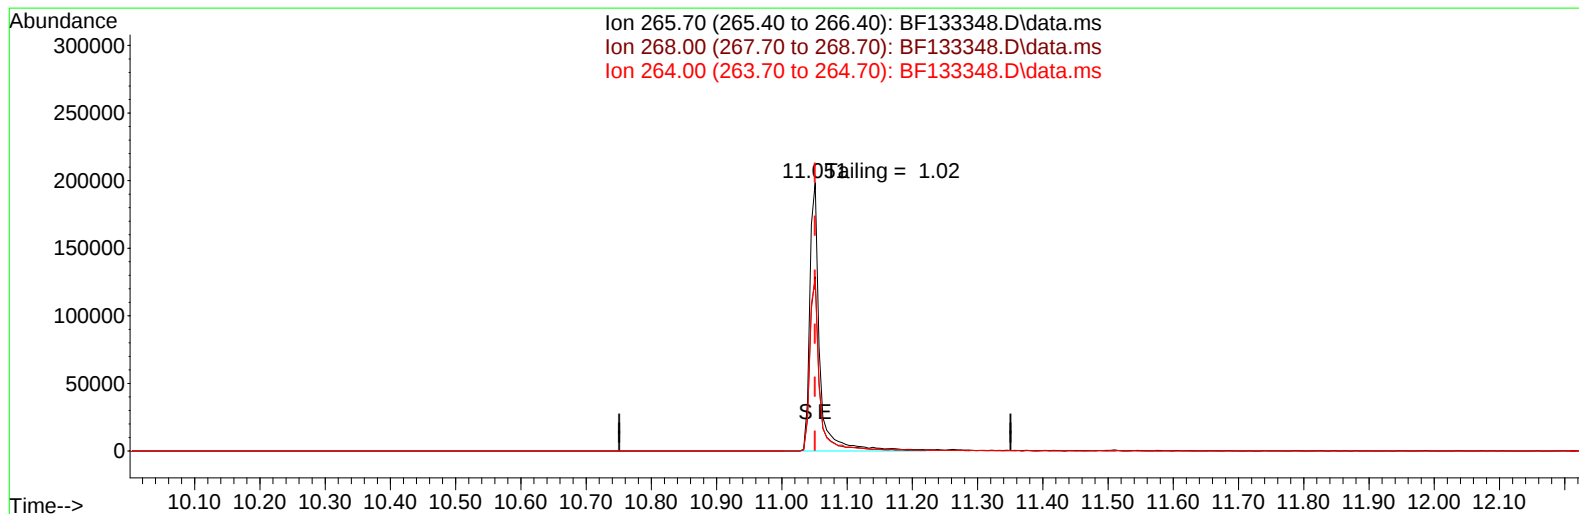

TIC: BF133348.D\data.ms

(70) Pentachlorophenol (C)




11.051min (+ 0.000) 77143.67 ng

response 212482

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	64.85
264.00	63.30	64.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051123\
Data File : BF133348.D
Acq On : 11 May 2023 11:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 11 12:32:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 09 04:59:36 2023
Response via : Initial Calibration

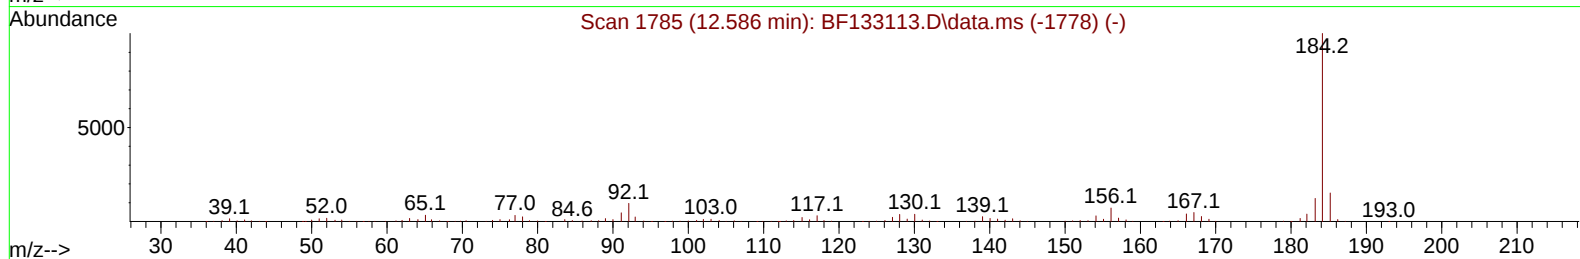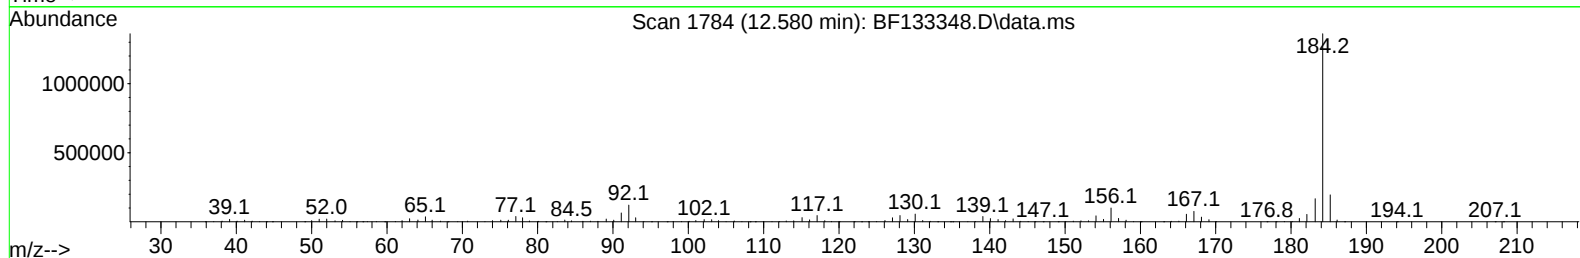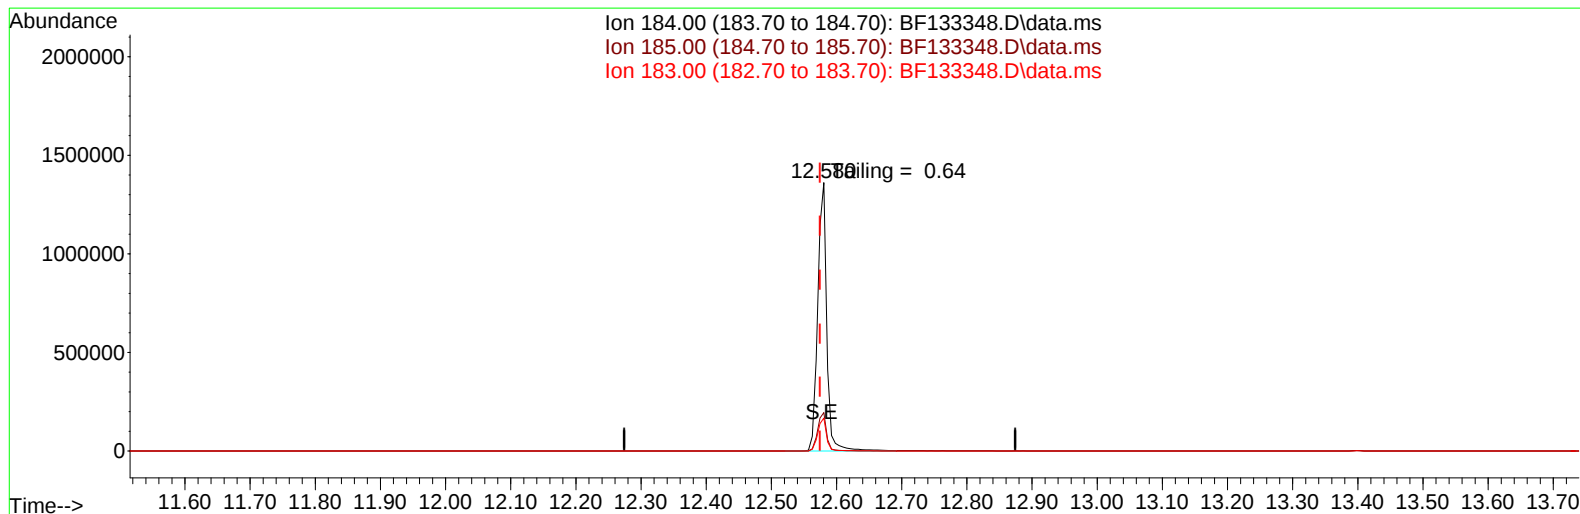

TIC: BF133348.D\data.ms

(77) Benzidine

12.580min (+ 0.006) 76771.17 ng

response 1315118

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.34#
183.00	11.70	12.27
0.00	0.00	0.00