


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051123\
 Data File : BF133348.D
 Acq On : 11 May 2023 11:17
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 11 16:40:17 2023

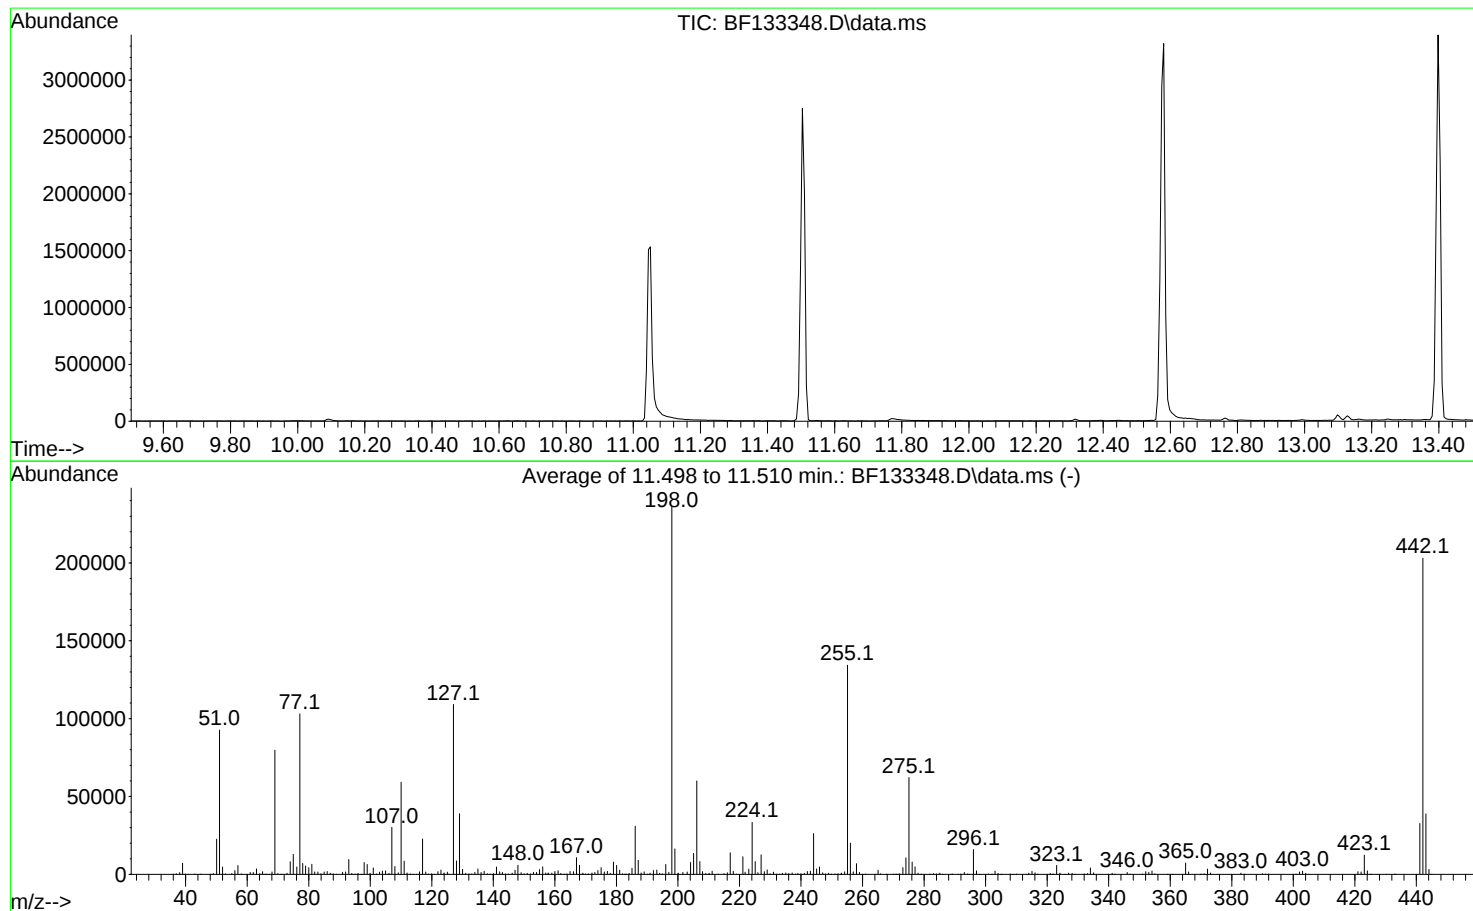

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	92712	PASS
68	69	0.00	2	2.0	1563	PASS
69	198	0.00	100	33.7	79723	PASS
70	69	0.00	2	0.7	547	PASS
127	198	10	80	46.2	109075	PASS
197	198	0.00	2	0.6	1352	PASS
198	198	100	100	100.0	236224	PASS
199	198	5	9	6.9	16344	PASS
275	198	10	60	26.3	62173	PASS
365	198	1	100	3.1	7331	PASS
441	198	0.01	100	13.8	32674	PASS
442	442	50	100	100.0	203003	PASS
443	442	15	24	19.1	38853	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/11/2023	BNA_F	<u>BF133348.D</u>
Compound Name	Response	Retention Time
DDT	574459	13.398
DDD	14528	13.098
DDE	2722	12.763
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17250	591709	2.92

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051123\
Data File : BF133348.D
Acq On : 11 May 2023 11:17
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 11 12:32:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 09 04:59:36 2023
Response via : Initial Calibration

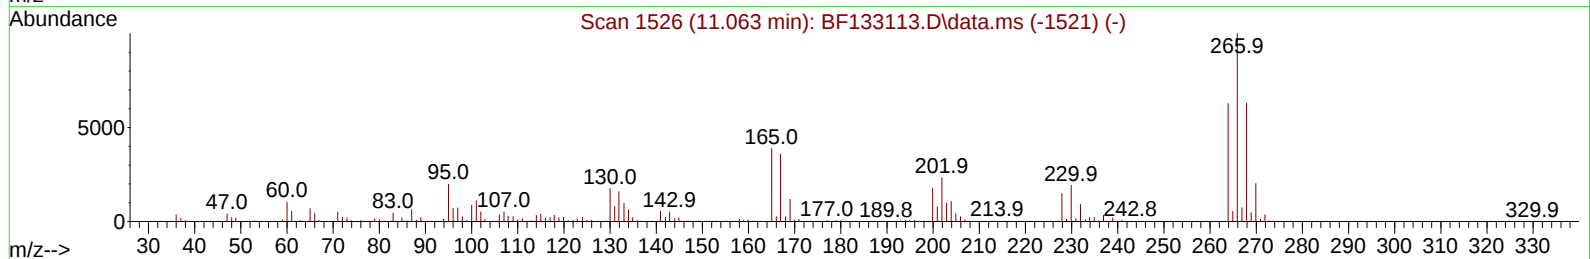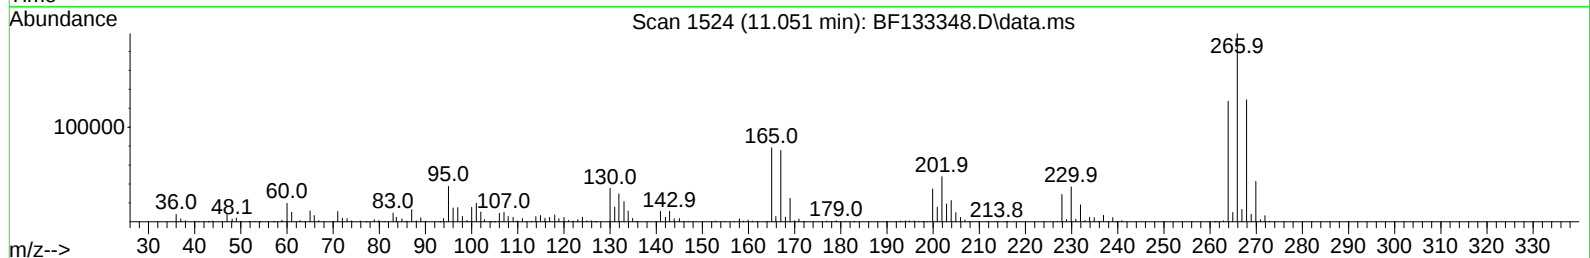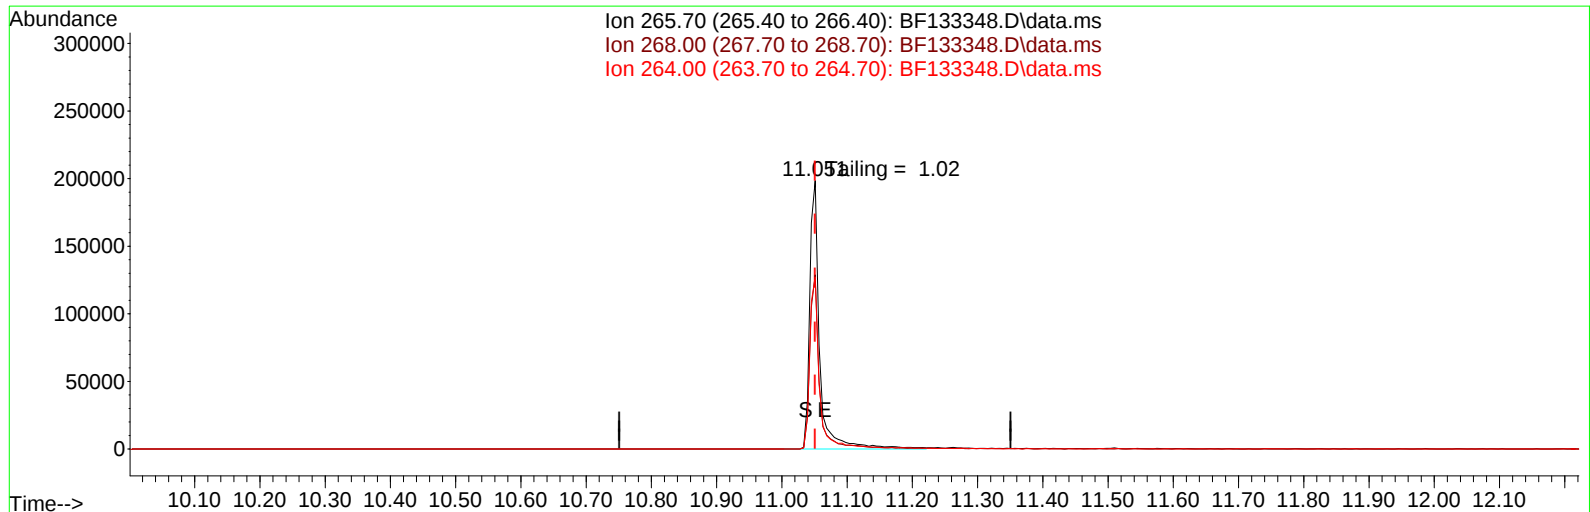

TIC: BF133348.D\data.ms

(70) Pentachlorophenol (C)

11.051min (+ 0.000) 77143.67 ng




response 212482

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	64.85
264.00	63.30	64.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051123\
 Data File : BF133348.D
 Acq On : 11 May 2023 11:17
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 11 12:32:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 09 04:59:36 2023
 Response via : Initial Calibration

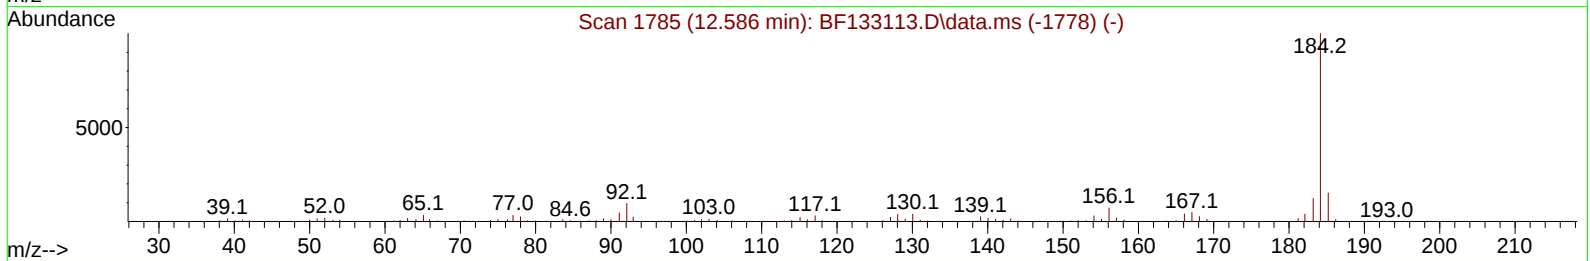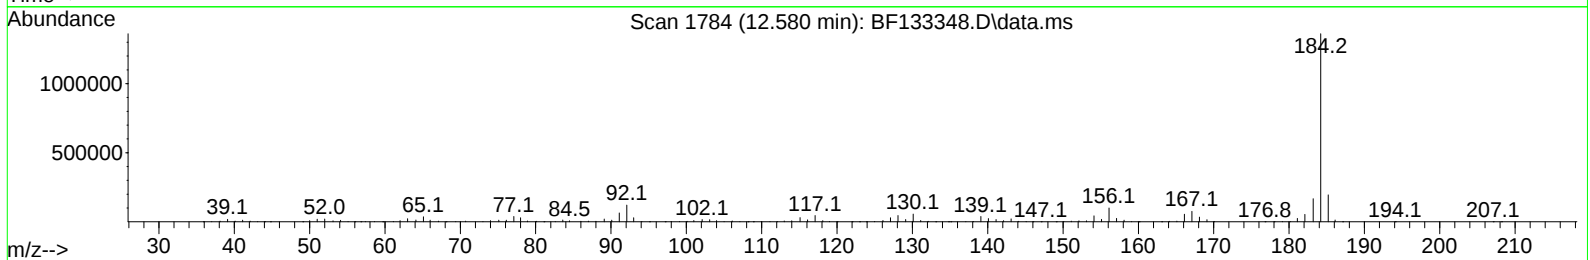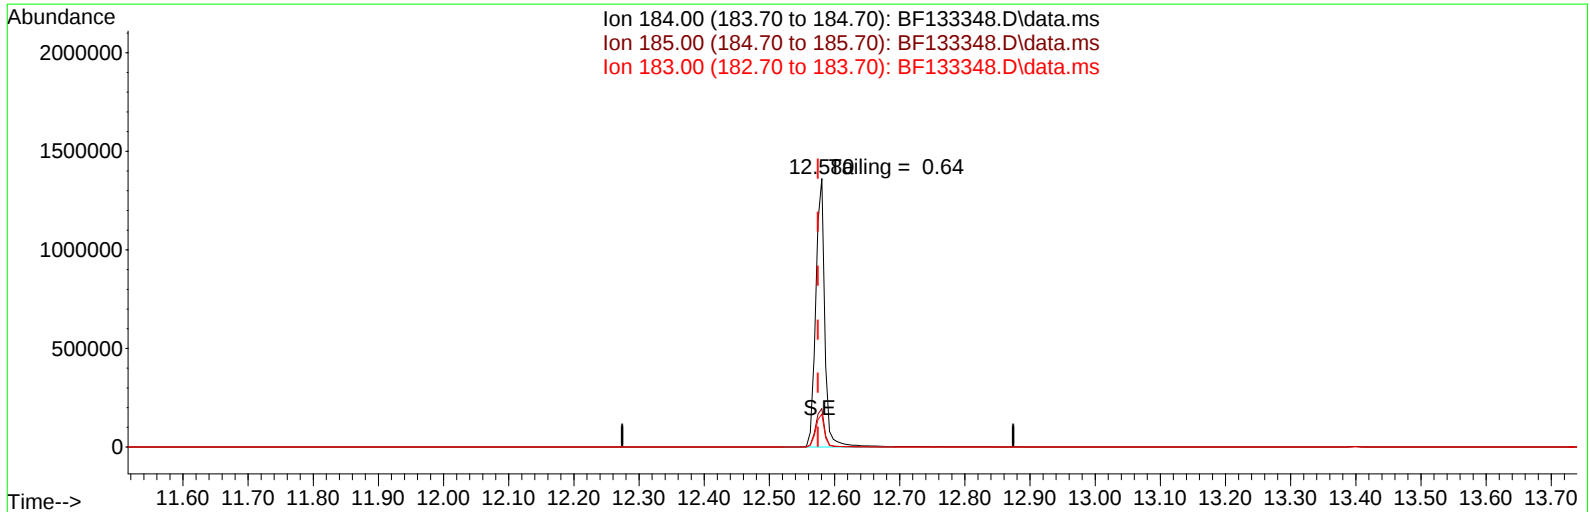

TIC: BF133348.D\data.ms

(77) Benzidine

12.580min (+ 0.006) 76771.17 ng

response 1315118

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.34#
183.00	11.70	12.27
0.00	0.00	0.00