


Data Path : Z:\HPCHEM1\BNA_F\Data\BF051215\
 Data File : BF079156.D
 Acq On : 12 May 2015 14:19
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 30 19:07:47 2015

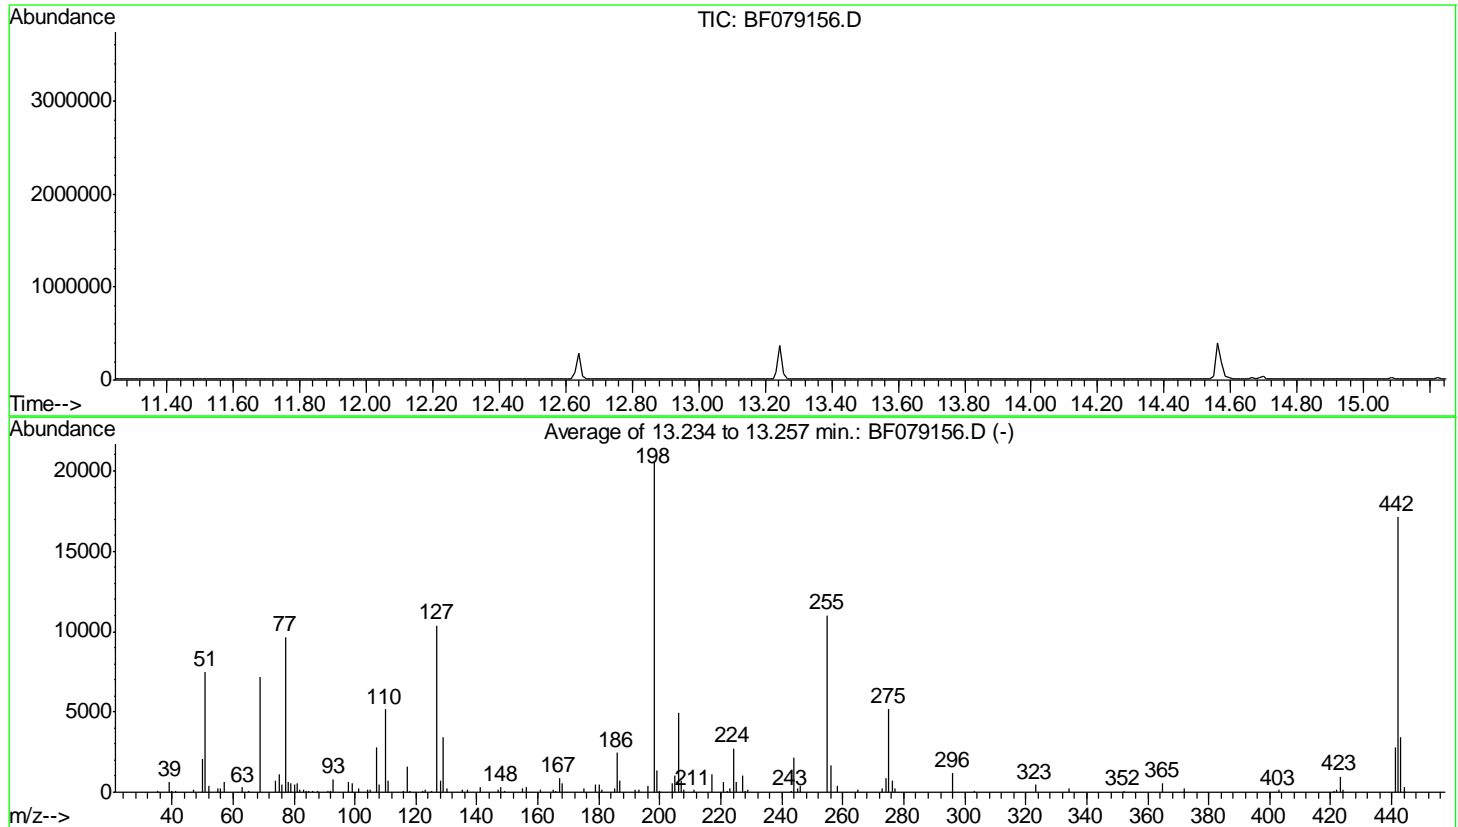

AutoFind: Scans 1054, 1055, 1056; Background Corrected with Scan 1051

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	7495	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.9	7202	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.3	10387	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	20637	PASS
199	198	5	9	6.7	1377	PASS
275	198	10	60	25.2	5192	PASS
365	198	1	100	2.8	583	PASS
441	442	0.01	24	16.0	2753	PASS
442	198	50	100	83.2	17169	PASS
443	442	15	24	20.1	3447	PASS