


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051215\
 Data File : BF079179.D
 Acq On : 13 May 2015 2:56
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 13 00:53:14 2015

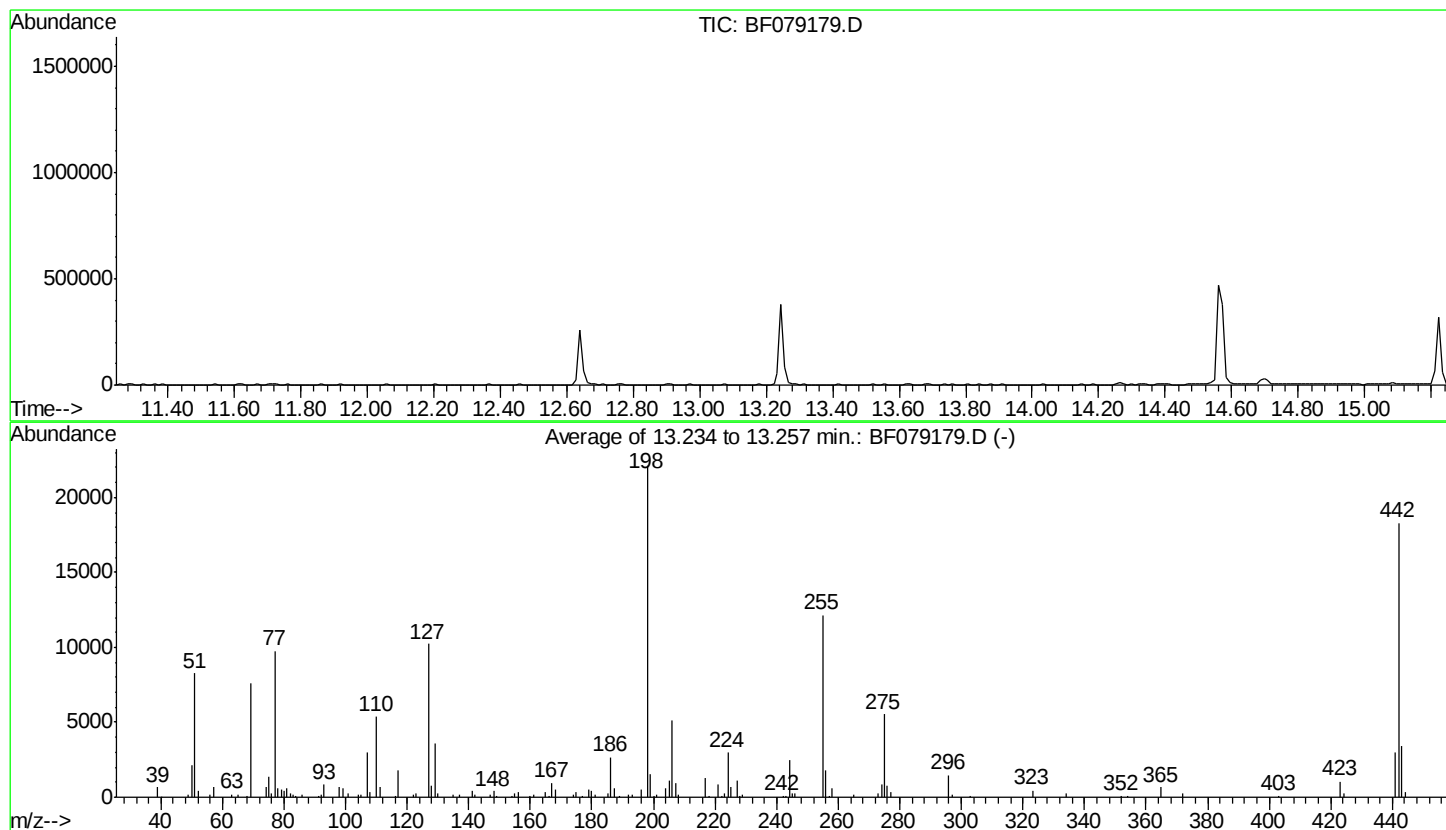

AutoFind: Scans 1054, 1055, 1056; Background Corrected with Scan 1051

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	8256	PASS
68	69	0.00	2	1.4	108	PASS
69	198	0.00	100	34.5	7630	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.2	10217	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	22124	PASS
199	198	5	9	6.9	1525	PASS
275	198	10	60	25.1	5546	PASS
365	198	1	100	3.0	672	PASS
441	442	0.01	24	16.4	2998	PASS
442	198	50	100	82.7	18286	PASS
443	442	15	24	18.7	3423	PASS