
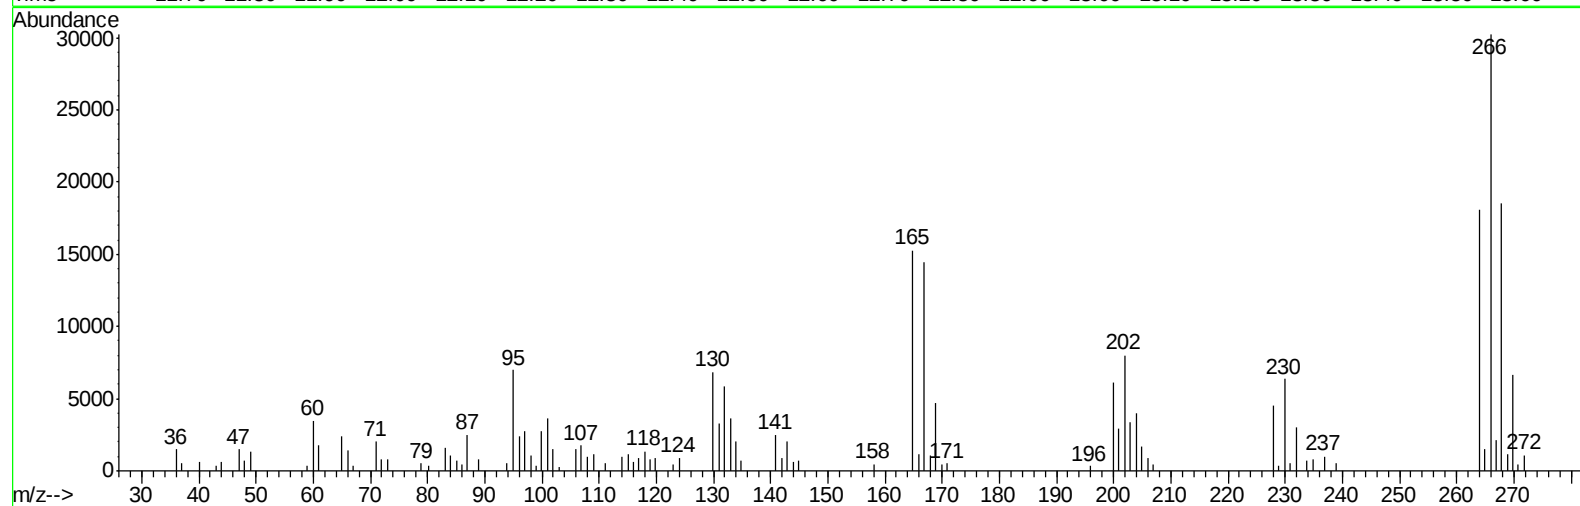


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051215\
Data File : BF079179.D
Acq On : 13 May 2015 2:56
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 13 07:38:29 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 13 04:45:03 2015
Response via : Initial Calibration

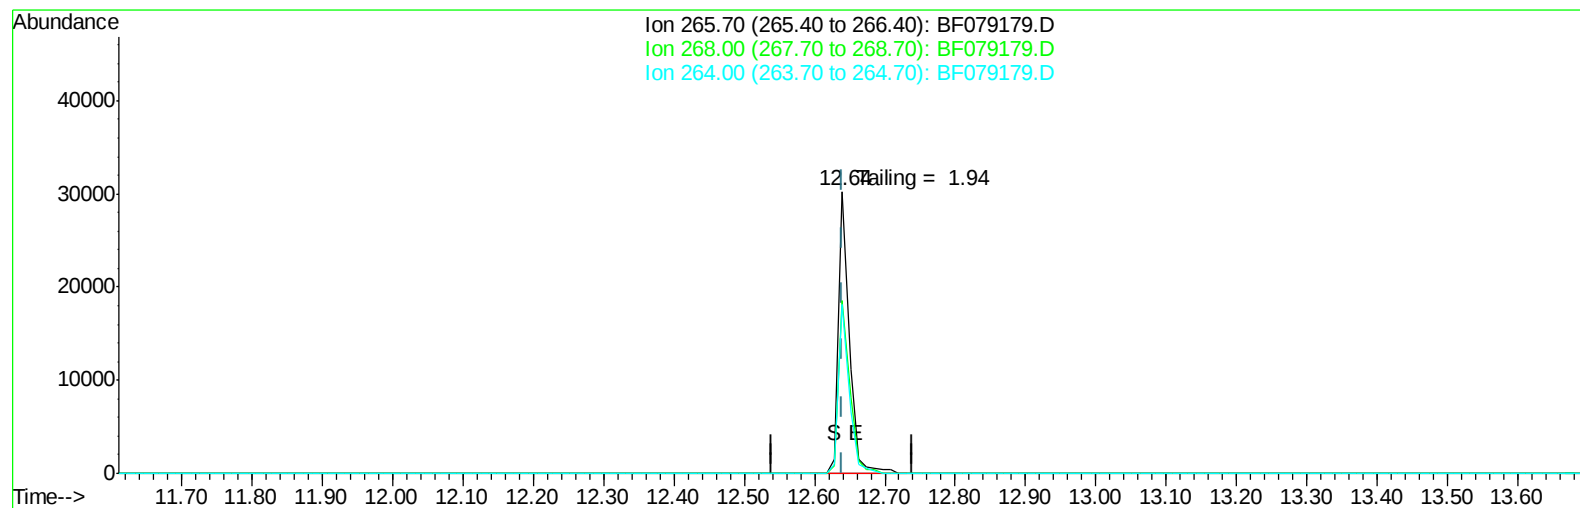

TIC: BF079179.D

(69) Pentachlorophenol (C)



12.639min (+0.000) 0.00ng

response 31571

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	61.36
264.00	60.20	59.93
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051215\
Data File : BF079179.D
Acq On : 13 May 2015 2:56
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 13 07:38:29 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 13 04:45:03 2015
Response via : Initial Calibration

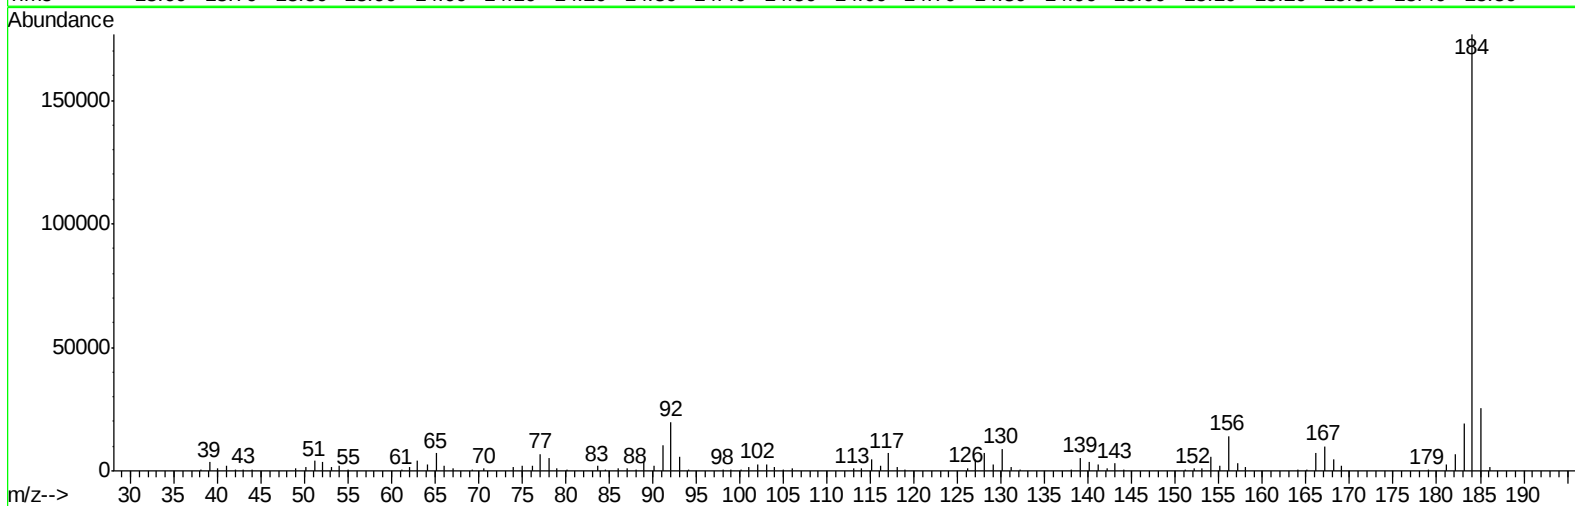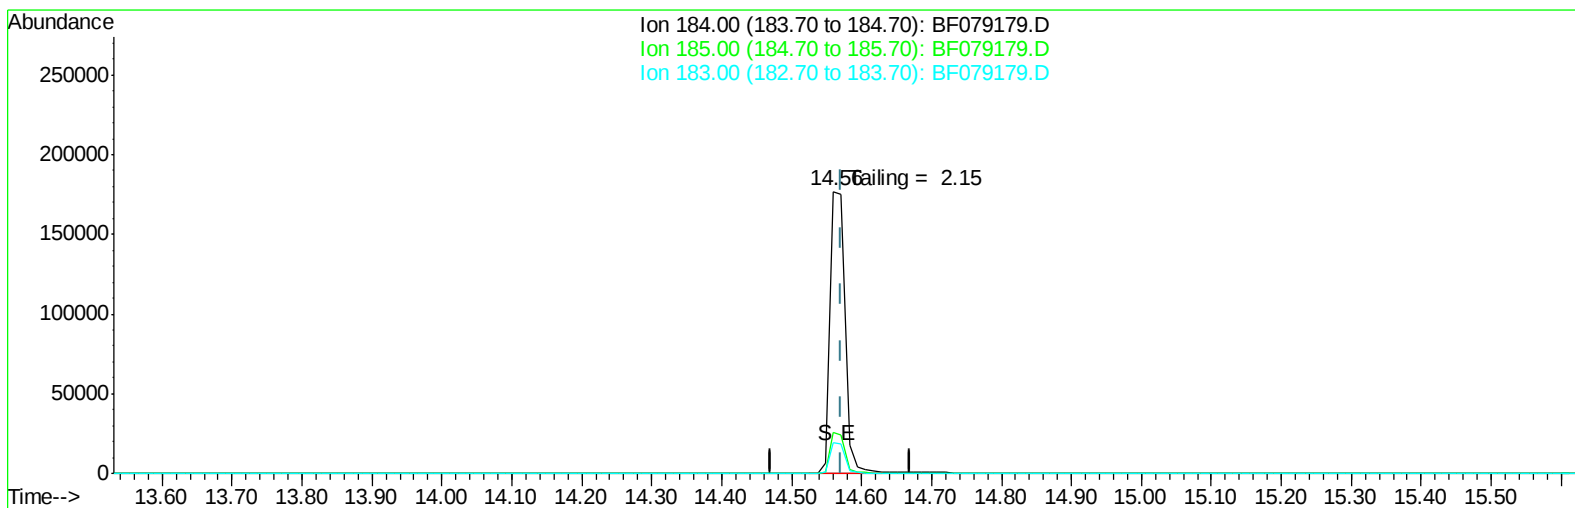

TIC: BF079179.D

(76) Benzidine

14.560min (-0.011) 21050.96ng

response 264382

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	14.51
183.00	10.50	11.01
0.00	0.00	0.00