

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051215\
 Data File : BF079186.D
 Acq On : 13 May 2015 6:45
 Operator : TP/IZ
 Sample : G2194-09
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TU021-SB-18-2.5

Quant Time: May 13 07:25:56 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF043015.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 13 04:45:03 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.28	152	56487	20.00	ng	0.00
21) Naphthalene-d8	8.86	136	230396	20.00	ng	0.00
38) Acenaphthene-d10	11.04	164	110799	20.00	ng	0.00
63) Phenanthrene-d10	12.88	188	214828	20.00	ng	0.00
75) Chrysene-d12	16.18	240	224931	20.00	ng	0.01
86) Perylene-d12	17.97	264	225632	20.00	ng	0.09
System Monitoring Compounds						
5) 2-Fluorophenol	5.59	112	568410	173.22	ng	0.00
7) Phenol-d6	6.86	99	785887	181.18	ng	0.01
23) Nitrobenzene-d5	7.98	82	440057	109.77	ng	0.00
41) 2,4,6-Tribromophenol	12.02	330	217135	181.15	ng	0.00
44) 2-Fluorobiphenyl	10.20	172	757472	95.25	ng	0.00
78) Terphenyl-d14	14.88	244	863163	91.87	ng	0.00
Target Compounds						Qvalue
49) Dimethylphthalate	10.71	163	157960	19.42	ng	100
74) Fluoranthene	14.39	202	34520	2.76	ng	96
77) Pyrene	14.66	202	46331	3.57	ng	# 95
82) Chrysene	16.22	228	24183	2.04	ng	95
87) Benzo(b)fluoranthene	17.51	252	31952m	2.59	ng	
89) Benzo(a)pyrene	17.90	252	26143	2.30	ng	# 90
91) Benzo(g,h,i)perylene	19.86	276	25042	2.07	ng	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051215\
Data File : BF079186.D
Acq On : 13 May 2015 6:45
Operator : TP/IZ
Sample : G2194-09
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TU021-SB-18-2.5

Quant Time: May 13 07:25:56 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 13 04:45:03 2015
Response via : Initial Calibration

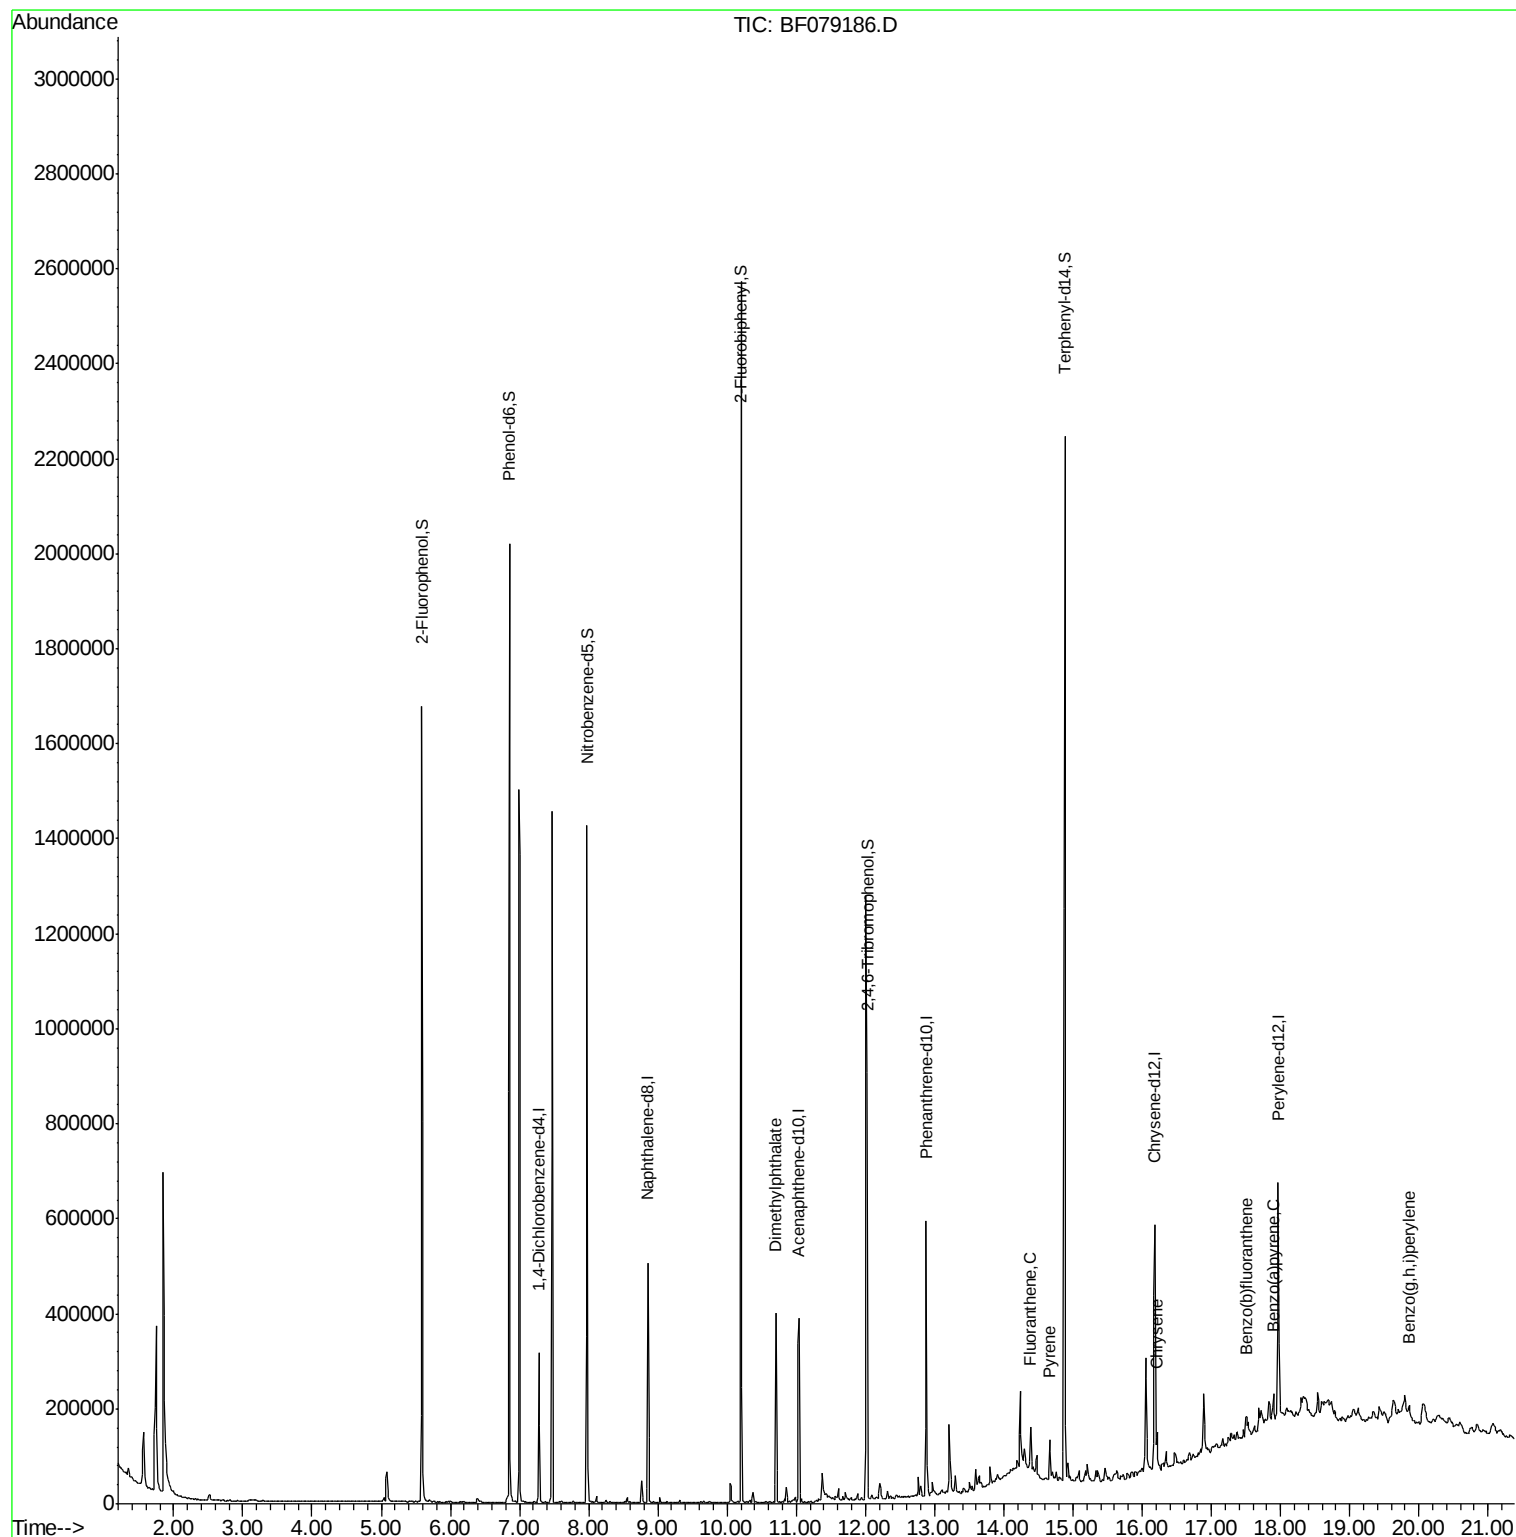


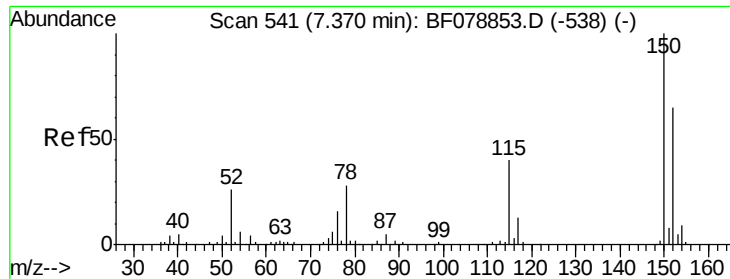




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 7.28 min Scan# 533
 Delta R.T. 0.00 min
 Lab File: BF079186.D
 Acq: 13 May 2015 6:45

Instrument :
 BNA_F
 ClientSampleId :
 TU021-SB-18-2.5

Tot Ion:152 Resp: 56487
 Ion Ratio Lower Upper
 152 100
 150 158.6 122.0 183.0
 115 64.4 46.3 69.5

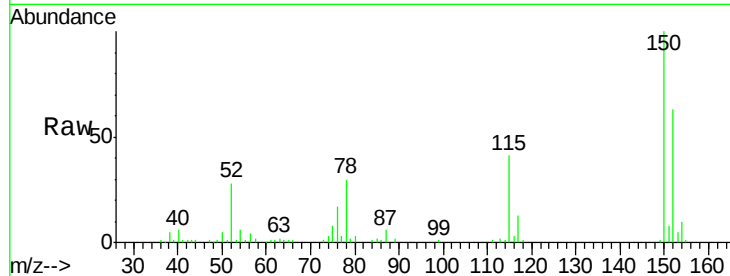


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

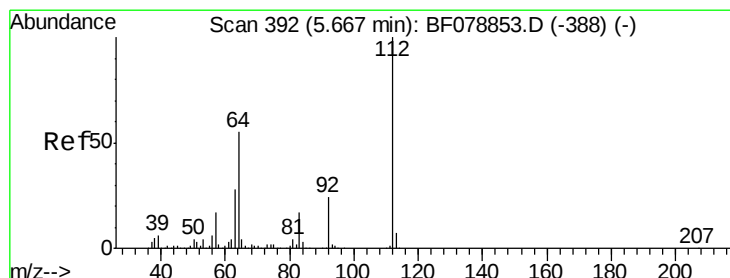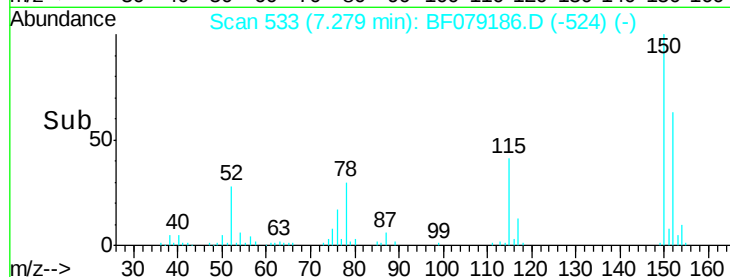
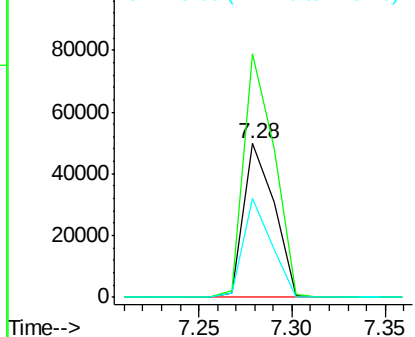


#5
 2-Fluorophenol
 Concen: 173.22 ng
 RT: 5.59 min Scan# 385
 Delta R.T. 0.00 min
 Lab File: BF079186.D
 Acq: 13 May 2015 6:45

Tgt Ion:112 Resp: 568410
 Ion Ratio Lower Upper
 112 100
 64 61.6 53.5 80.3
 63 30.5 27.5 41.3

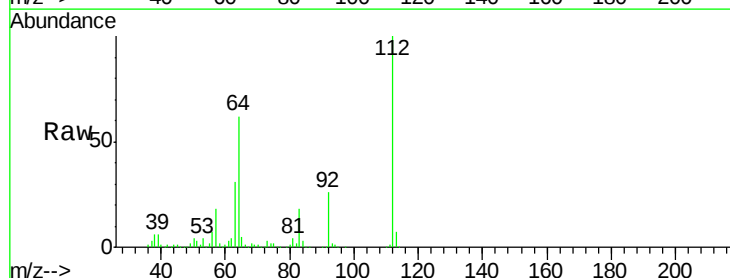

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

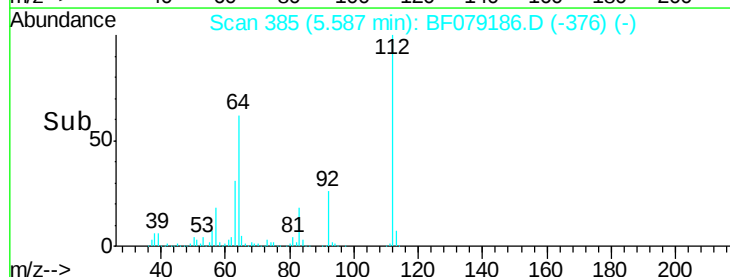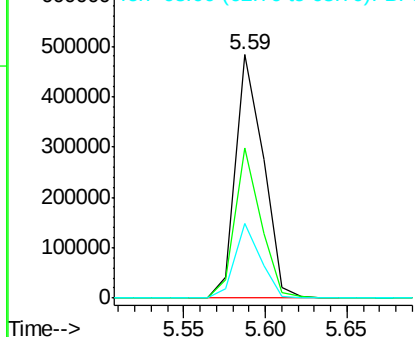



#7

Phenol-d6

Concen: 181.18 ng

RT: 6.86 min Scan# 496

Delta R.T. 0.01 min

Lab File: BF079186.D

Acq: 13 May 2015 6:45

Instrument :

BNA_F

ClientSampleId :

TU021-SB-18-2.5


Tot Ion: 99 Resp: 785887

Ion Ratio Lower Upper

99 100

42 15.4 12.8 19.2




71 28.9 23.4 35.2

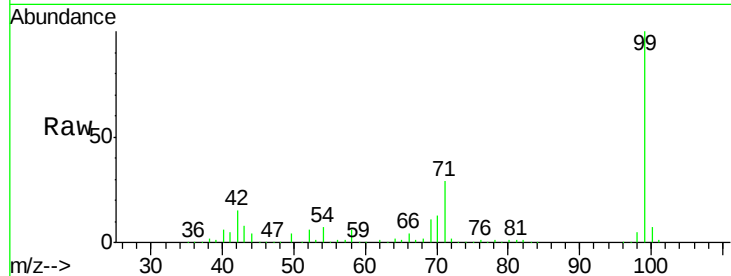

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

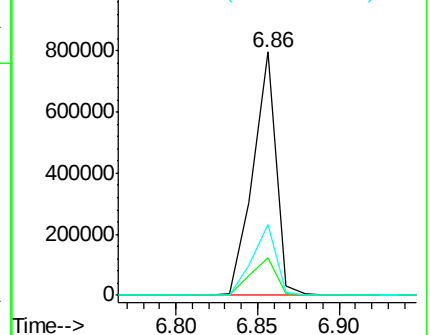

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.86 min Scan# 671

Delta R.T. 0.00 min

Lab File: BF079186.D

Acq: 13 May 2015 6:45

Tgt Ion: 136 Resp: 230396


Ion Ratio Lower Upper

136 100

137 10.9 8.7 13.1

54 8.8 5.8 8.8#

68 6.7 4.2 6.4#






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

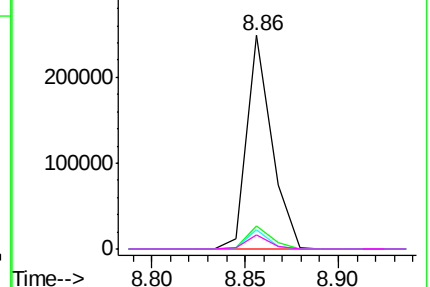

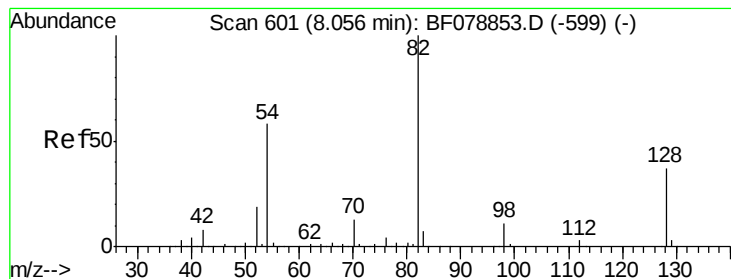

#23

Nitrobenzene-d5

Concen: 109.77 ng

RT: 7.98 min Scan# 594

Delta R.T. 0.00 min

Lab File: BF079186.D

Acq: 13 May 2015 6:45

Instrument :

BNA_F

ClientSampleId :

TU021-SB-18-2.5


Tot Ion: 82 Resp: 440057

Ion Ratio Lower Upper

82 100

128 46.2 30.0 45.0#




54 51.1 46.4 69.6



Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

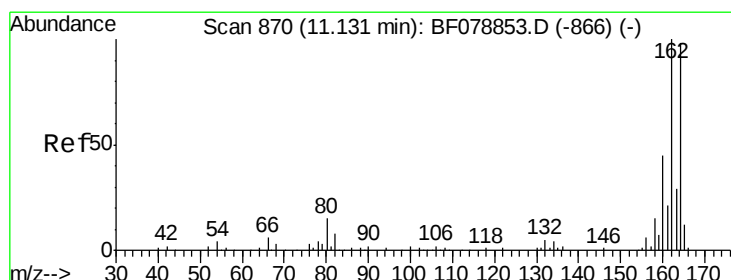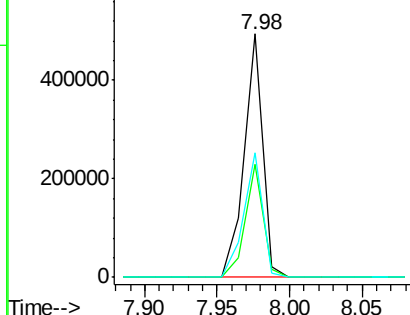

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 11.04 min Scan# 862

Delta R.T. 0.00 min

Lab File: BF079186.D

Acq: 13 May 2015 6:45


Tgt Ion:164 Resp: 110799

Ion Ratio Lower Upper

164 100

162 106.6 82.7 124.1



160 47.2 35.8 53.8




Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

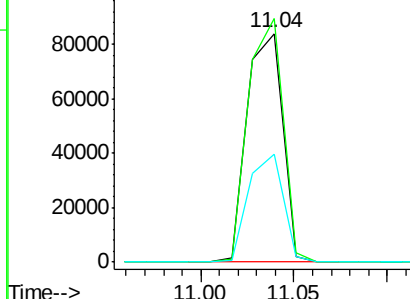




#41
 2,4,6-Tribromophenol
 Concen: 181.15 ng
 RT: 12.02 min Scan# 948
 Delta R.T. 0.00 min
 Lab File: BF079186.D
 Acq: 13 May 2015 6:45

Instrument :
 BNA_F
 ClientSampleId :
 TU021-SB-18-2.5

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.0	0.0	0.0#
141	31.1	0.0	0.0#



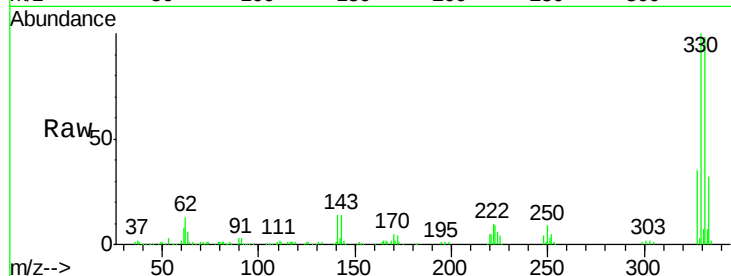


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

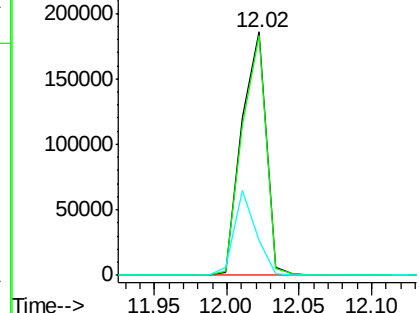

#44
 2-Fluorobiphenyl
 Concen: 95.25 ng
 RT: 10.20 min Scan# 789
 Delta R.T. 0.00 min
 Lab File: BF079186.D
 Acq: 13 May 2015 6:45

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.6	27.9	41.9
170	24.1	19.4	29.0






Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



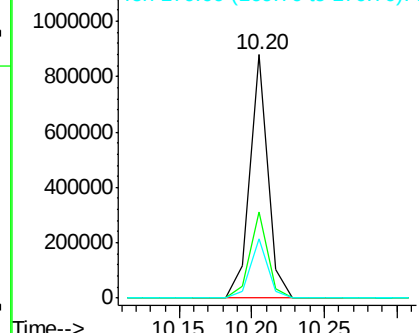



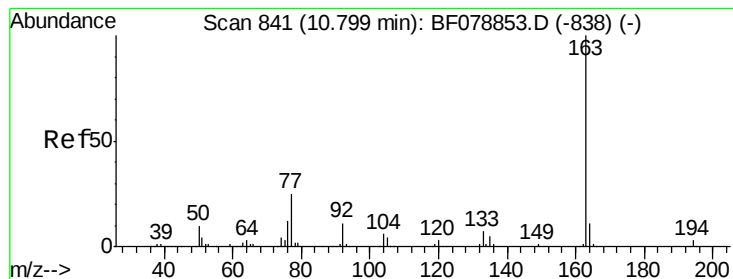

#49
Dimethylphthalate
Concen: 19.42 ng
RT: 10.71 min Scan# 833
Delta R.T. -0.01 min
Lab File: BF079186.D
Acq: 13 May 2015 6:45




Instrument :
BNA_F
ClientSampleId :
TU021-SB-18-2.5


Tot Ion:163 Resp: 157960
Ion Ratio Lower Upper
163 100
194 3.0 2.6 4.0
164 10.0 8.1 12.1

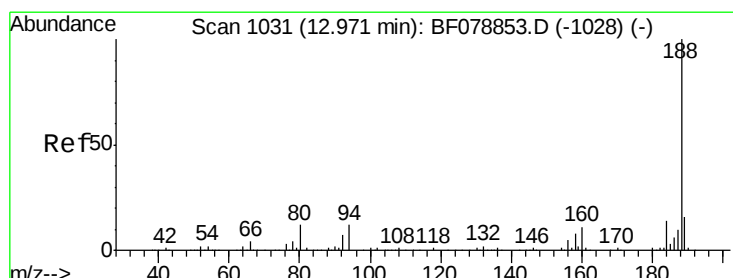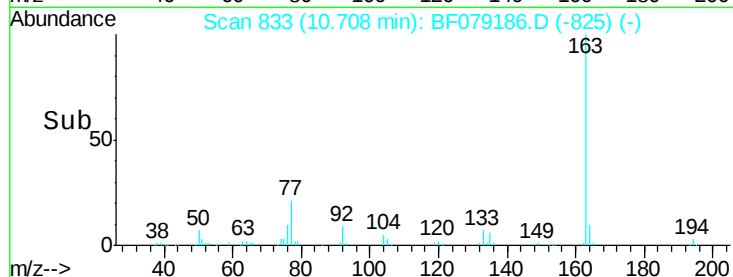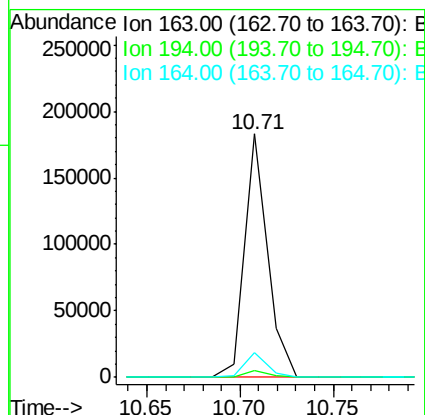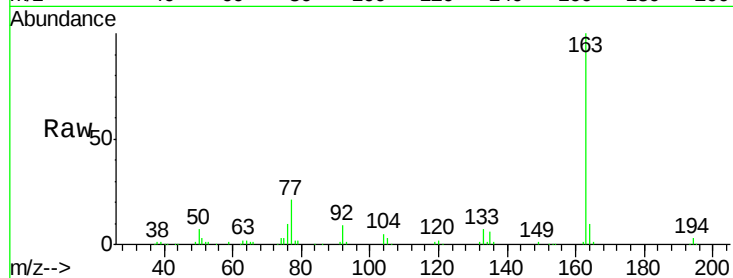

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 12.88 min Scan# 1023
Delta R.T. 0.00 min
Lab File: BF079186.D
Acq: 13 May 2015 6:45

Tgt Ion:188 Resp: 214828
Ion Ratio Lower Upper
188 100
94 10.3 8.2 12.2
80 10.5 8.9 13.3

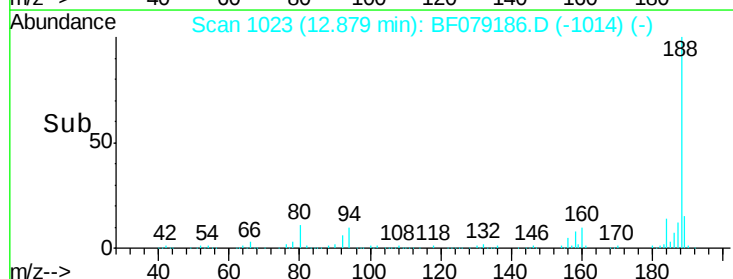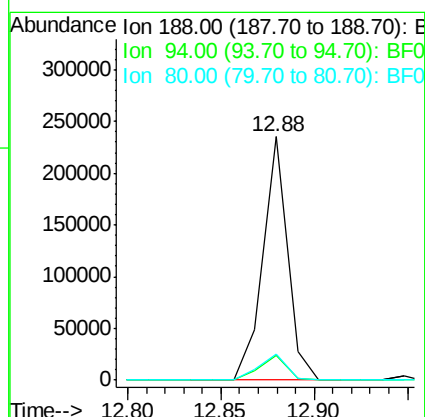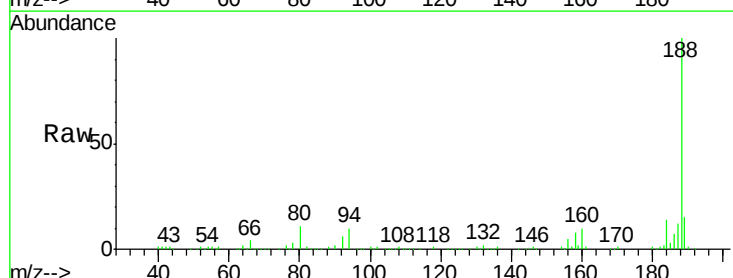



#74

Fluoranthene

Concen: 2.76 ng

RT: 14.39 min Scan# 1155

Delta R.T. 0.00 min

Lab File: BF079186.D

Acq: 13 May 2015 6:45

Instrument :

BNA_F

ClientSampleId :

TU021-SB-18-2.5


Tot Ion:202 Resp: 34520

Ion Ratio Lower Upper

202 100

101 12.4 0.0 34.6




203 17.2 0.0 38.4



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

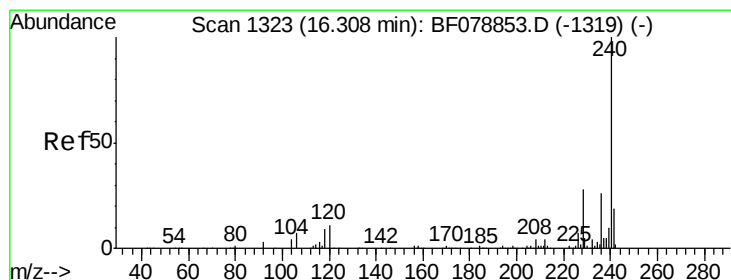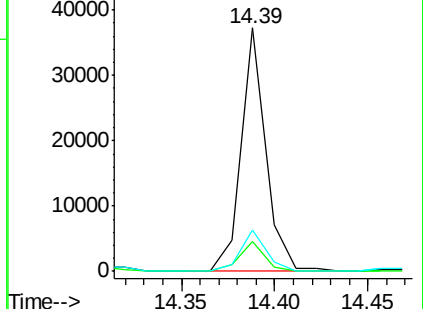

#75

Chrysene-d12

Concen: 20.00 ng

RT: 16.18 min Scan# 1312

Delta R.T. 0.01 min

Lab File: BF079186.D

Acq: 13 May 2015 6:45


Tgt Ion:240 Resp: 224931

Ion Ratio Lower Upper

240 100

120 9.9 9.7 14.5



236 25.6 20.2 30.4




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

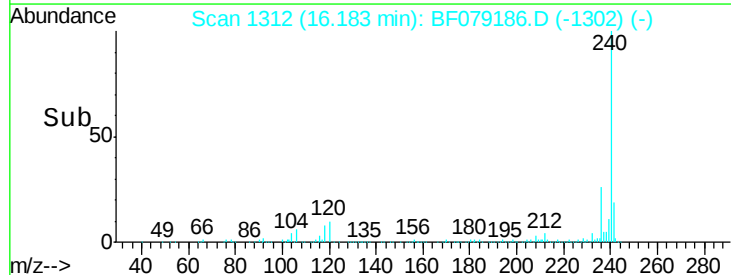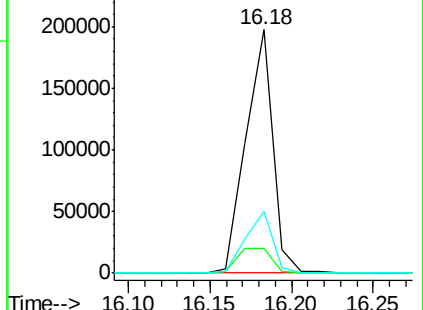





#77
Pvrene
Concen: 3.57 ng
RT: 14.66 min Scan# 1179
Delta R.T. -0.01 min
Lab File: BF079186.D
Acq: 13 May 2015 6:45

Instrument :
BNA_F
ClientSampleId :
TU021-SB-18-2.5



Tot Ion:202 Resp: 46331
Ion Ratio Lower Upper
202 100
200 21.2 17.5 26.3
203 21.6 13.9 20.9#



Abundance Ion 202.00 (201.70 to 202.70): E
Ion 200.00 (199.70 to 200.70): E
Ion 203.00 (202.70 to 203.70): E

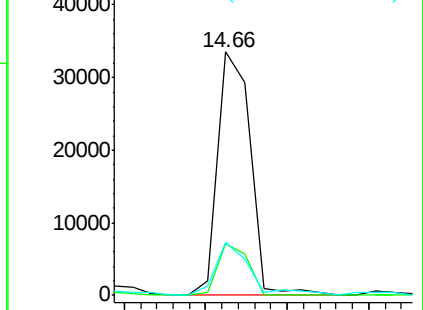


Time--> 14.60 14.65 14.70 14.75




#78
Terphenyl-d14
Concen: 91.87 ng
RT: 14.88 min Scan# 1198
Delta R.T. 0.00 min
Lab File: BF079186.D
Acq: 13 May 2015 6:45


Tgt Ion:244 Resp: 863163
Ion Ratio Lower Upper
244 100
212 6.4 5.6 8.4
122 10.2 10.3 15.5#




Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

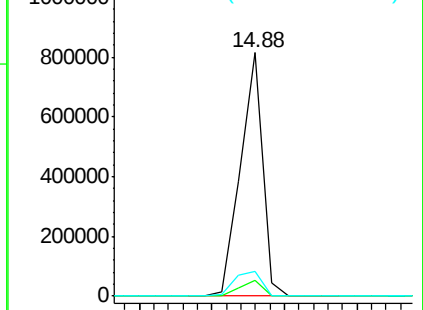

Time--> 14.80 14.85 14.90 14.95





#82

Chrysene

Concen: 2.04 ng

RT: 16.22 min Scan# 1315

Delta R.T. 0.01 min

Lab File: BF079186.D

Acq: 13 May 2015 6:45

Instrument :

BNA_F

ClientSampleId :

TU021-SB-18-2.5


Tot Ion:228 Resp: 24183

Ion Ratio Lower Upper

228 100

226 32.9 24.9 37.3




229 23.0 16.0 24.0

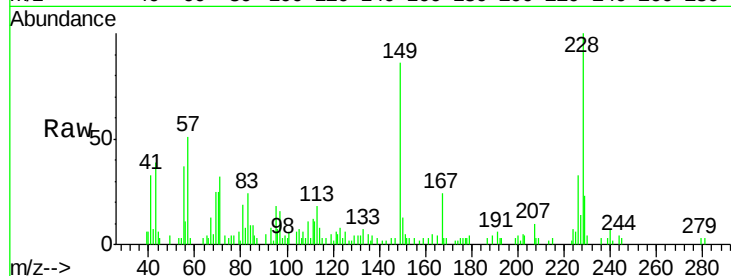

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

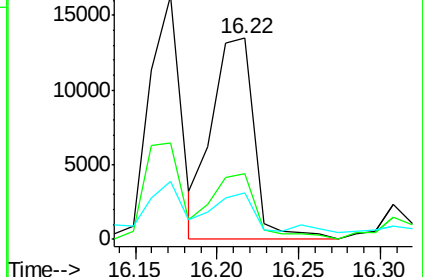

#86

Perylene-d12

Concen: 20.00 ng

RT: 17.97 min Scan# 1468

Delta R.T. 0.09 min

Lab File: BF079186.D

Acq: 13 May 2015 6:45


Tgt Ion:264 Resp: 225632

Ion Ratio Lower Upper

264 100

260 24.7 19.4 29.2



265 22.5 18.3 27.5




Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E



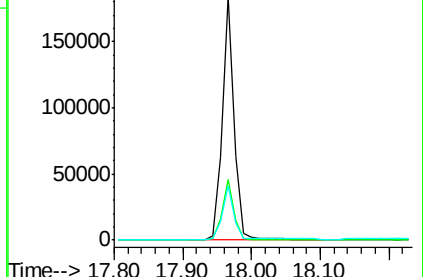



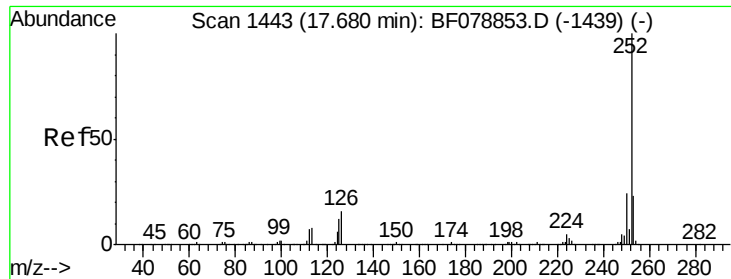

#87
Benzo(b)fluoranthene
Concen: 2.59 ng
RT: 17.51 min Scan# 1428
Delta R.T. 0.07 min
Lab File: BF079186.D
Acq: 13 May 2015 6:45




Instrument :
BNA_F
ClientSampleId :
TU021-SB-18-2.5


Tot Ion:252 Resp: 31952
Ion Ratio Lower Upper
252 100
253 24.2 17.7 26.5
125 18.6 9.5 14.3#

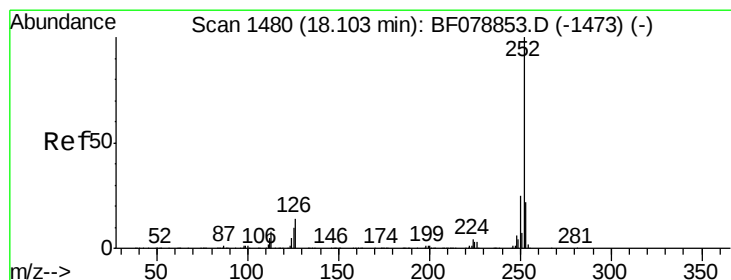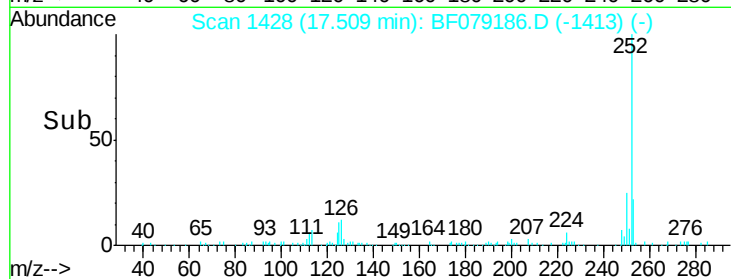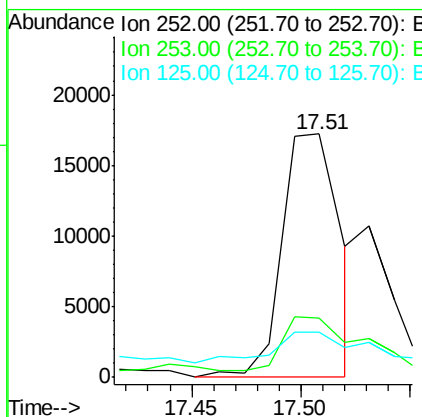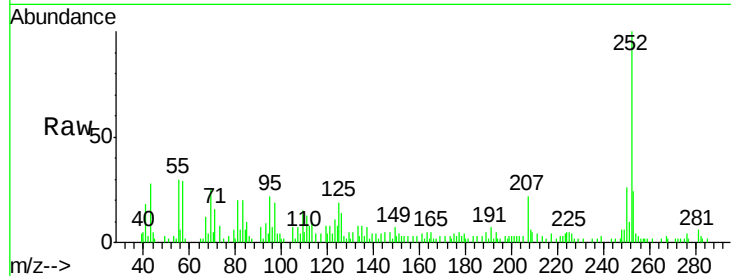

#89
Benzo(a)pyrene
Concen: 2.30 ng
RT: 17.90 min Scan# 1462
Delta R.T. 0.09 min
Lab File: BF079186.D
Acq: 13 May 2015 6:45

Tgt Ion:252 Resp: 26143
Ion Ratio Lower Upper
252 100
253 23.3 17.3 25.9
125 17.5 7.0 10.6#

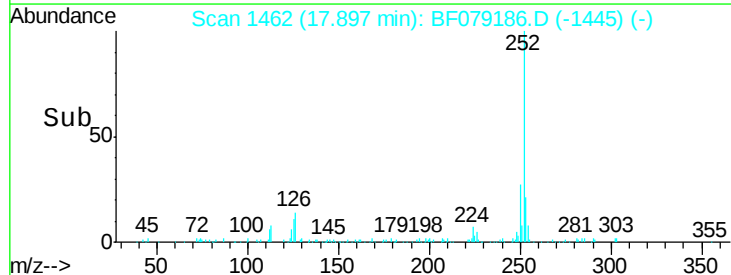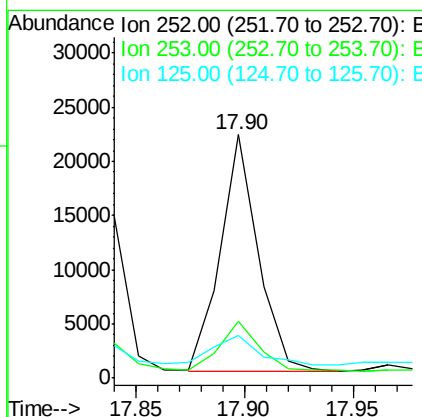

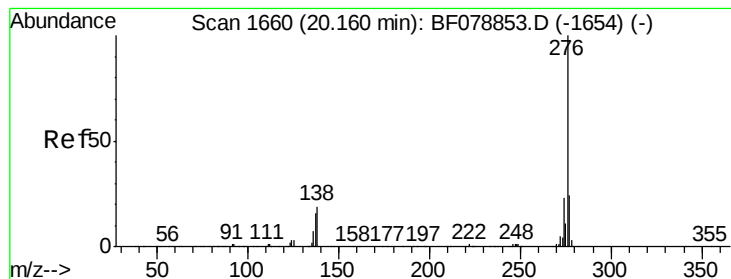

#91

Benzo(a,h,i)perylene

Concen: 2.07 ng

RT: 19.86 min Scan# 1634

Delta R.T. 0.09 min

Lab File: BF079186.D

Acq: 13 May 2015 6:45

Instrument :

BNA_F

ClientSampleId :

TU021-SB-18-2.5


Tot Ion: 276 Resp: 25042

Ion Ratio Lower Upper

276 100

277 27.1 18.6 28.0

138 24.1 17.4 26.0



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

