

Data Path : Z:\HPCHEM1\BNA F\Data\BF051216\
 Data File : BF086969.D
 Acq On : 13 May 2016 12:01
 Operator : UM/SJ
 Sample : H2916-03RE
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: May 13 14:53:21 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 09 16:04:56 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ng	-6.69
21) Naphthalene-d8	7.91	136	544141	20.00	ng	-0.08
38) Acenaphthene-d10	9.66	164	216400	20.00	ng	-0.08
63) Phenanthrene-d10	11.13	188	320111	20.00	ng	-0.08
75) Chrysene-d12	13.76	240	311128	20.00	ng	-0.08
86) Perylene-d12	15.12	264	247186	20.00	ng	-0.09
System Monitoring Compounds						
5) 2-Fluorophenol	5.22	112	1023225	0.00	ng	-0.07
7) Phenol-d6	6.28	99	1232904	0.00	ng	-0.08
23) Nitrobenzene-d5	7.20	82	923554	85.22	ng	-0.07
41) 2,4,6-Tribromophenol	10.44	330	192415	83.99	ng	-0.08
44) 2-Fluorobiphenyl	8.99	172	1303498	101.24	ng	-0.07
78) Terphenyl-d14	12.72	244	896685	61.15	ng	-0.08
Target Compounds						
25) Isophorone	7.20	82	911438	45.33	ng	# 68
49) Dimethylphthalate	9.39	163	155352	9.41	ng	# 98
56) 2,4-Dinitrotoluene	9.66	165	28386	6.60	ng	# 16
66) 4-Bromophenyl-phenylether	10.44	248	12411	3.82	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\Data\BF051216\
Data File : BF086969.D
Acq On : 13 May 2016 12:01
Operator : UM/SJ
Sample : H2916-03RE
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: May 13 14:53:21 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 09 16:04:56 2016
Response via : Initial Calibration

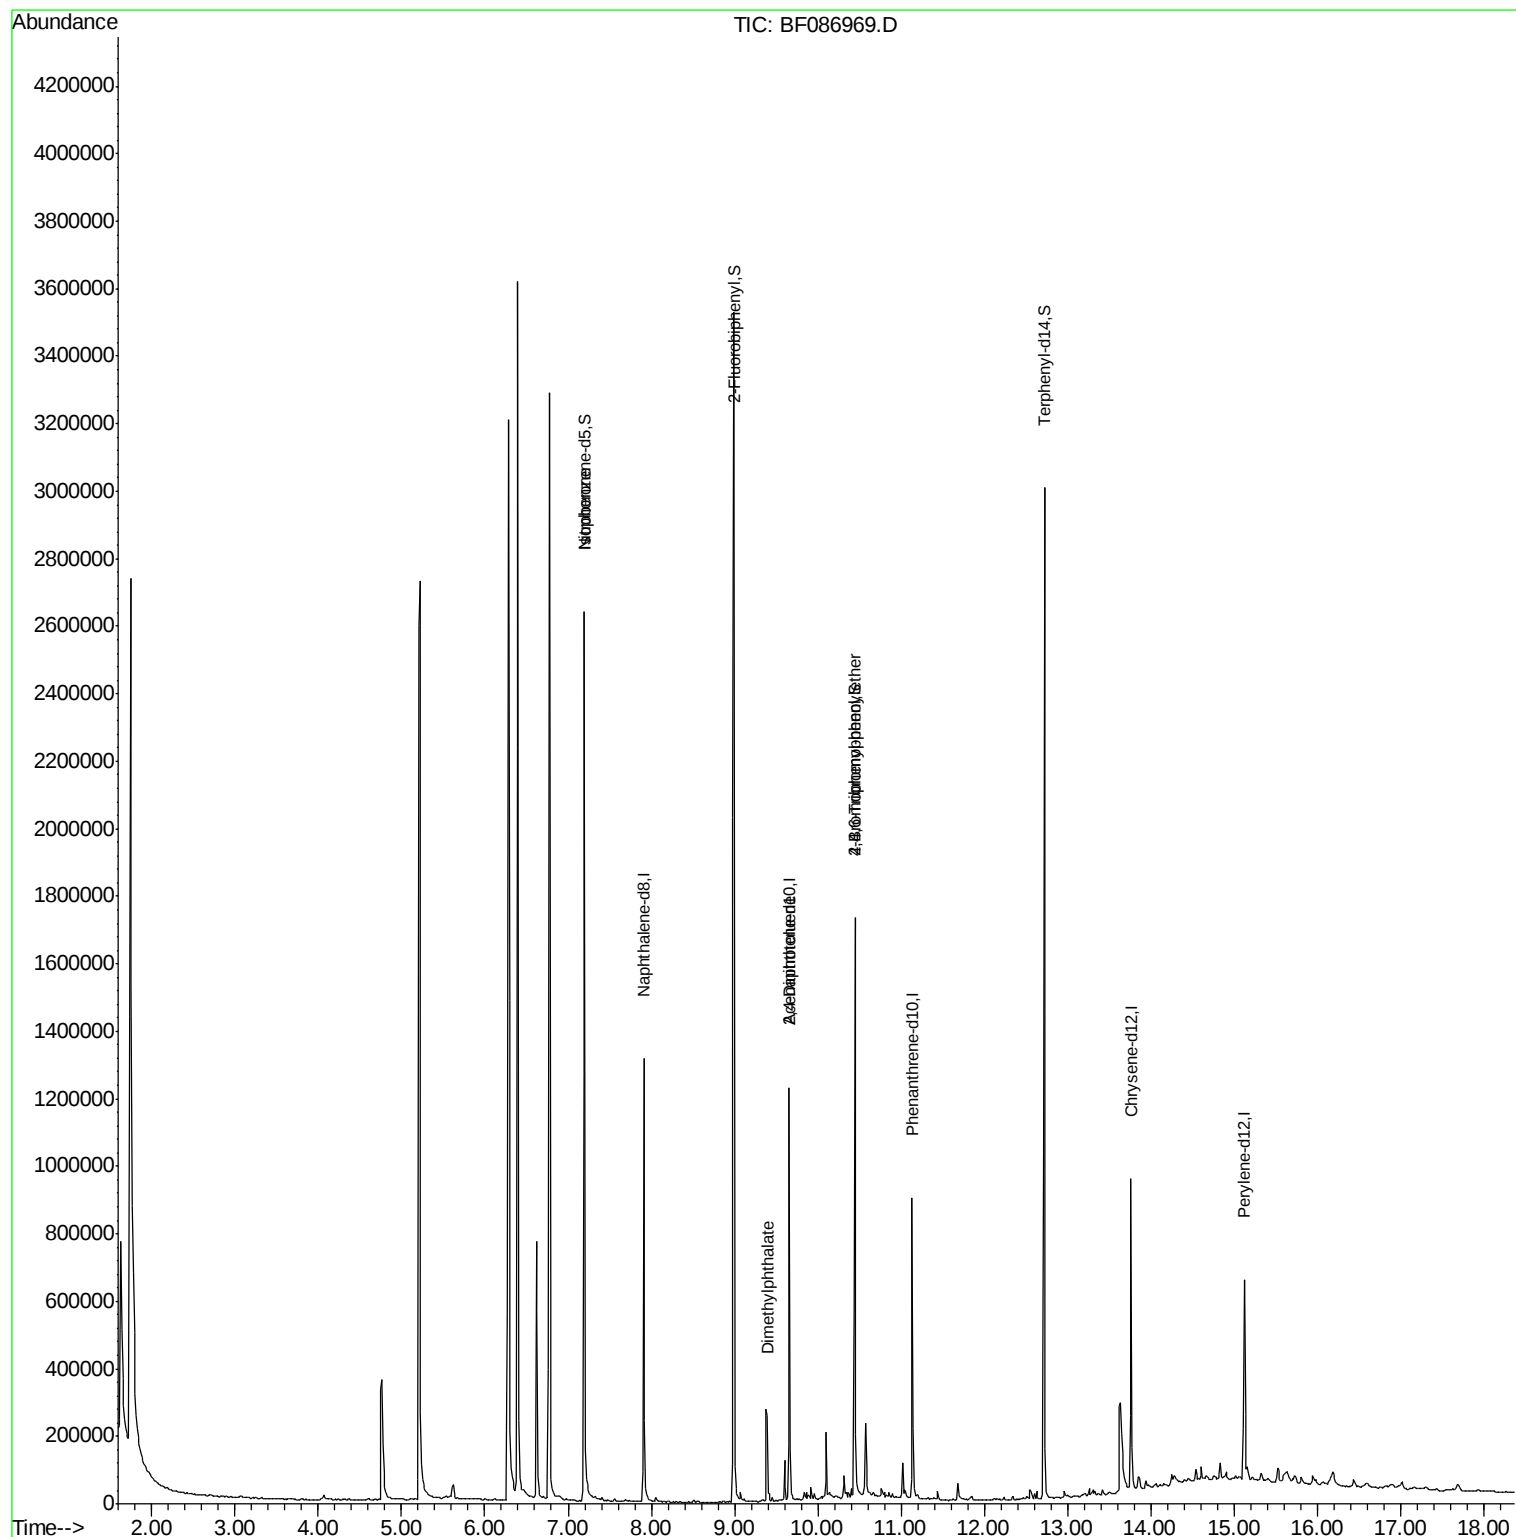

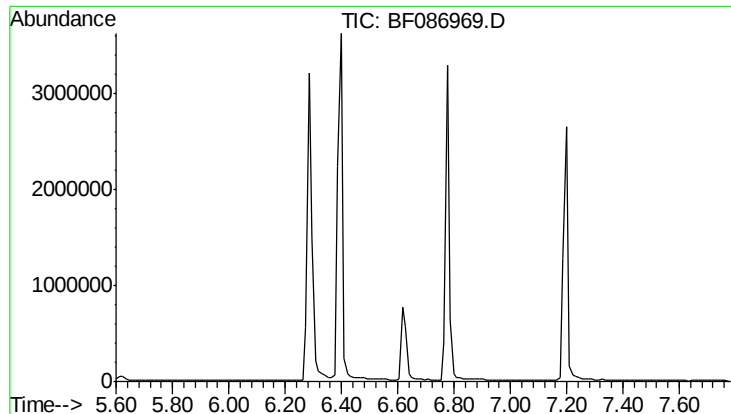

#1

1,4-Dichlorobenzene-d4

Concen: 0.00 ng

Expected RT: 6.69 min

Lab File: BF086969.D

Acq: 13 May 2016 12:01

Instrument :

BNA_F

ClientSampleId :



Tot Ion: 152

Sig Exp Ratio

152 100

150 157.2

115 64.4

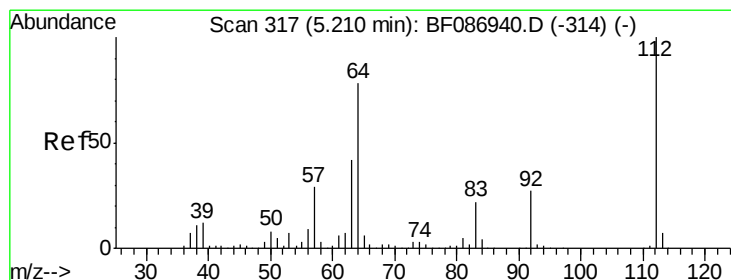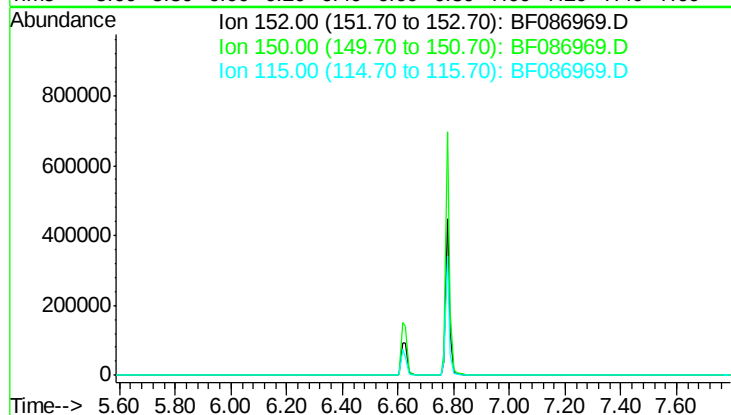

#5

2-Fluorophenol

Concen: 0.00 ng

RT: 5.22 min Scan# 318

Delta R.T. -0.07 min

Lab File: BF086969.D

Acq: 13 May 2016 12:01




Tgt Ion:112 Resp: 1023225

Ion Ratio Lower Upper

112 100

64 61.4 52.1 78.1

63 33.6 25.7 38.5

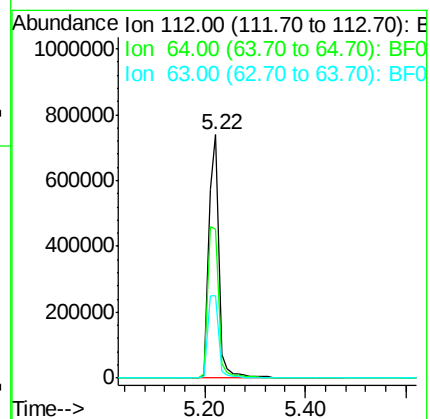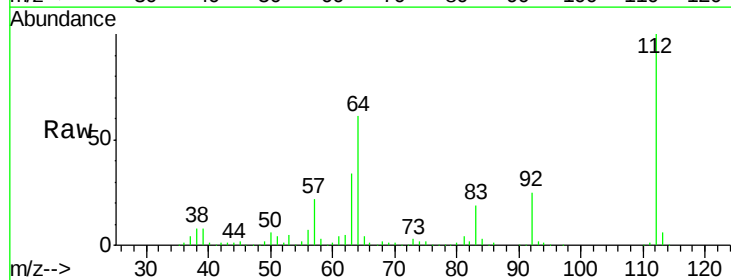



#7

Phenol-d6

Concen: 0.00 ng

RT: 6.28 min Scan# 411

Delta R.T. -0.08 min

Lab File: BF086969.D

Acq: 13 May 2016 12:01


Instrument :

BNA_F




ClientSampleId :

Tot Ion: 99 Resp: 1232904

Ion	Ratio	Lower	Upper
99	100		
42	31.4	13.6	20.4#
71	39.3	24.6	36.8#

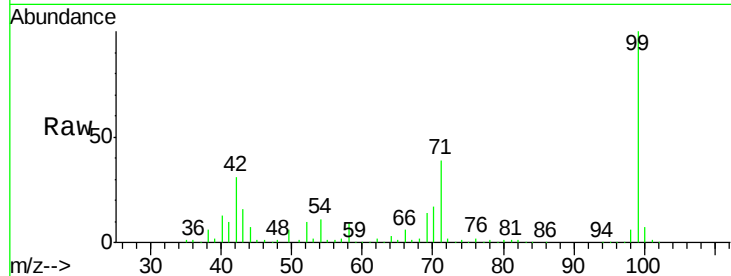

Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

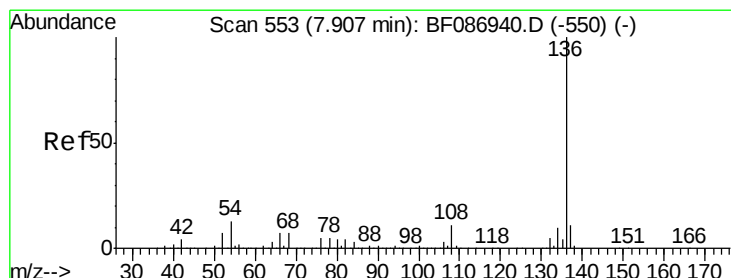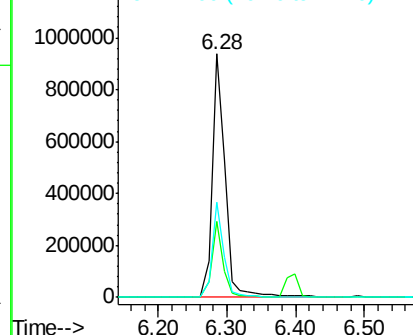

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.91 min Scan# 553


Delta R.T. -0.08 min

Lab File: BF086969.D



Acq: 13 May 2016 12:01


Tgt Ion: 136 Resp: 544141

Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.8	13.2
54	13.7	5.0	7.4#
68	7.1	4.4	6.6#

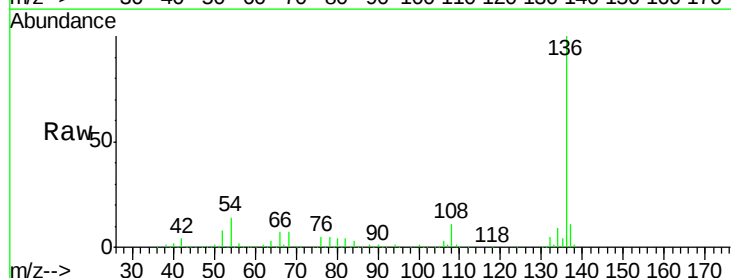

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0




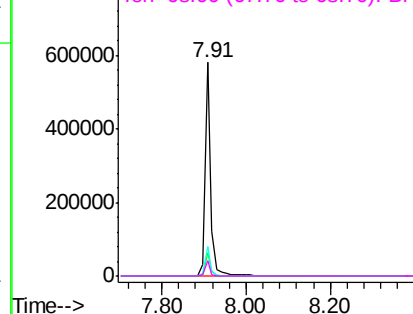




#23
 Nitrobenzene-d5
 Concen: 85.22 ng
 RT: 7.20 min Scan# 491
 Delta R.T. -0.07 min
 Lab File: BF086969.D
 Acq: 13 May 2016 12:01




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion	82	Resp	923554
Ion Ratio	100	Lower	Upper
128	41.3	40.6	61.0
54	67.0	38.1	57.1#

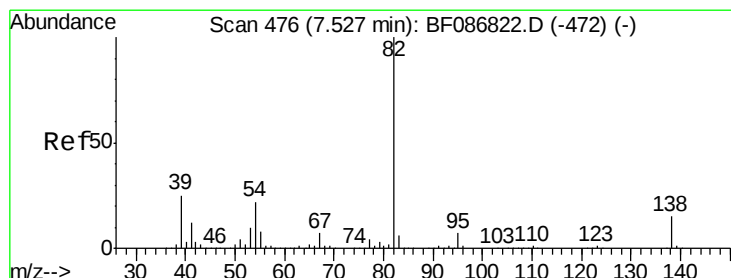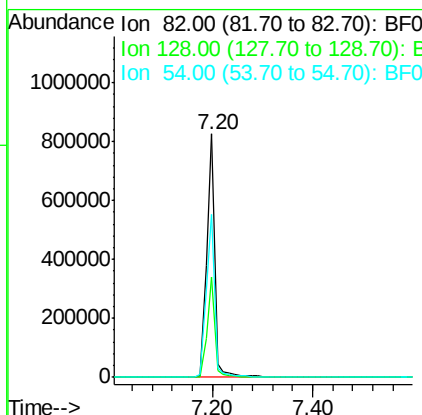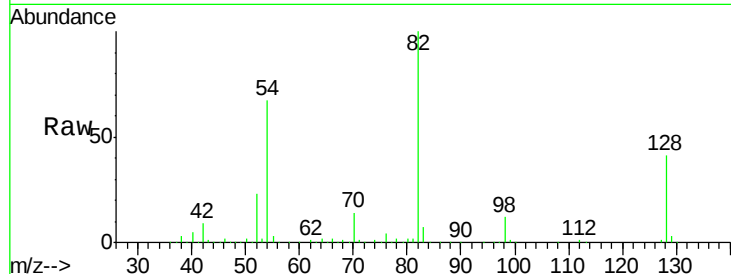

#25
 Isophorone
 Concen: 45.33 ng
 RT: 7.20 min Scan# 491
 Delta R.T. -0.33 min
 Lab File: BF086969.D
 Acq: 13 May 2016 12:01

Tgt Ion	82	Resp	911438
Ion Ratio	100	Lower	Upper
95	0.0	5.1	7.7#
138	0.0	12.4	18.6#

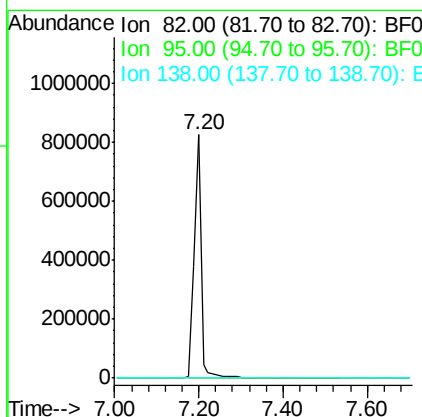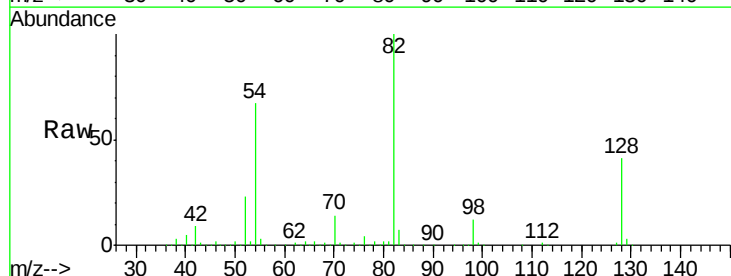


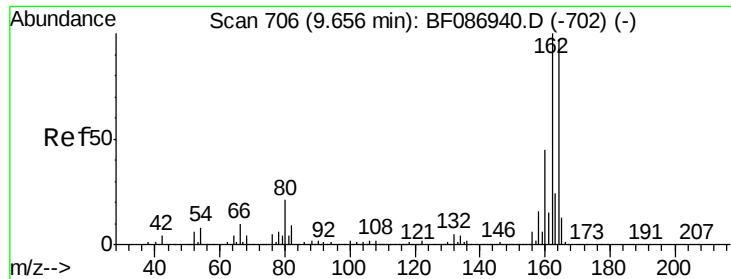




#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.66 min Scan# 706
Delta R.T. -0.08 min
Lab File: BF086969.D
Acq: 13 May 2016 12:01

Instrument :
BNA_F
ClientSampleId :

Tot Ion:164 Resp: 216400
Ion Ratio Lower Upper
164 100
162 102.7 82.8 124.2
160 47.1 36.9 55.3

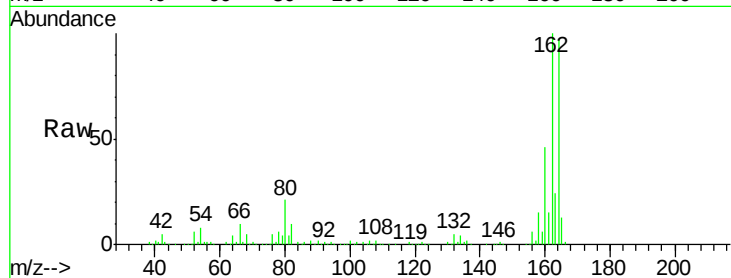


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

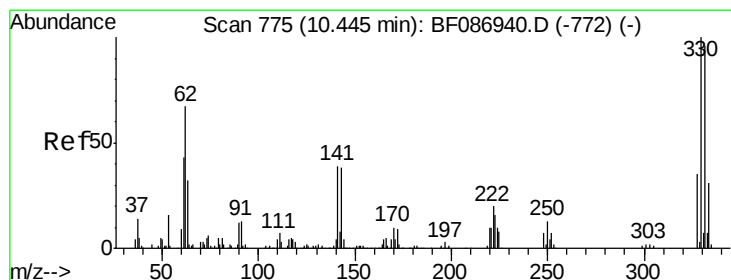
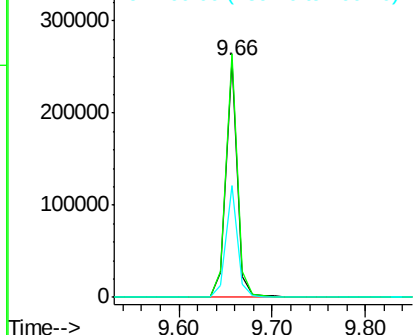



#41
2,4,6-Tribromophenol
Concen: 83.99 ng
RT: 10.44 min Scan# 775
Delta R.T. -0.08 min
Lab File: BF086969.D
Acq: 13 May 2016 12:01

Tgt Ion:330 Resp: 192415
Ion Ratio Lower Upper
330 100
332 95.3 79.0 118.4
141 39.6 31.2 46.8

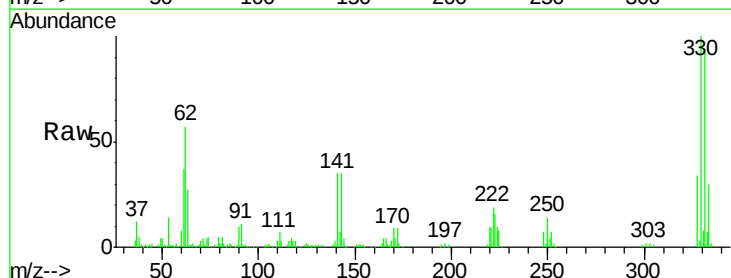

Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

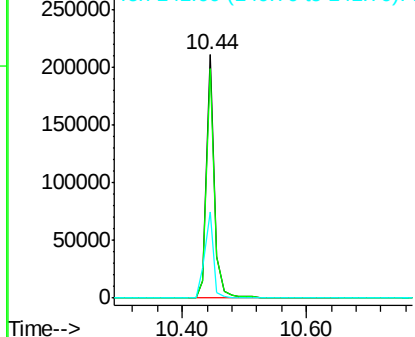




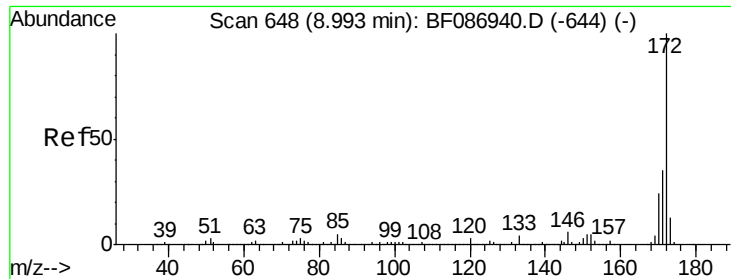


#44
 2-Fluorobiphenyl
 Concen: 101.24 ng
 RT: 8.99 min Scan# 648
 Delta R.T. -0.07 min
 Lab File: BF086969.D
 Acq: 13 May 2016 12:01

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:172 Resp: 1303498




Ion	Ratio	Lower	Upper
172	100		
171	36.5	29.0	43.6
170	24.4	19.8	29.8

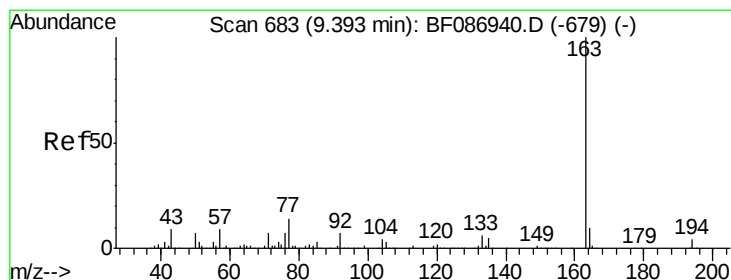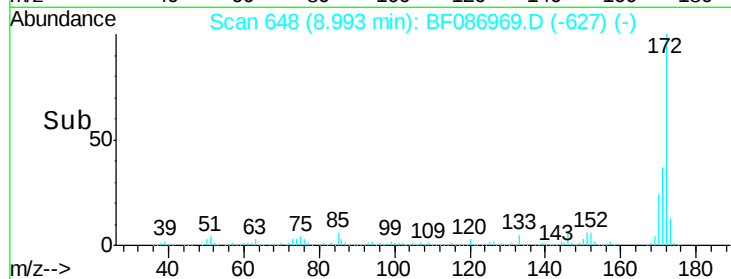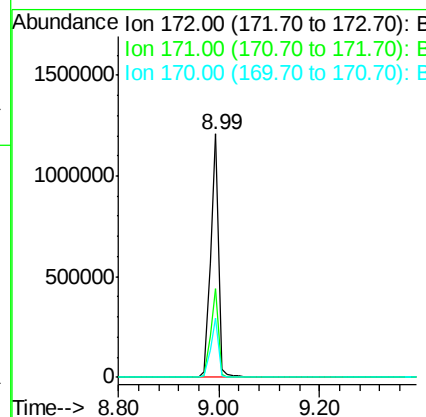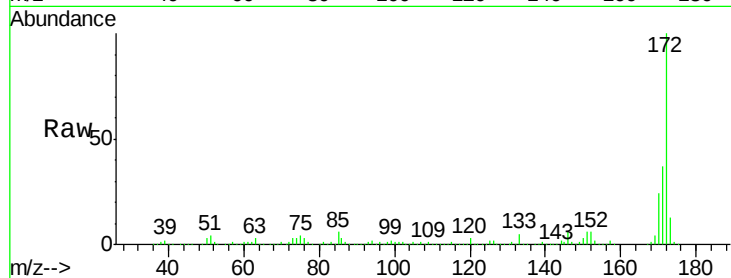


#49
 Dimethylphthalate
 Concen: 9.41 ng
 RT: 9.39 min Scan# 683
 Delta R.T. -0.08 min
 Lab File: BF086969.D
 Acq: 13 May 2016 12:01

Tgt Ion:163 Resp: 155352

Ion	Ratio	Lower	Upper
163	100		
194	3.6	2.6	4.0
164	9.3	8.2	12.4

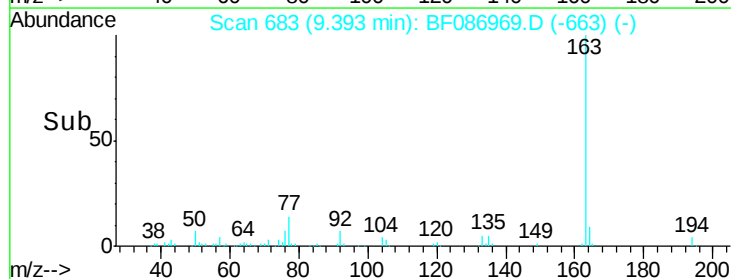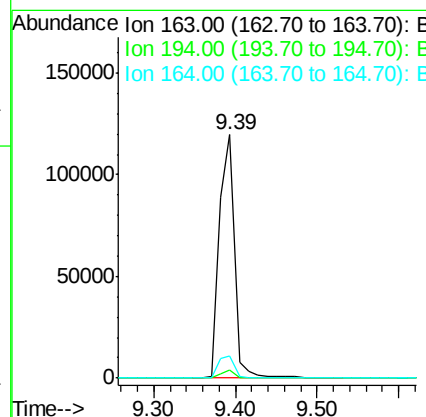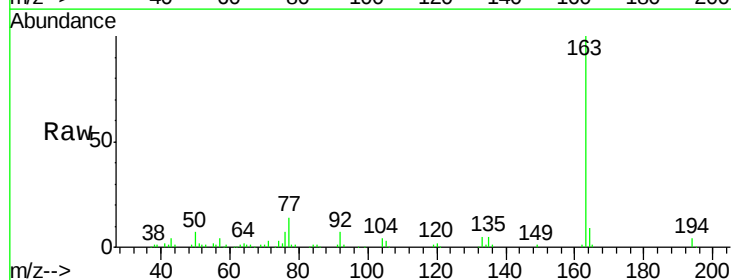


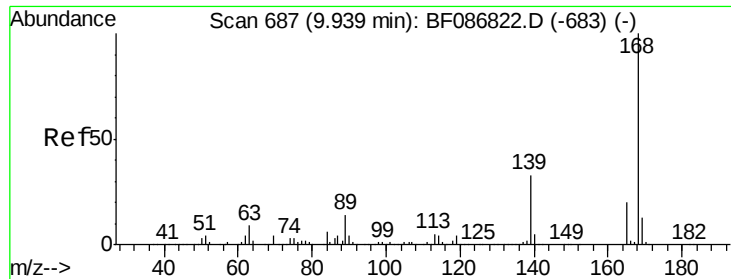




#56
 2,4-Dinitrotoluene
 Concen: 6.60 ng
 RT: 9.66 min Scan# 706
 Delta R.T. -0.28 min
 Lab File: BF086969.D
 Acq: 13 May 2016 12:01

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:165 Resp: 28386
 Ion Ratio Lower Upper
 165 100
 63 1.6 44.3 66.5#
 89 1.3 70.0 105.0#
 182 0.0 1.8 2.6#

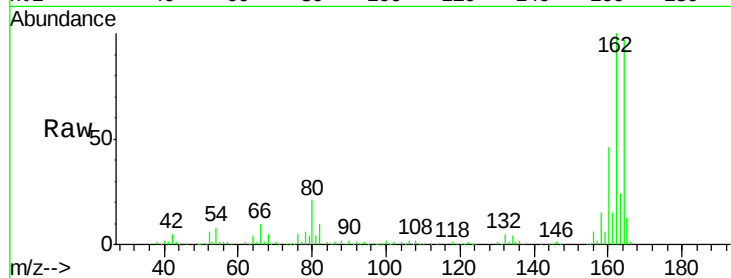


Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF0
 Ion 89.00 (88.70 to 89.70): BF0
 Ion 182.00 (181.70 to 182.70): E

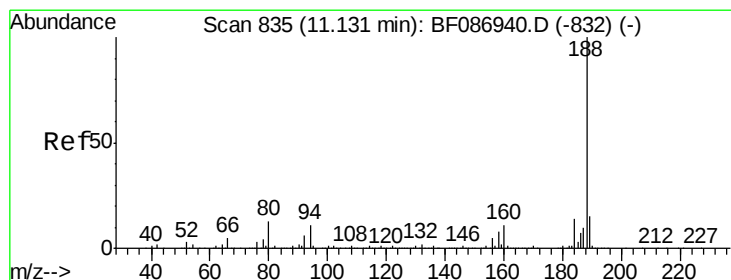
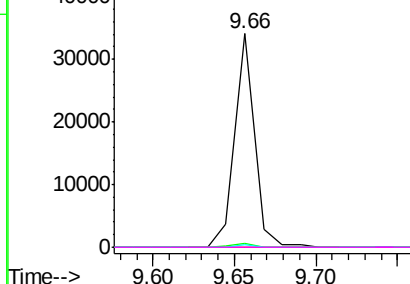



#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.13 min Scan# 835
 Delta R.T. -0.08 min
 Lab File: BF086969.D
 Acq: 13 May 2016 12:01

Tgt Ion:188 Resp: 320111
 Ion Ratio Lower Upper
 188 100
 94 11.6 6.8 10.2#
 80 12.5 7.1 10.7#

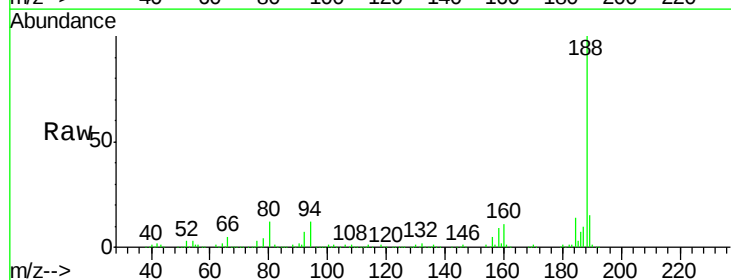

Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF0
 Ion 80.00 (79.70 to 80.70): BF0

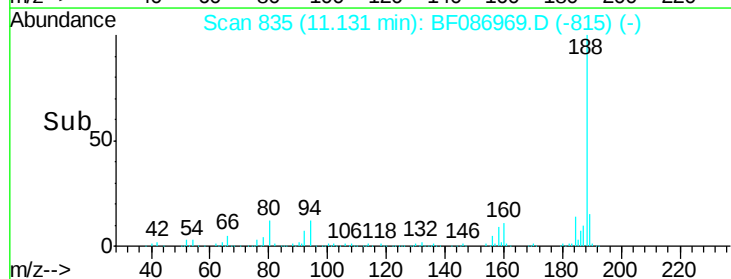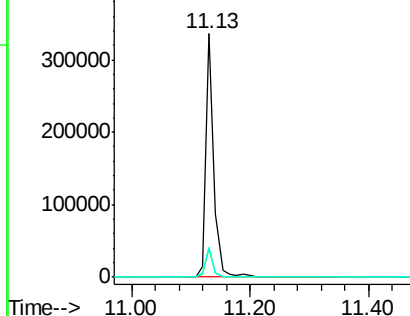


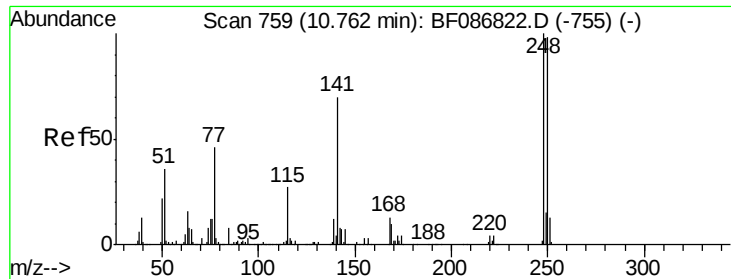




#66
4-Bromophenyl-phenylether
Concen: 3.82 ng
RT: 10.44 min Scan# 775
Delta R.T. -0.32 min
Lab File: BF086969.D
Acq: 13 May 2016 12:01

Instrument :
BNA_F
ClientSampled :

Tot Ion:248 Resp: 12411
Ion Ratio Lower Upper
248 100
250 207.2 78.6 117.8#
141 532.1 76.0 114.0#

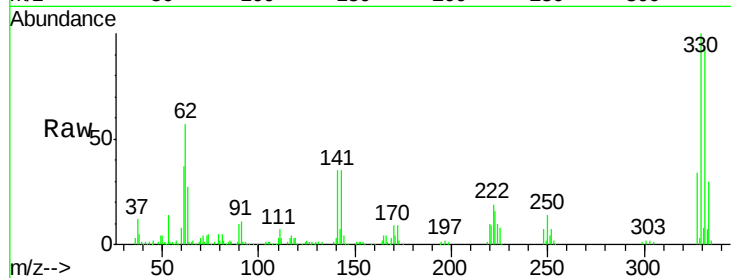


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

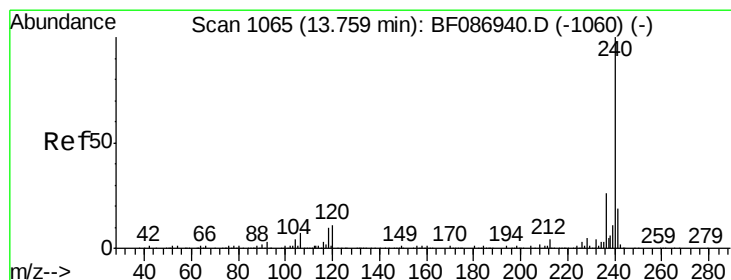
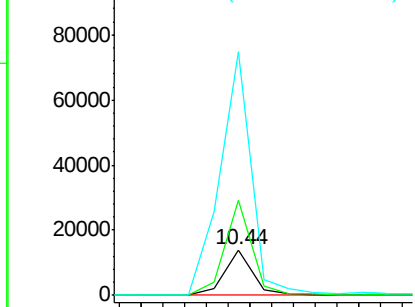



#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.76 min Scan# 1065
Delta R.T. -0.08 min
Lab File: BF086969.D
Acq: 13 May 2016 12:01

Tgt Ion:240 Resp: 311128
Ion Ratio Lower Upper
240 100
120 11.4 11.2 16.8
236 26.4 21.2 31.8

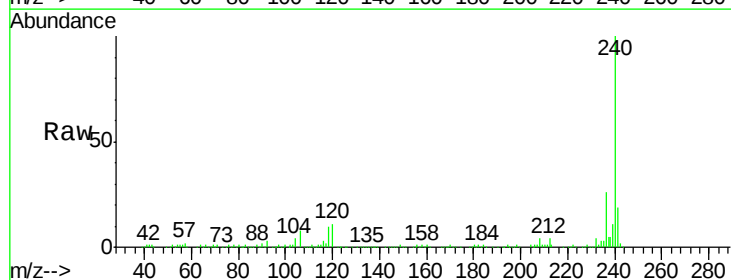

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

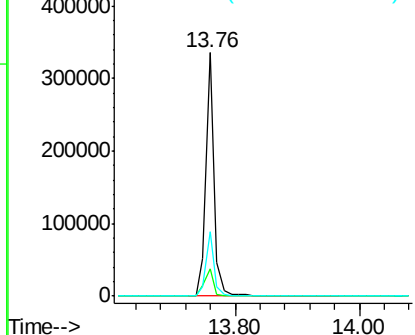

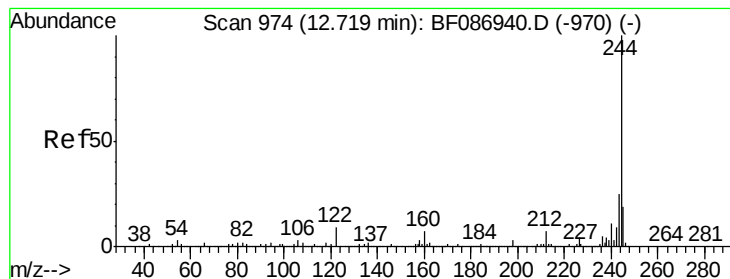

#78

Terphenyl-d14

Concen: 61.15 ng

RT: 12.72 min Scan# 974

Delta R.T. -0.08 min

Lab File: BF086969.D

Acq: 13 May 2016 12:01

Instrument :

BNA_F

ClientSampleId :


Tot Ion:244 Resp: 896685

Ion Ratio Lower Upper

244 100

212 7.9 6.2 9.2




122 11.3 12.0 18.0#

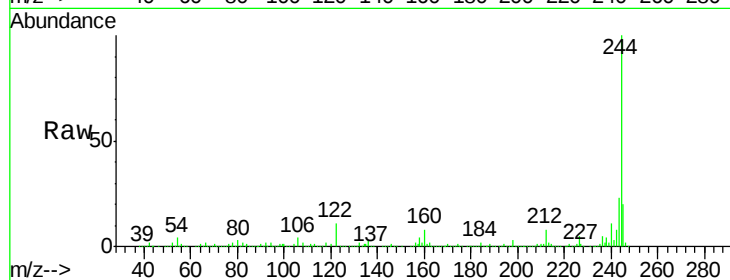

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

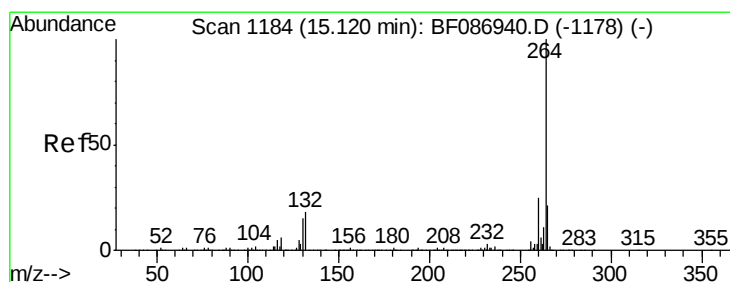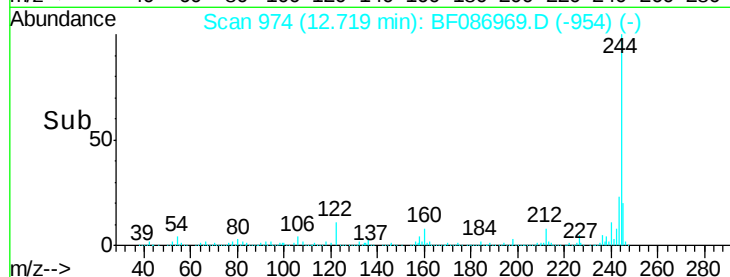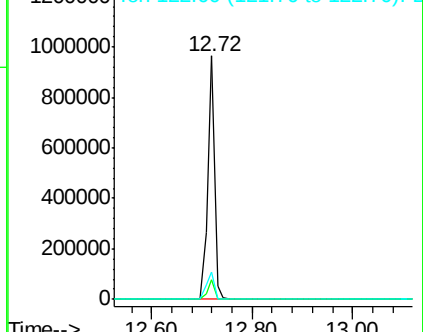

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.12 min Scan# 1184

Delta R.T. -0.09 min

Lab File: BF086969.D

Acq: 13 May 2016 12:01


Tgt Ion:264 Resp: 247186

Ion Ratio Lower Upper

264 100

260 22.9 19.5 29.3

265 20.6 17.3 25.9

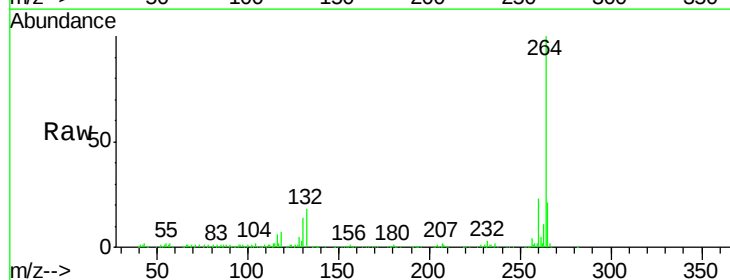

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

