
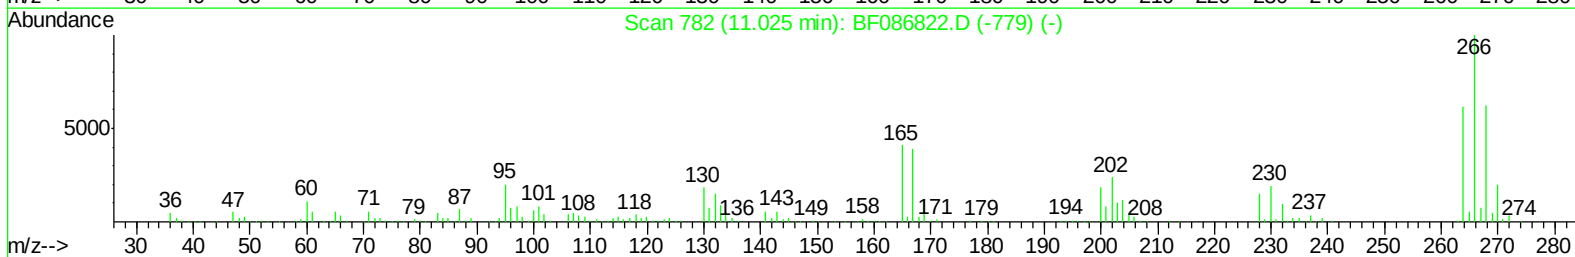
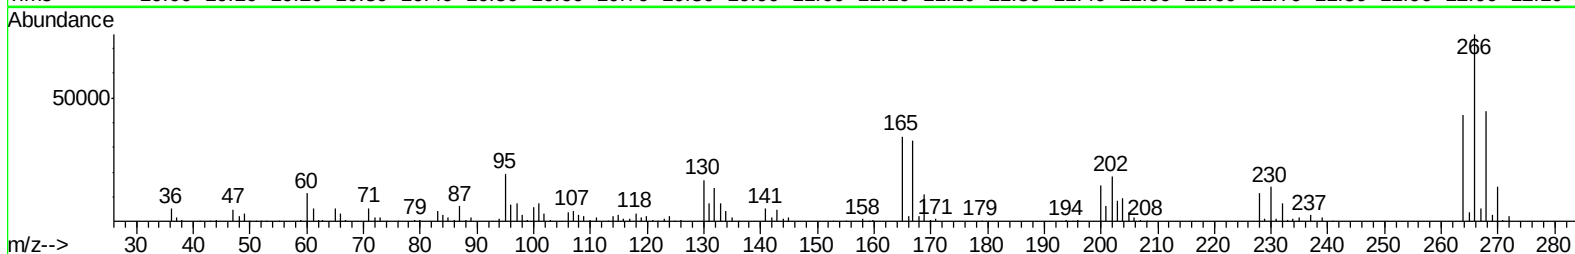


Data Path : Z:\HPCHEM1\BNA\_F\Data\BF051216\  
Data File : BF086927.D  
Acq On : 12 May 2016 13:27  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 18:53:29 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050916.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon May 09 16:04:56 2016  
Response via : Initial Calibration

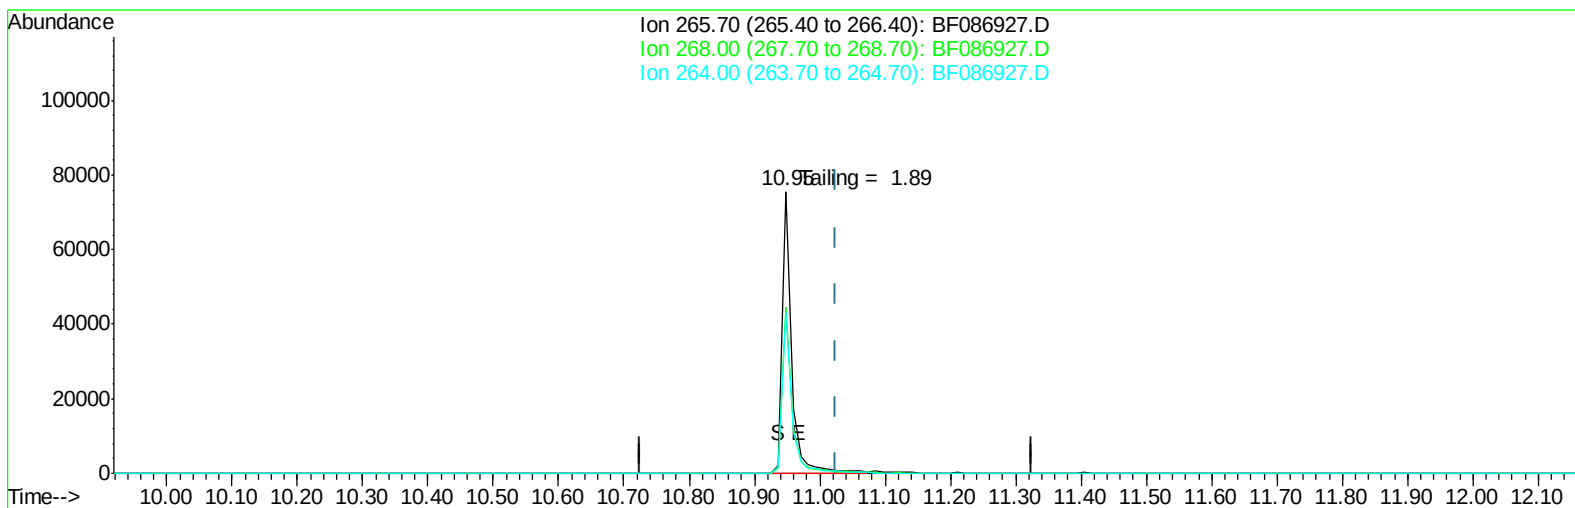

TIC: BF086927.D

(69) Pentachlorophenol (C)




10.948min (-0.077) 56009.69ng

response 76372

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 64.40 | 58.94 |
| 264.00 | 66.10 | 57.35 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_F\Data\BF051216\  
Data File : BF086927.D  
Acq On : 12 May 2016 13:27  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 18:53:29 2016  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF050916.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon May 09 16:04:56 2016  
Response via : Initial Calibration

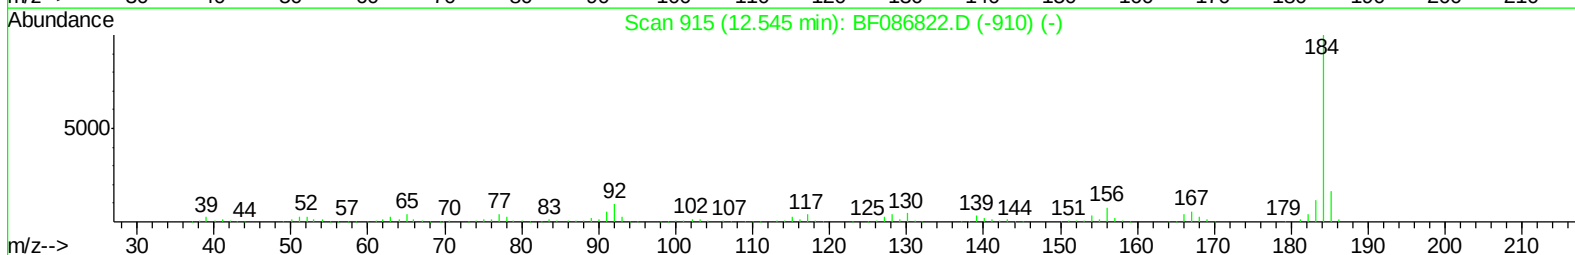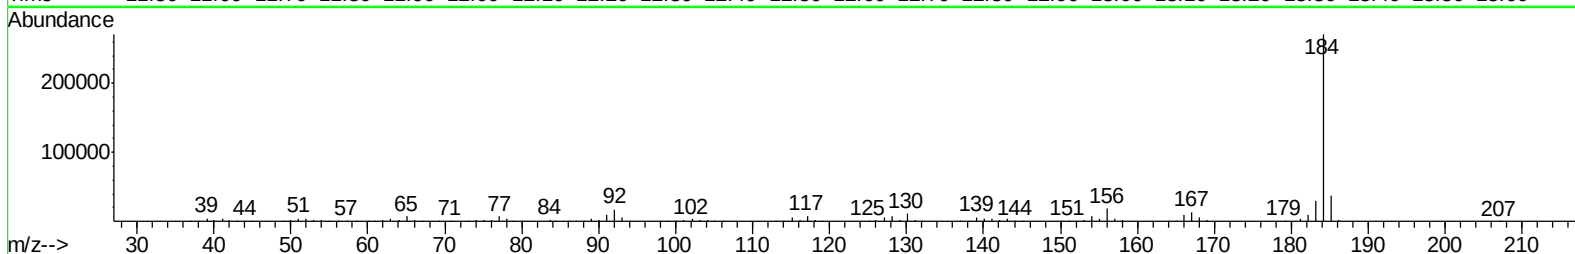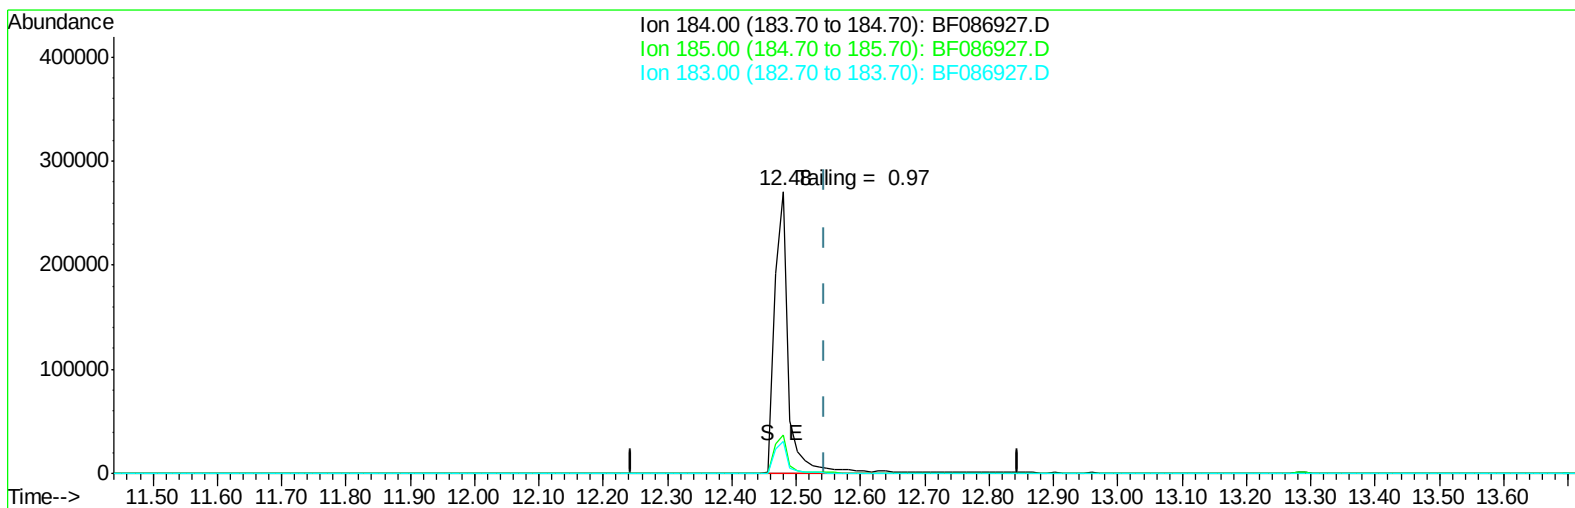

TIC: BF086927.D

(76) Benzidine

12.479min (-0.066) 56771.32ng

response 409585

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 17.00 | 13.69 |
| 183.00 | 12.20 | 11.37 |
| 0.00   | 0.00  | 0.00  |