
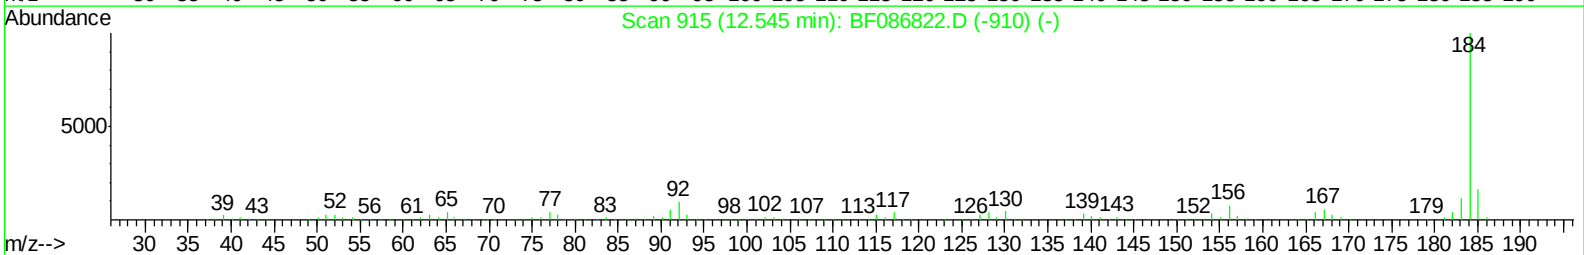
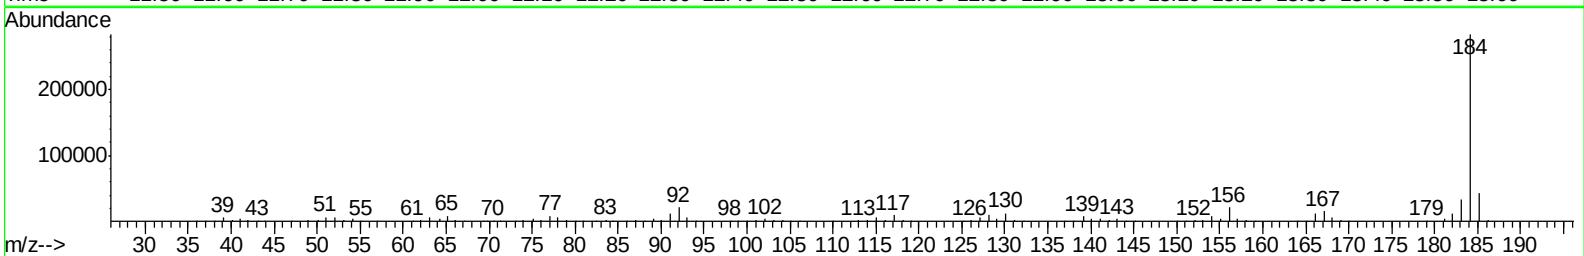


```
Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051216\  
Data File : BF086956.D  
Acq On    : 13 May 2016    5:14  
Operator  : UM/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: May 13 08:24:37 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 13 00:58:18 2016
Response via : Initial Calibration

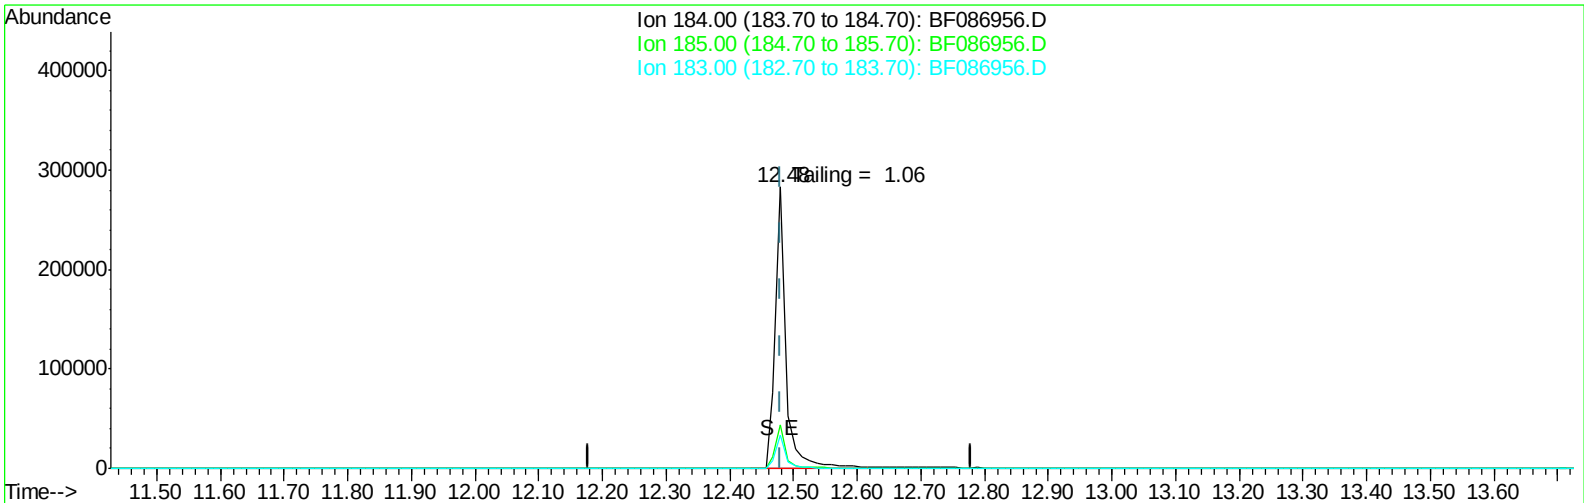

TIC: BF086956.D

(76) Benzidine




12.479min (+0.000) 0.00ng

response 332838

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	15.49
183.00	12.20	11.76
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051216\
Data File : BF086956.D
Acq On : 13 May 2016 5:14
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 13 08:24:37 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 13 00:58:18 2016
Response via : Initial Calibration

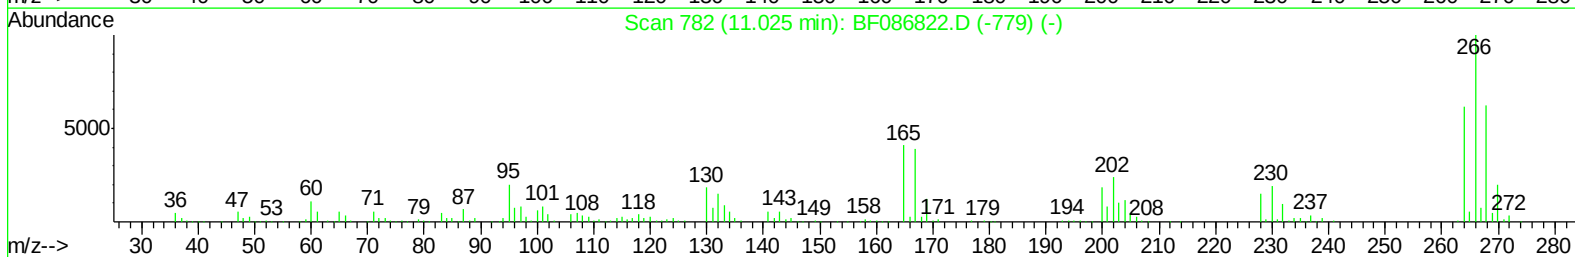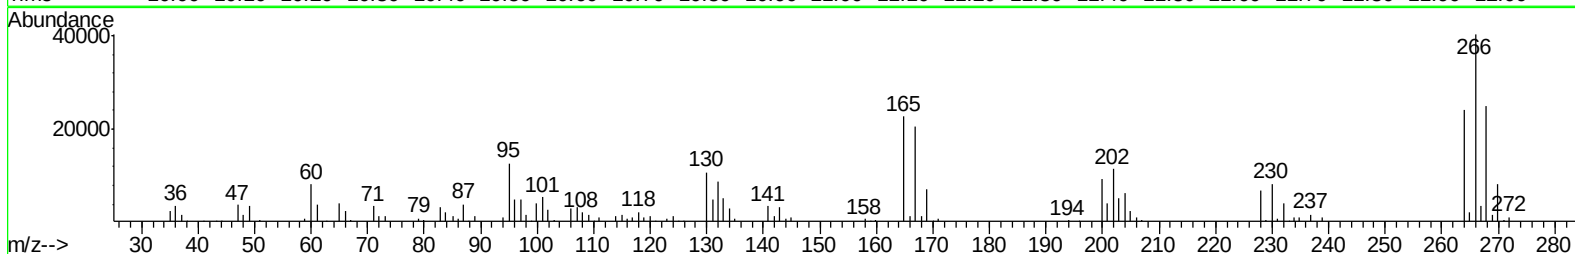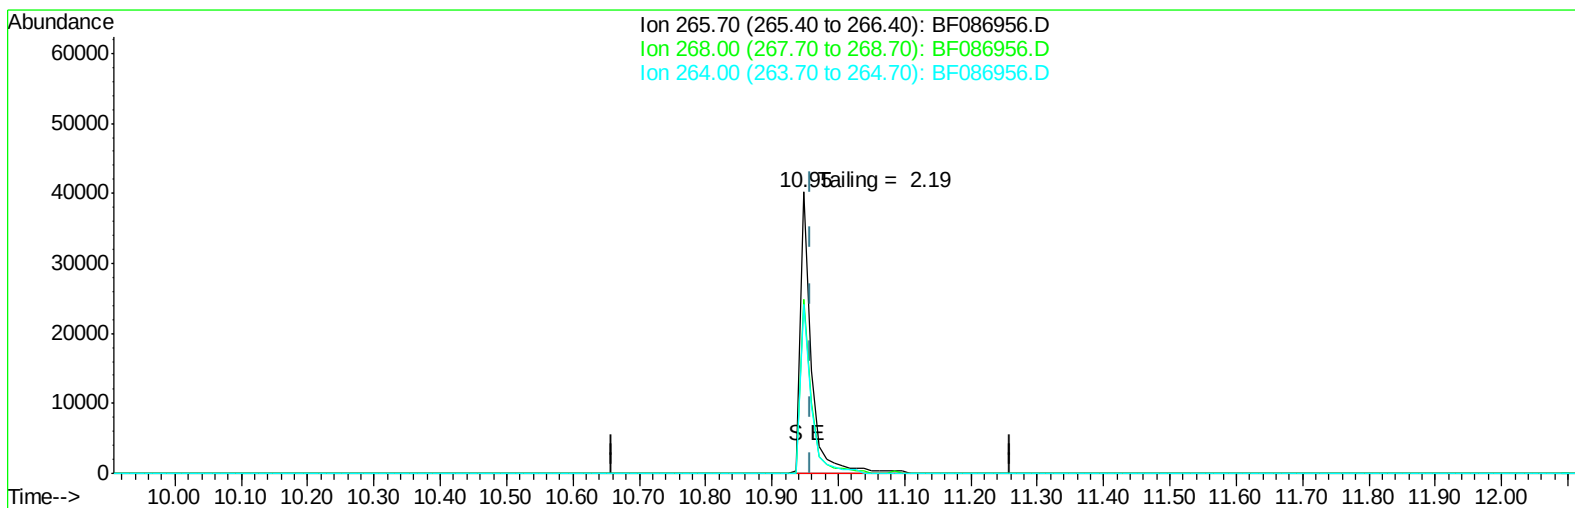

TIC: BF086956.D

(69) Pentachlorophenol (C)

10.948min (-0.011) 0.00ng

response 46414

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	62.02
264.00	66.10	59.95
0.00	0.00	0.00