

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051216\
 Data File : BF086954.D
 Acq On : 13 May 2016 2:44
 Operator : UM/SJ
 Sample : H2968-07 5X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DUPB

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.747	12	14	63	rVB	4268208	9435698	100.00%	42.270%
2	5.210	315	317	331	rBV	503471	605264	6.41%	2.711%
3	6.284	409	411	419	rBV	586457	668399	7.08%	2.994%
4	6.399	419	421	438	rVB	451545	672878	7.13%	3.014%
5	6.616	438	440	443	rBV	868731	1066578	11.30%	4.778%
6	6.776	452	454	457	rBV	581333	516884	5.48%	2.316%
7	7.187	488	490	504	rBV7	285951	401636	4.26%	1.799%
8	7.907	551	553	556	rBV	1430370	1341888	14.22%	6.011%
9	8.982	645	647	650	rBV	544586	596367	6.32%	2.672%
10	9.656	704	706	709	rBV	1500769	1302829	13.81%	5.836%
11	10.445	773	775	778	rBV	274083	282548	2.99%	1.266%
12	11.131	833	835	840	rBV	1134837	1151741	12.21%	5.160%
13	12.342	939	941	943	rBV	350482	383685	4.07%	1.719%
14	12.559	958	960	963	rBV	274707	372027	3.94%	1.667%
15	12.719	972	974	976	rVB	349491	451161	4.78%	2.021%
16	12.891	986	989	991	rBV	71261	113190	1.20%	0.507%
17	12.959	991	995	997	rBV	81652	100486	1.06%	0.450%
18	13.759	1062	1065	1071	rBV2	1244403	1579914	16.74%	7.078%
19	14.754	1150	1152	1156	rBV	154292	291041	3.08%	1.304%
20	15.074	1177	1180	1182	rBV	101627	156204	1.66%	0.700%
21	15.120	1182	1184	1187	rBV	560894	831981	8.82%	3.727%


Sum of corrected areas: 22322399

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051216\
Data File : BF086954.D
Acq On : 13 May 2016 2:44
Operator : UM/SJ
Sample : H2968-07 5X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DUPB

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

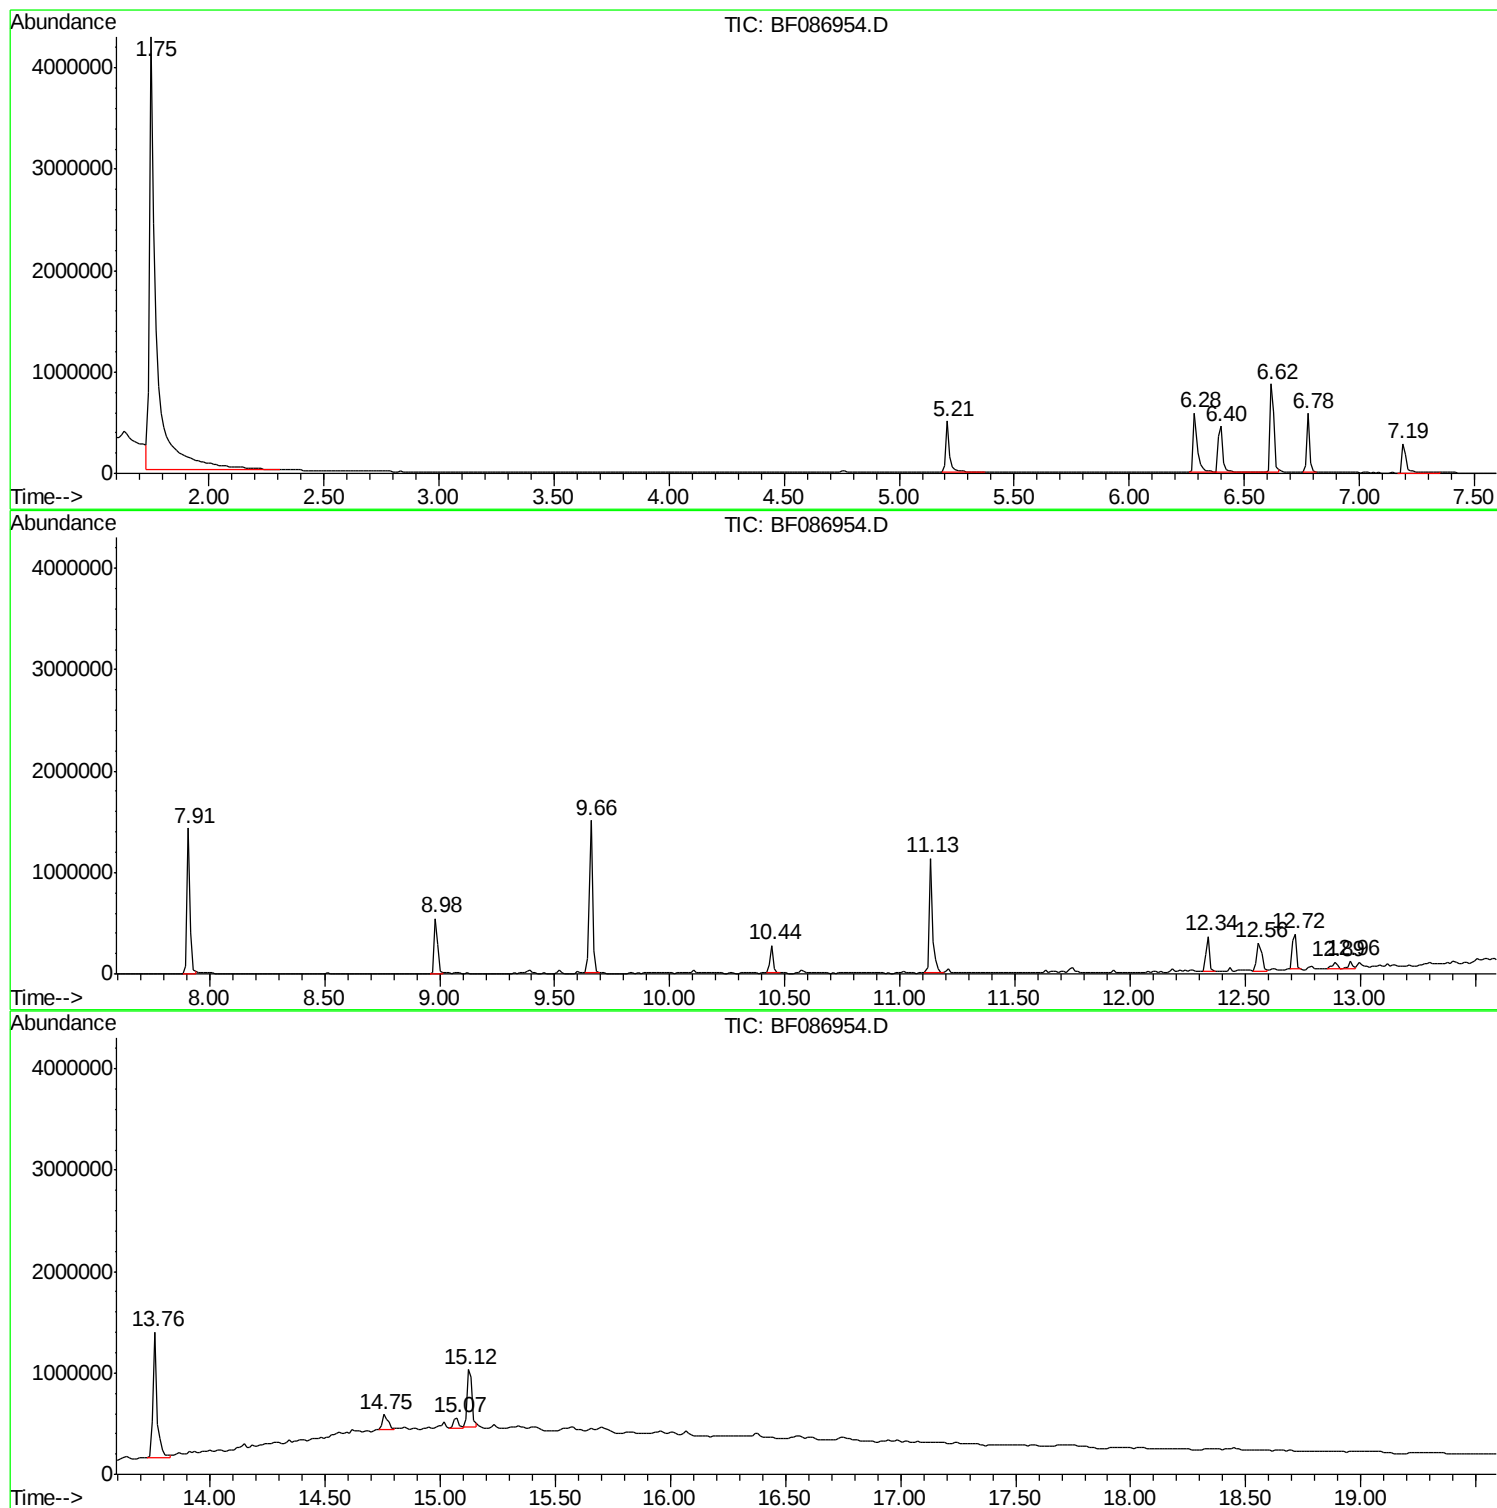

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051216\
Data File : BF086954.D
Acq On : 13 May 2016 2:44
Operator : UM/SJ
Sample : H2968-07 5X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DUPB










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.40 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.40	12.62 ng	672878	1,4-Dichlorobenzene-d4	6.62

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12
4		5-Aminoindole	132	C8H8N2	005192-03-0	9
5		Imidazole, 4,5-dicyano-1-methyl-	132	C6H4N4	019485-35-9	9

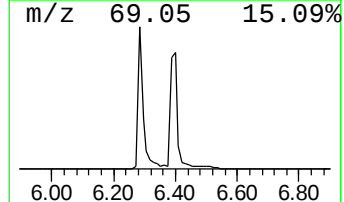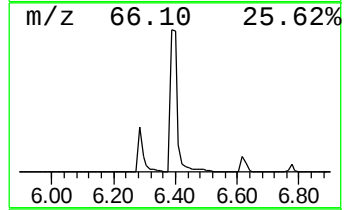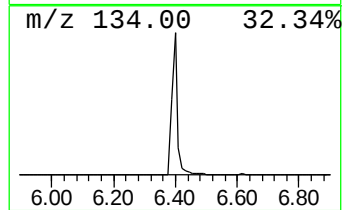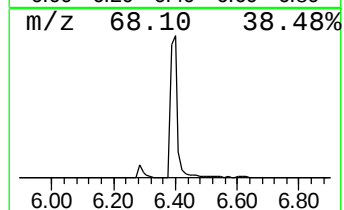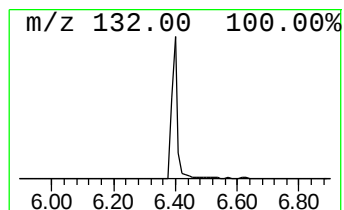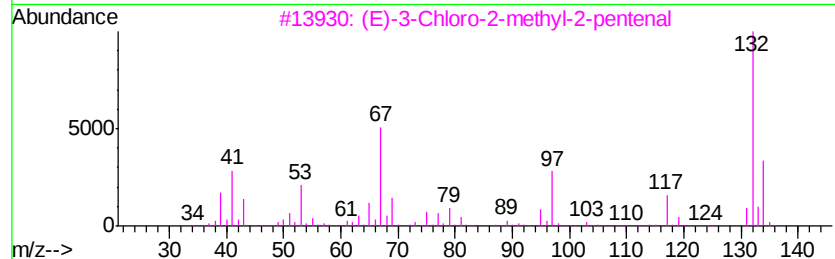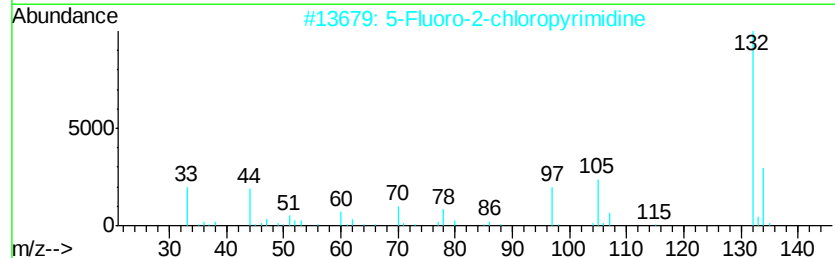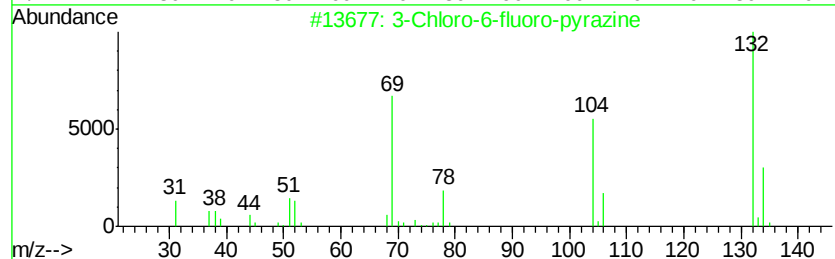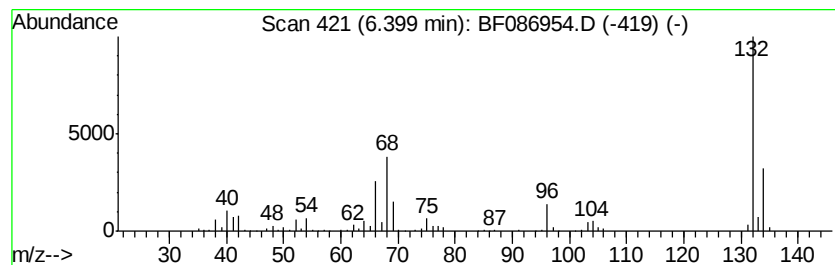

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051216\
Data File : BF086954.D
Acq On : 13 May 2016 2:44
Operator : UM/SJ
Sample : H2968-07 5X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DUPB

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.40	6.40	12.6	ng	672878	1	6.62	1066580	20.0