


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051216\
 Data File : BF086927.D
 Acq On : 12 May 2016 13:27
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 13 14:55:23 2016

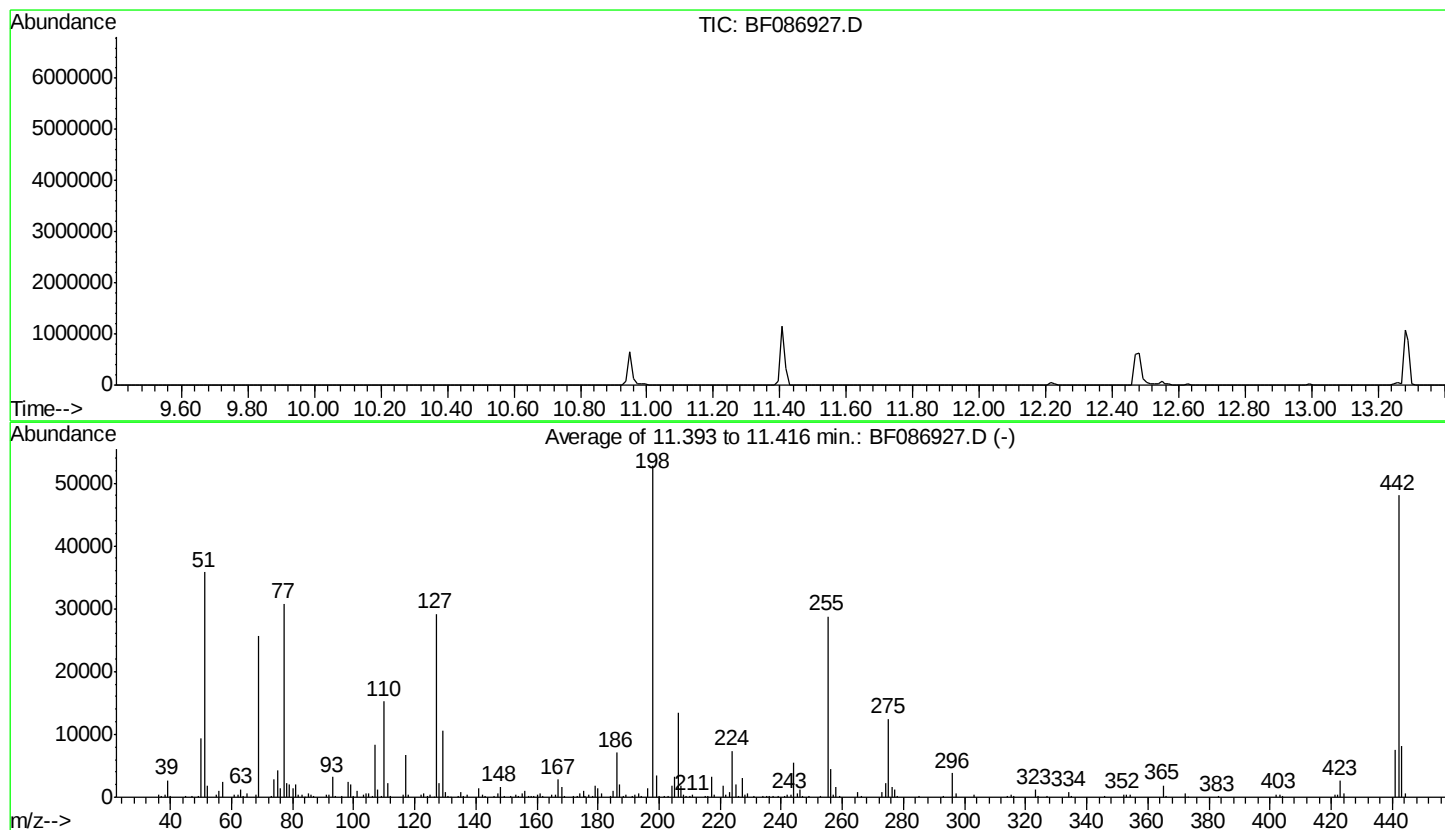

AutoFind: Scans 858, 859, 860; Background Corrected with Scan 855

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	67.9	35849	PASS
68	69	0.00	2	1.6	404	PASS
69	198	0.00	100	48.7	25679	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.4	29233	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	52767	PASS
199	198	5	9	6.8	3570	PASS
275	198	10	60	23.7	12520	PASS
365	198	1	100	3.6	1893	PASS
441	442	0.01	24	15.6	7516	PASS
442	198	50	100	91.1	48067	PASS
443	442	15	24	17.1	8205	PASS