


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051216\
 Data File : BF086956.D
 Acq On : 13 May 2016 5:14
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 13 14:55:23 2016

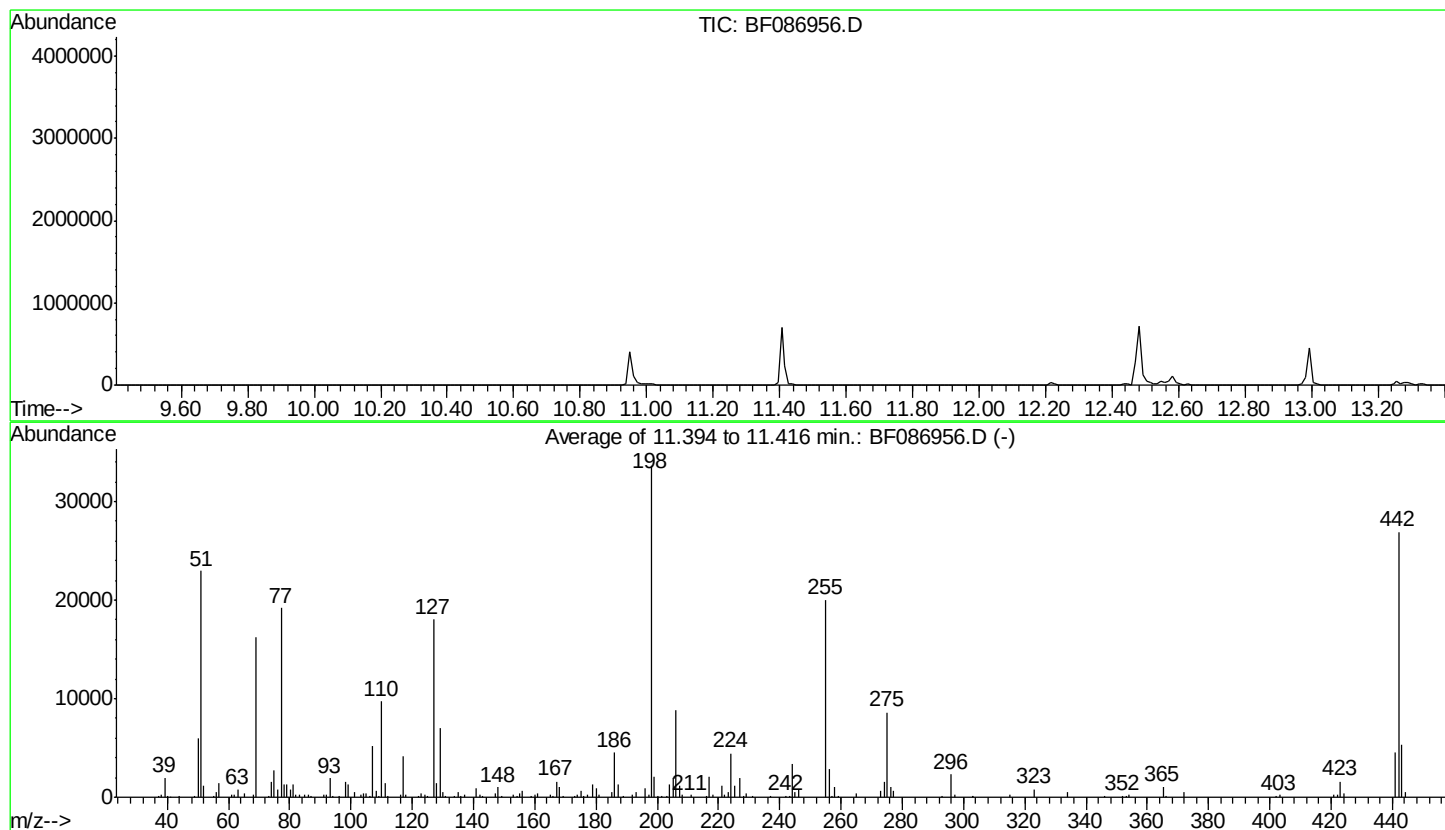

AutoFind: Scans 858, 859, 860; Background Corrected with Scan 855

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	68.3	22977	PASS
68	69	0.00	2	1.7	275	PASS
69	198	0.00	100	48.1	16200	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.5	18008	PASS
197	198	0.00	2	0.8	261	PASS
198	198	100	100	100.0	33648	PASS
199	198	5	9	6.3	2132	PASS
275	198	10	60	25.5	8586	PASS
365	198	1	100	3.3	1105	PASS
441	442	0.01	24	17.0	4567	PASS
442	198	50	100	79.9	26901	PASS
443	442	15	24	19.6	5272	PASS