
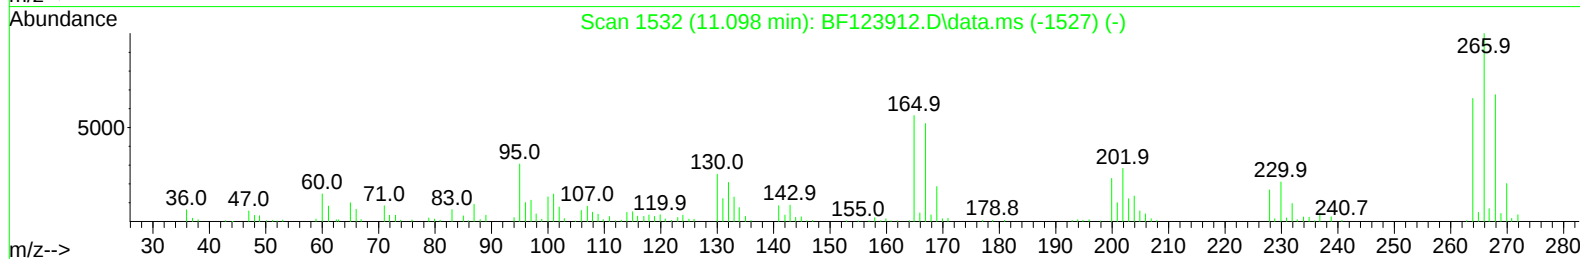
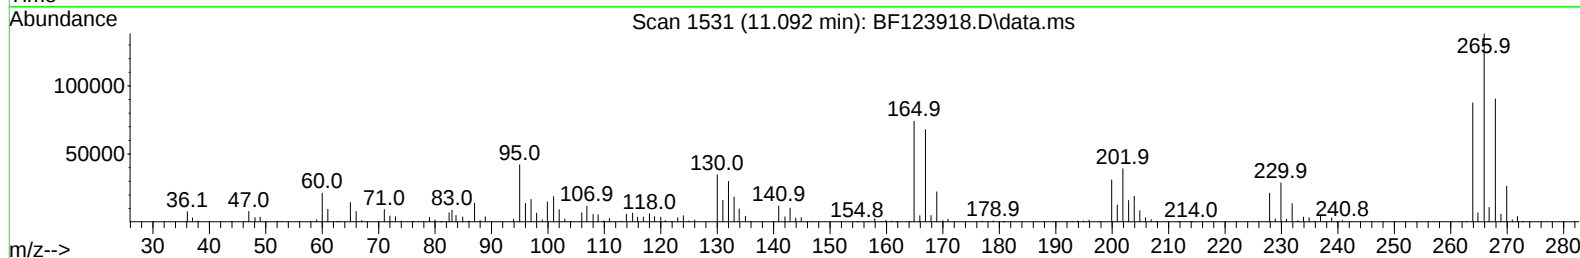


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF051221\  
Data File : BF123918.D  
Acq On : 12 May 2021 9:23  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 11:23:12 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF051121.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue May 11 18:02:17 2021  
Response via : Initial Calibration

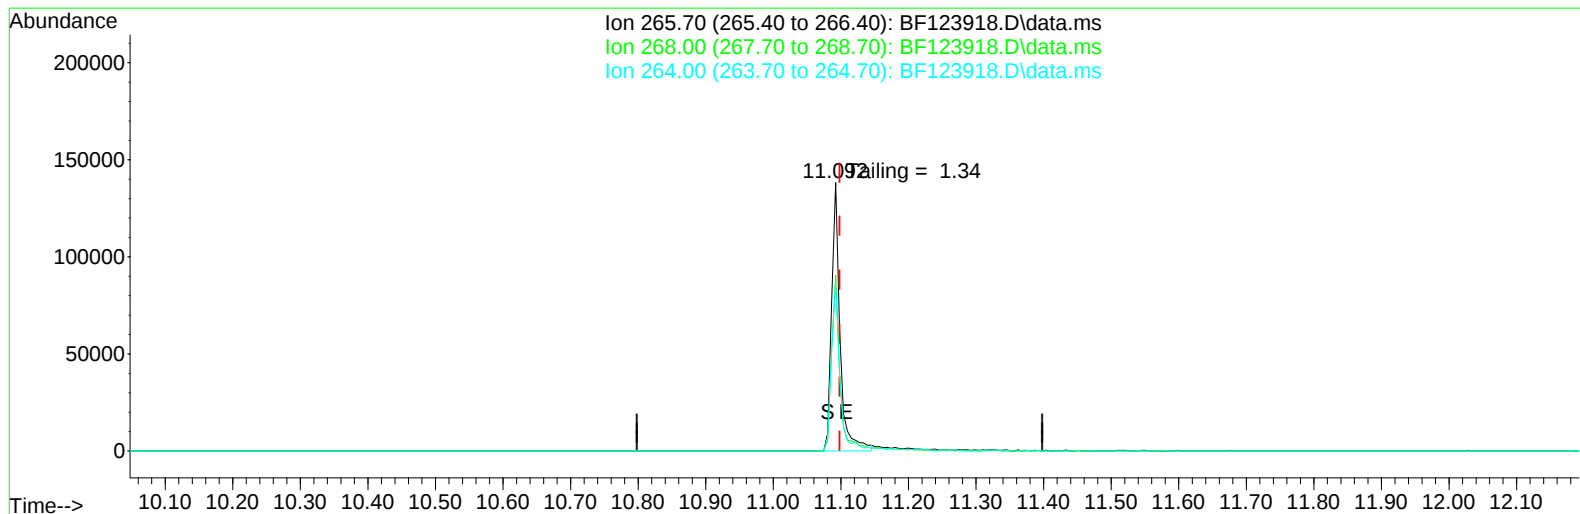

TIC: BF123918.D\data.ms

**(70) Pentachlorophenol (C)**




11.092min (-0.006) 34830.44 ng

response 126316

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.50  | 65.46  |
| 264.00 | 65.70  | 63.31  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF051221\  
Data File : BF123918.D  
Acq On : 12 May 2021 9:23  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 11:23:12 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF051121.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue May 11 18:02:17 2021  
Response via : Initial Calibration

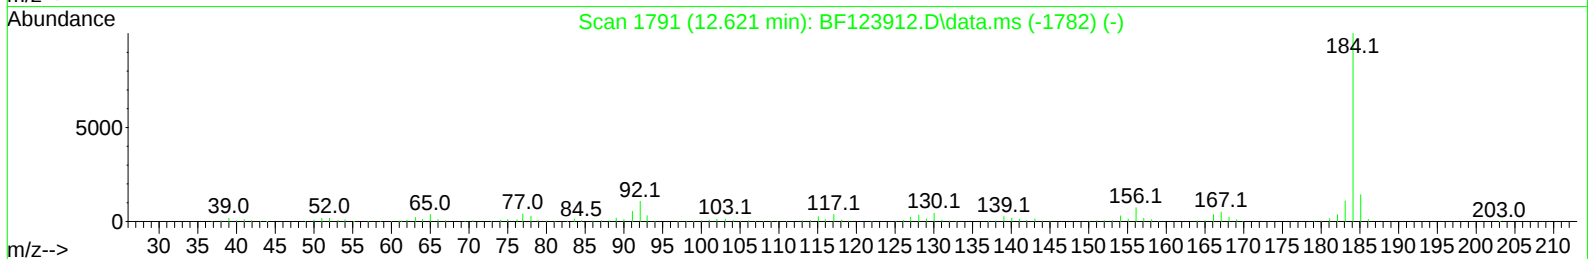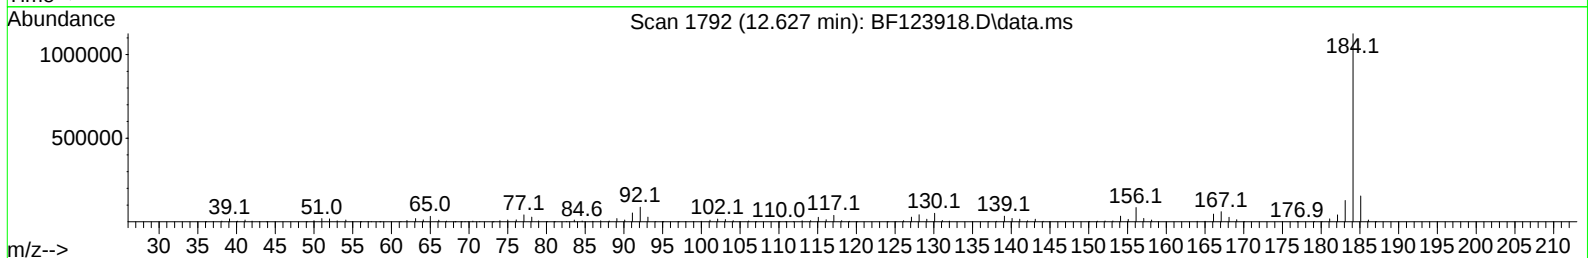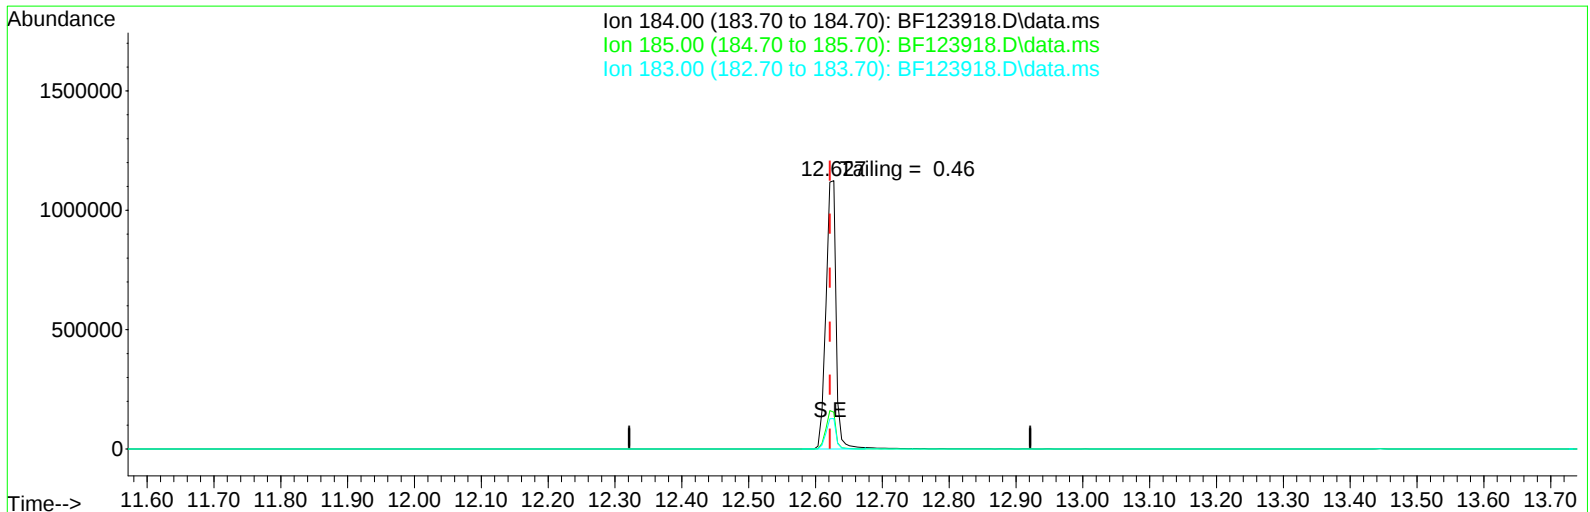

TIC: BF123918.D\data.ms

**(77) Benzidine**

12.627min (+ 0.006) 0.00 ng

response 1185018

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.10  | 13.71  |
| 183.00 | 9.80   | 11.37  |
| 0.00   | 0.00   | 0.00   |