
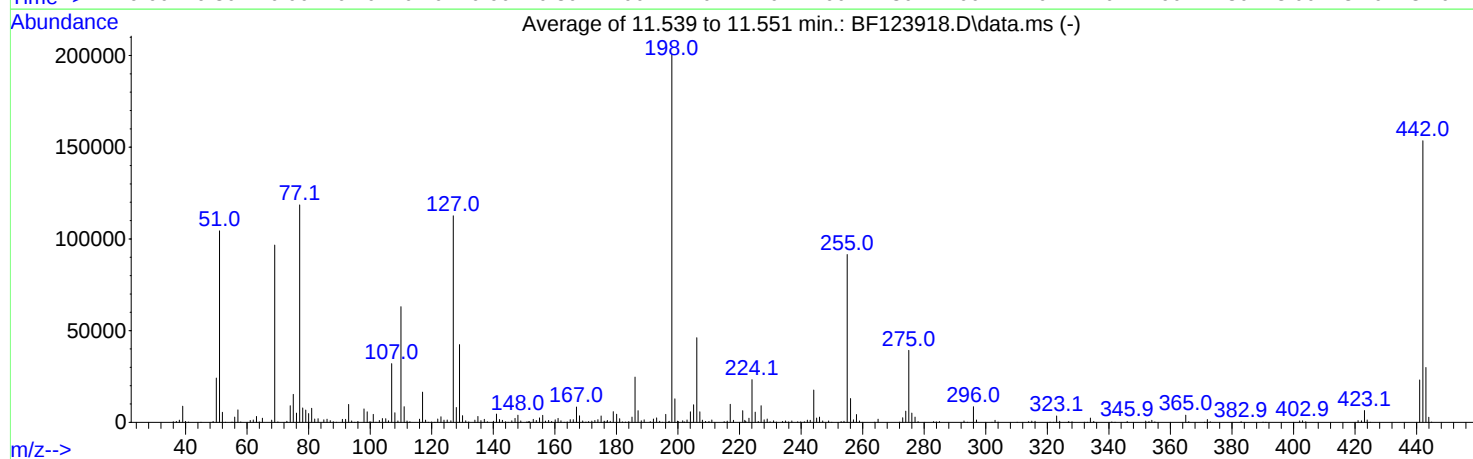


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051221\
 Data File : BF123918.D
 Acq On : 12 May 2021 9:23
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 11 18:02:17 2021

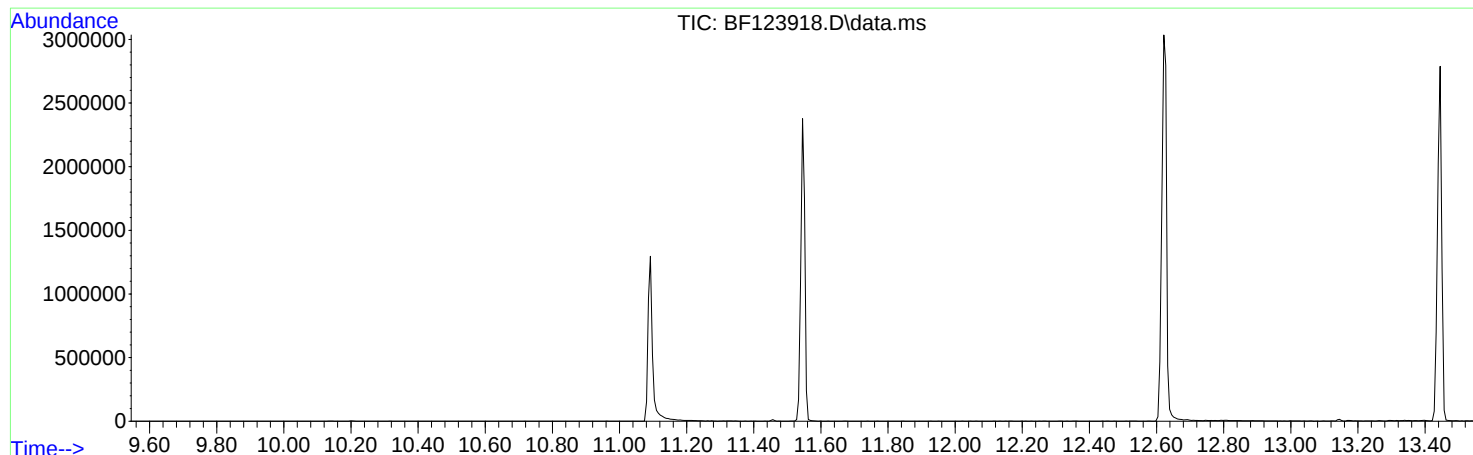




AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.1	104405	PASS
68	69	0.00	2	1.3	1215	PASS
69	198	0.00	100	48.2	96619	PASS
70	69	0.00	2	0.3	261	PASS
127	198	10	80	56.2	112624	PASS
197	198	0.00	2	0.3	654	PASS
198	198	100	100	100.0	200541	PASS
199	198	5	9	6.4	12848	PASS
275	198	10	60	19.6	39235	PASS
365	198	1	100	1.9	3899	PASS
441	198	0.01	100	11.5	23133	PASS
442	442	50	100	100.0	153507	PASS
443	442	15	24	19.5	29888	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051221\
 Data File : BF123918.D
 Acq On : 12 May 2021 9:23
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 12 11:23:12 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 11 18:02:17 2021
 Response via : Initial Calibration

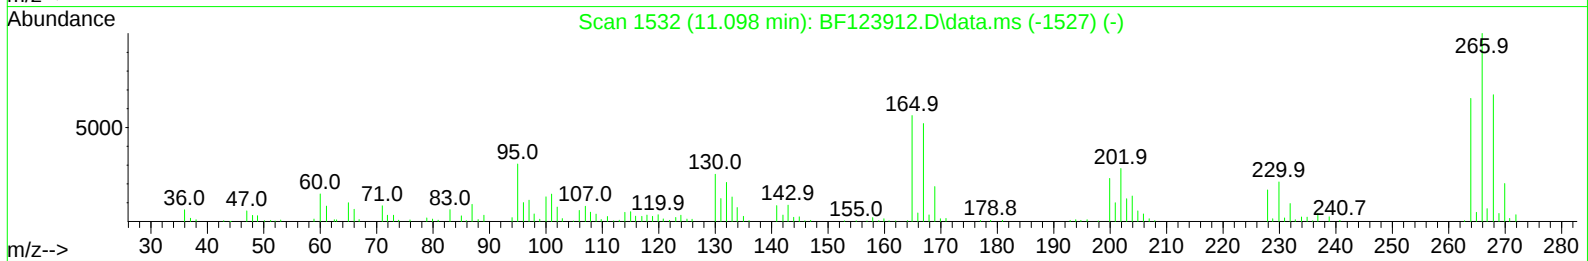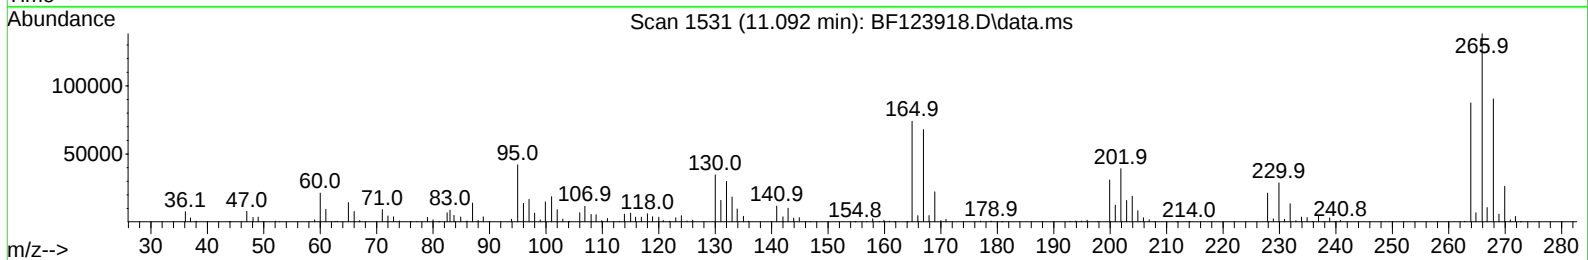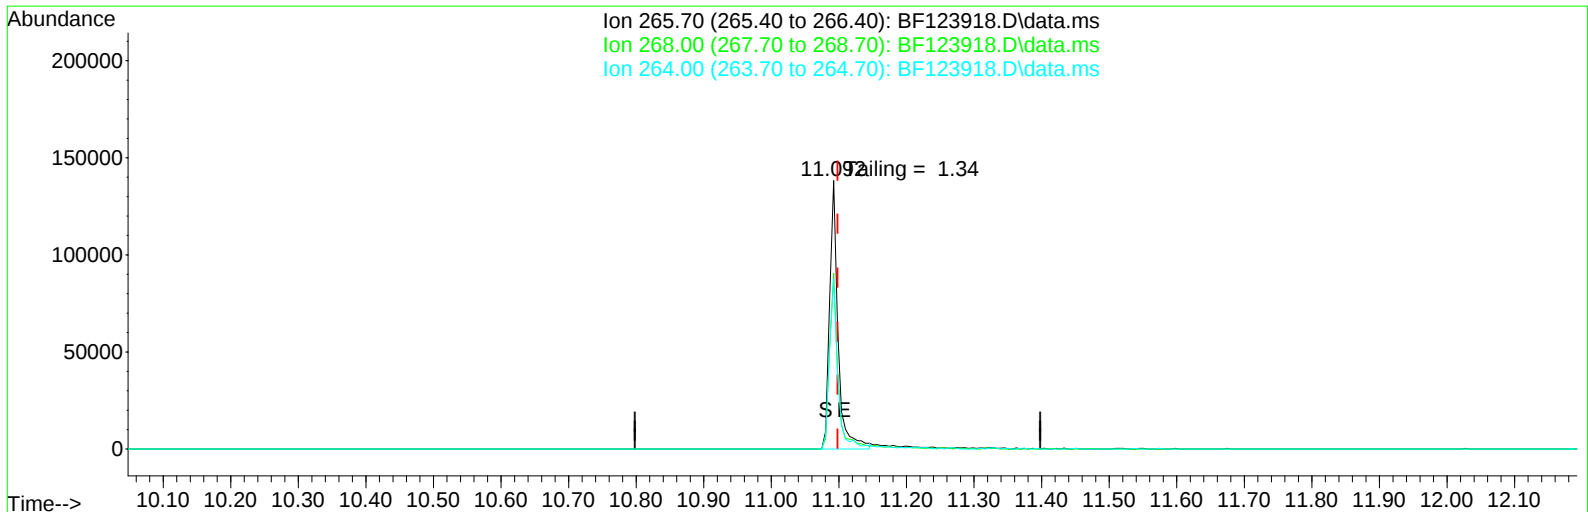

TIC: BF123918.D\data.ms

(70) Pentachlorophenol (C)

11.092min (-0.006) 34830.44 ng




response 126316

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	65.46
264.00	65.70	63.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051221\
Data File : BF123918.D
Acq On : 12 May 2021 9:23
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 12 11:23:12 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 11 18:02:17 2021
Response via : Initial Calibration

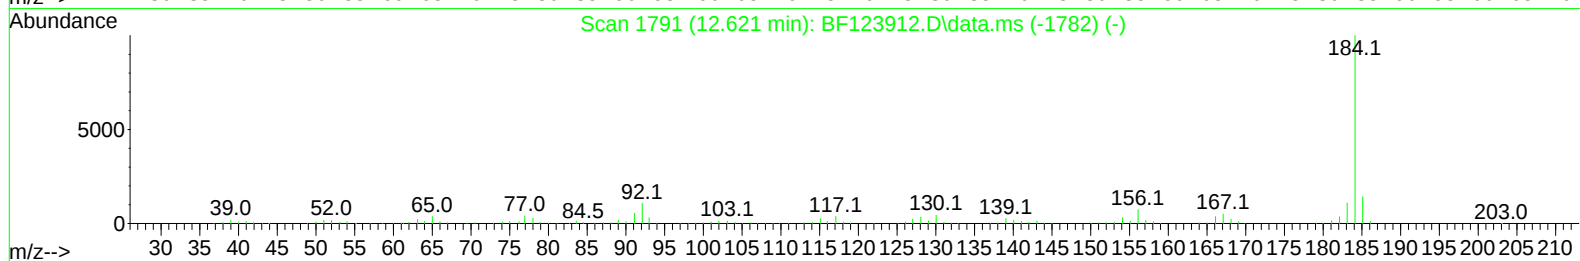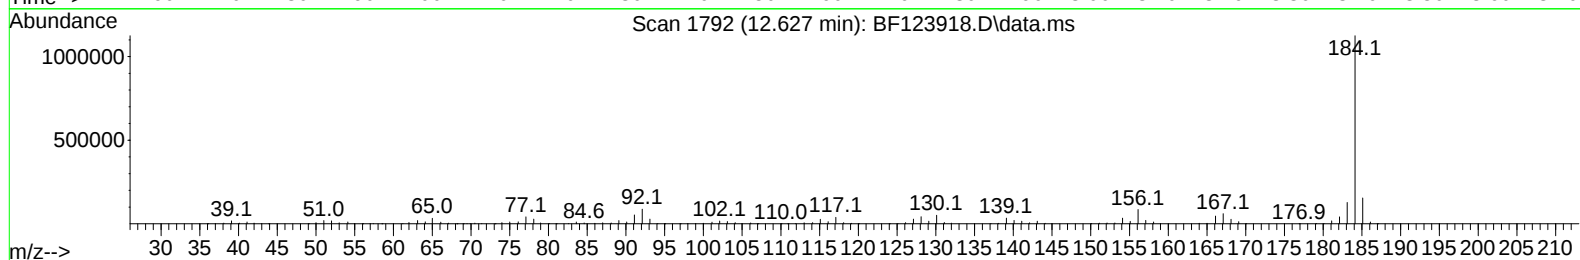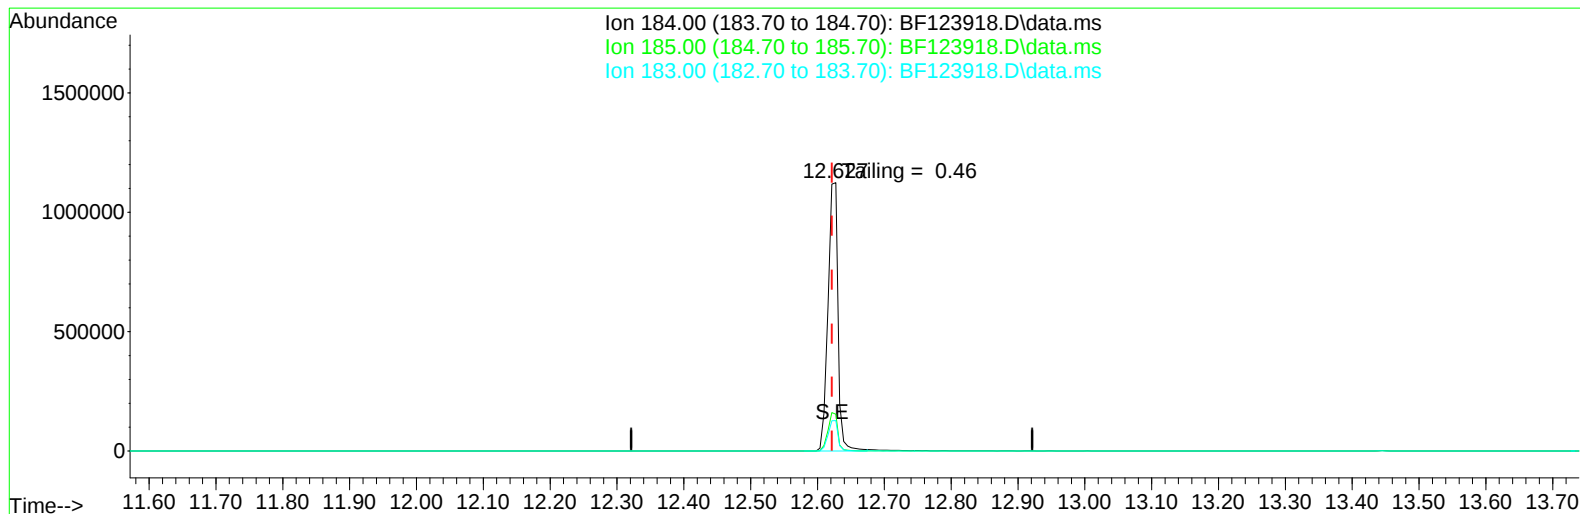

TIC: BF123918.D\data.ms

(77) Benzidine

12.627min (+ 0.006) 0.00 ng

response 1185018

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	13.71
183.00	9.80	11.37
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/19/2019	BNA_G	<u>BF123918.D</u>
Compound Name	Response	Retention Time
DDT	450066	13.44
DDD	2822	13.14
DDE	576	12.81
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3398	453464	0.75