

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051222\
 Data File : BF128224.D
 Acq On : 12 May 2022 19:31
 Operator : CG\JU
 Sample : N2804-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FETWP-3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128224.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.116	478	481	489	rVB	41179	44320	1.89%	0.396%
2	5.516	546	549	564	rBV	889958	799614	34.03%	7.144%
3	6.522	716	720	733	rBV	568000	527107	22.43%	4.709%
4	6.893	780	783	787	rBV	512669	433673	18.46%	3.875%
5	7.463	874	880	883	rBV	1557769	1471498	62.63%	13.147%
6	8.181	997	1002	1005	rBV	542056	504974	21.49%	4.512%
7	9.251	1179	1184	1188	rBV	2368426	2349688	100.00%	20.993%
8	9.934	1296	1300	1310	rVB	561784	508410	21.64%	4.542%
9	10.728	1431	1435	1444	rBV	1064384	936937	39.87%	8.371%
10	11.428	1550	1554	1563	rBV	591549	490879	20.89%	4.386%
11	13.016	1819	1824	1827	rBV	2497056	2181988	92.86%	19.494%
12	13.939	1976	1981	1995	rBV8	27521	89660	3.82%	0.801%
13	14.074	2000	2004	2008	rBV	513052	468165	19.92%	4.183%
14	14.169	2017	2020	2023	rVB	24490	26029	1.11%	0.233%
15	15.574	2254	2259	2267	rBV	276115	360040	15.32%	3.217%




Sum of corrected areas: 11192982

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051222\
Data File : BF128224.D
Acq On : 12 May 2022 19:31
Operator : CG\JU
Sample : N2804-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FETWP-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

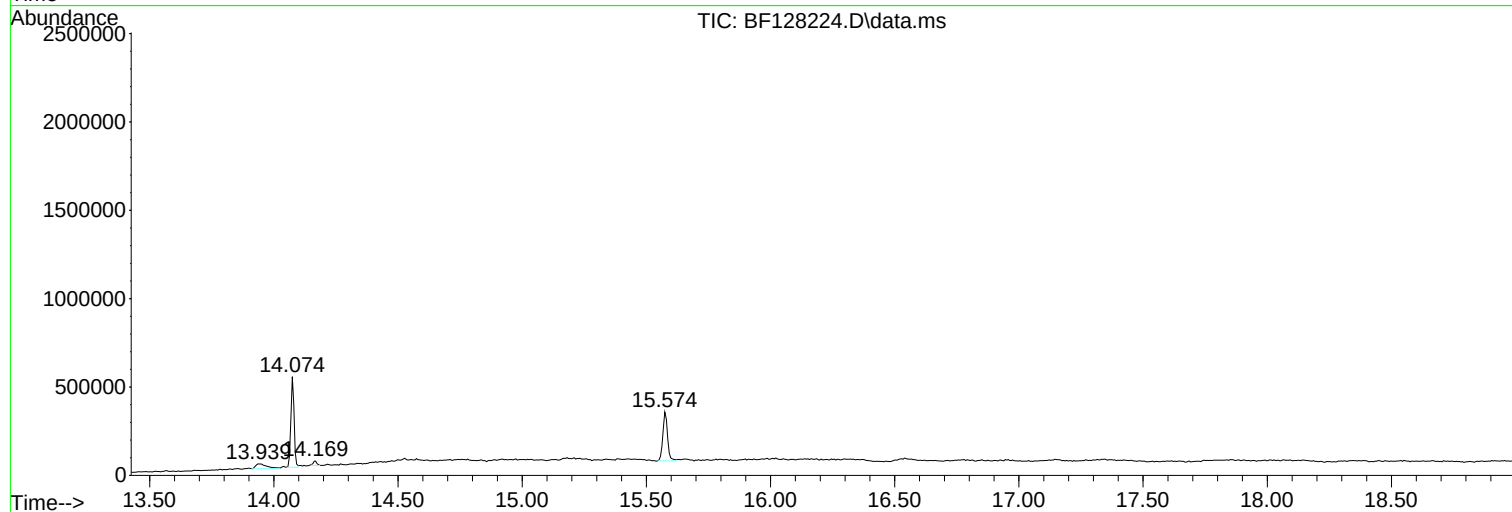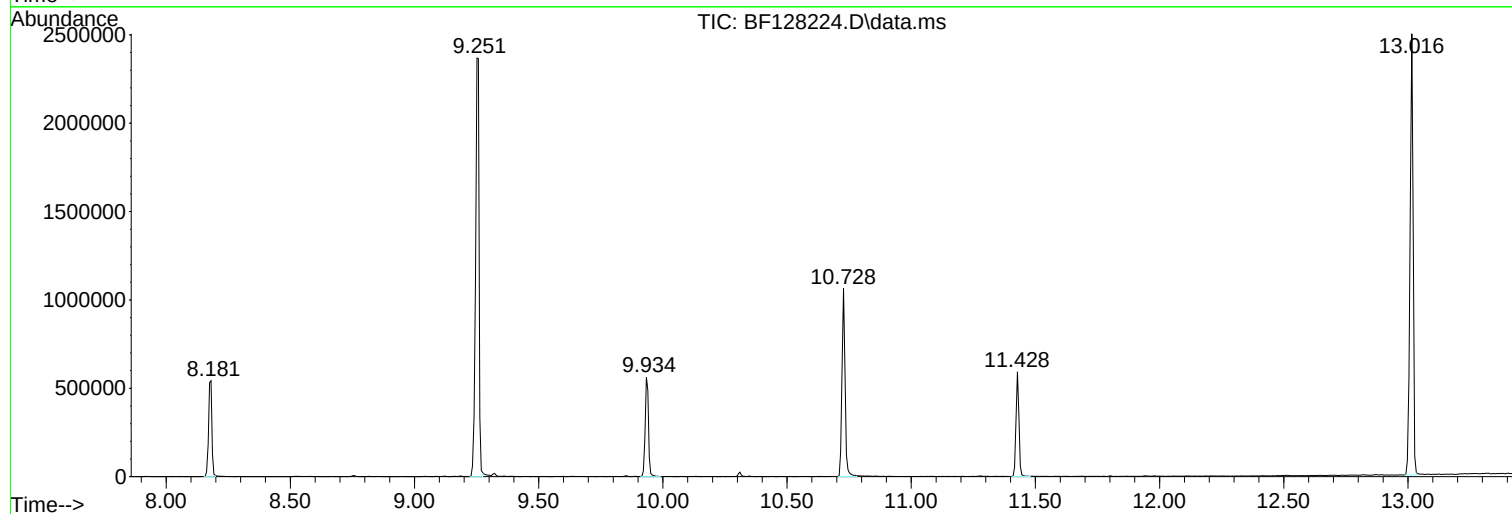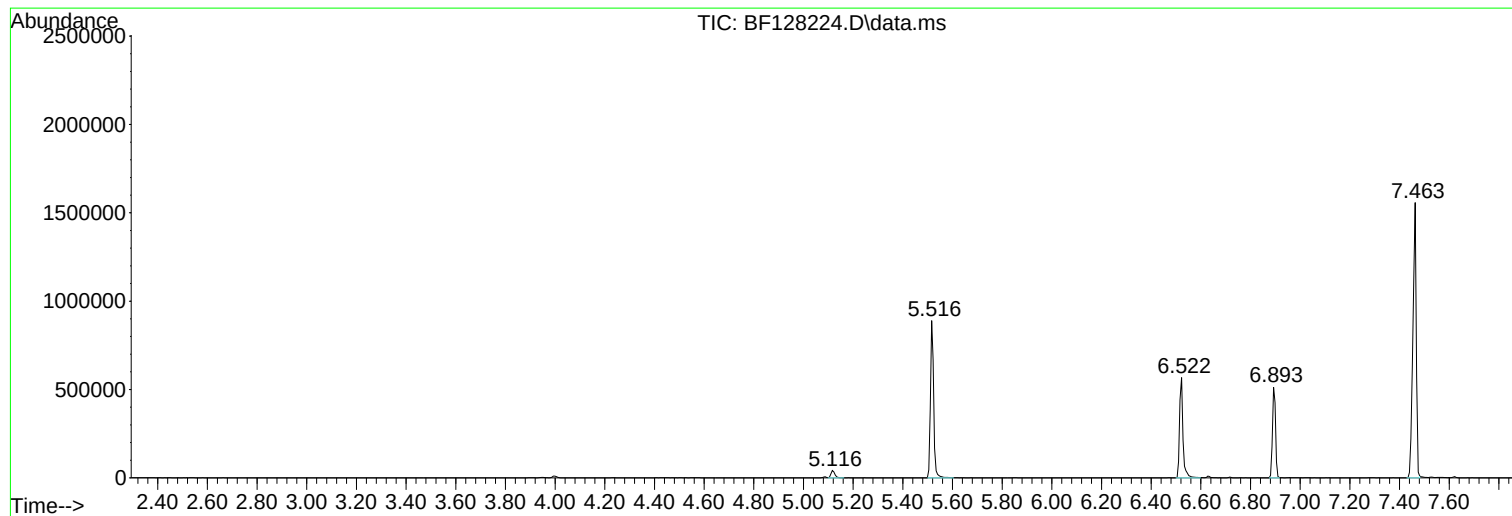

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051222\
Data File : BF128224.D
Acq On : 12 May 2022 19:31
Operator : CG\JU
Sample : N2804-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FETWP-3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.116	2.04 ng	44320	1,4-Dichlorobenzene-d4	6.893

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72		
2	Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	36		
3	3-Octanol	130	C8H18O	000589-98-0	36		
4	3-Hydroxy-3-methyl-2-butanone	102	C5H10O2	000115-22-0	32		
5	3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	25		

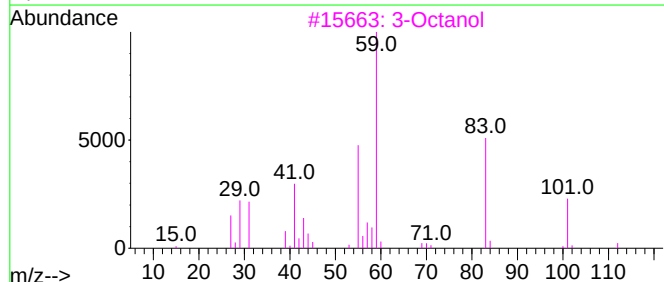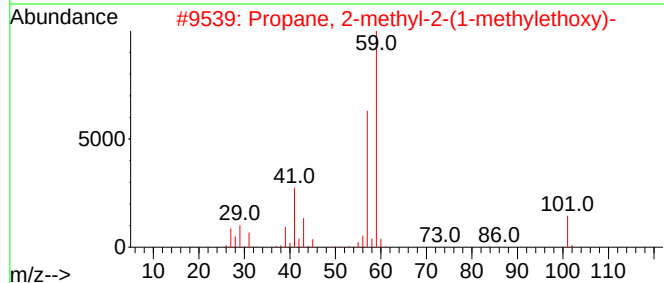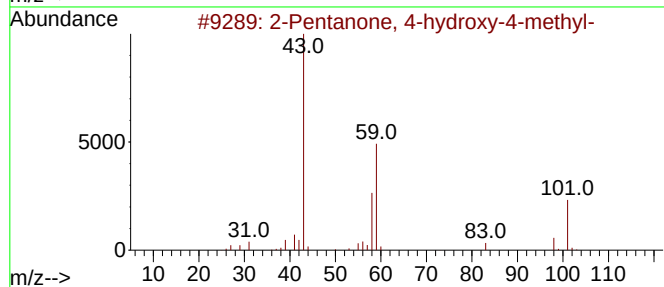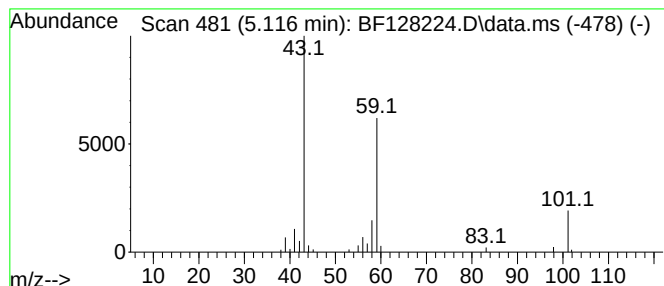

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051222\
Data File : BF128224.D
Acq On : 12 May 2022 19:31
Operator : CG\JU
Sample : N2804-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FETWP-3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 E-15-Heptadecenal Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.939	3.83 ng	89660	Chrysene-d12	14.074

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		E-15-Heptadecenal	252	C17H32O	1000130-97-9	74
2		Pentafluoropropionic acid, tetra...	360	C17H29F5O2	006222-06-6	58
3		1-Octadecanol	270	C18H38O	000112-92-5	53
4		1-Octadecene	252	C18H36	000112-88-9	52
5		Tetradecyl trifluoroacetate	310	C16H29F3O2	006222-02-2	52

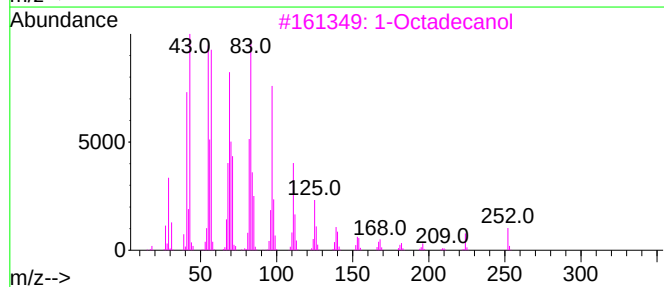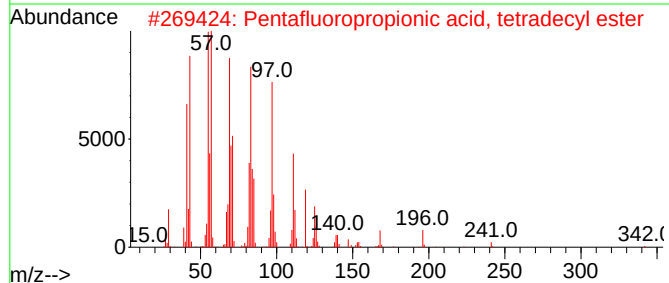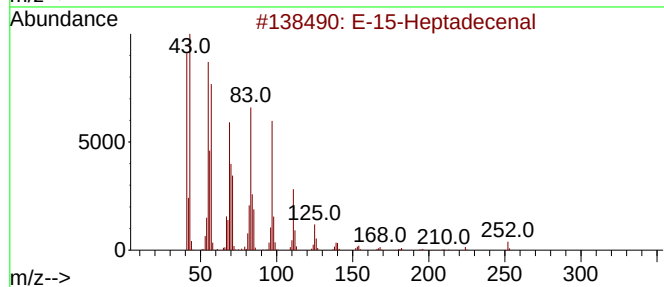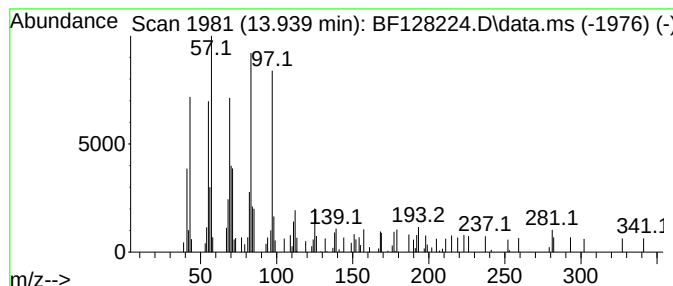

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051222\
Data File : BF128224.D
Acq On : 12 May 2022 19:31
Operator : CG\JU
Sample : N2804-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FETWP-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.116	2.0	ng	44320	1	6.893	433673	20.0
E-15-Heptadecenal	13.939	3.8	ng	89660	5	14.074	468165	20.0