

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051222\
 Data File : BF128229.D
 Acq On : 12 May 2022 21:57
 Operator : CG\JU
 Sample : N2804-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FEDUP

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128229.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.116	478	481	487	rVB	35454	36769	1.77%	0.360%
2	5.516	545	549	561	rBV	796645	719737	34.61%	7.048%
3	6.522	716	720	732	rBV	525386	471825	22.69%	4.620%
4	6.892	780	783	787	rBV	505544	413374	19.88%	4.048%
5	7.463	874	880	883	rBV	1347756	1302756	62.65%	12.757%
6	8.175	997	1001	1005	rBV	522456	483209	23.24%	4.732%
7	9.251	1179	1184	1187	rBV	2281789	2079385	100.00%	20.362%
8	9.933	1296	1300	1312	rVB	559742	477102	22.94%	4.672%
9	10.310	1361	1364	1369	rBV	27305	23721	1.14%	0.232%
10	10.727	1431	1435	1449	rBV	989029	869436	41.81%	8.514%
11	11.427	1550	1554	1560	rBV	544418	443345	21.32%	4.341%
12	13.015	1819	1824	1827	rBV	2352859	2066001	99.36%	20.231%
13	13.933	1976	1980	1988	rBV7	19082	48926	2.35%	0.479%
14	14.074	2000	2004	2010	rBV	491342	429943	20.68%	4.210%
15	14.162	2016	2019	2024	rVB	23917	23945	1.15%	0.234%
16	15.574	2254	2259	2265	rBV	245995	322580	15.51%	3.159%




Sum of corrected areas: 10212054

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051222\
Data File : BF128229.D
Acq On : 12 May 2022 21:57
Operator : CG\JU
Sample : N2804-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FEDUP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

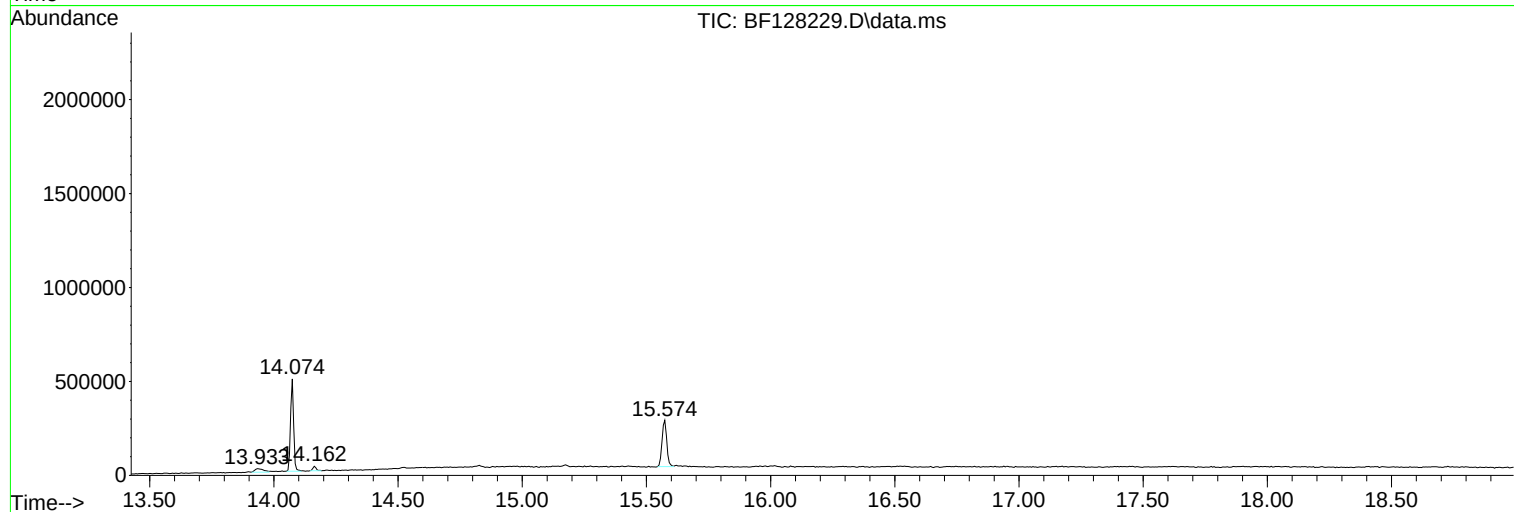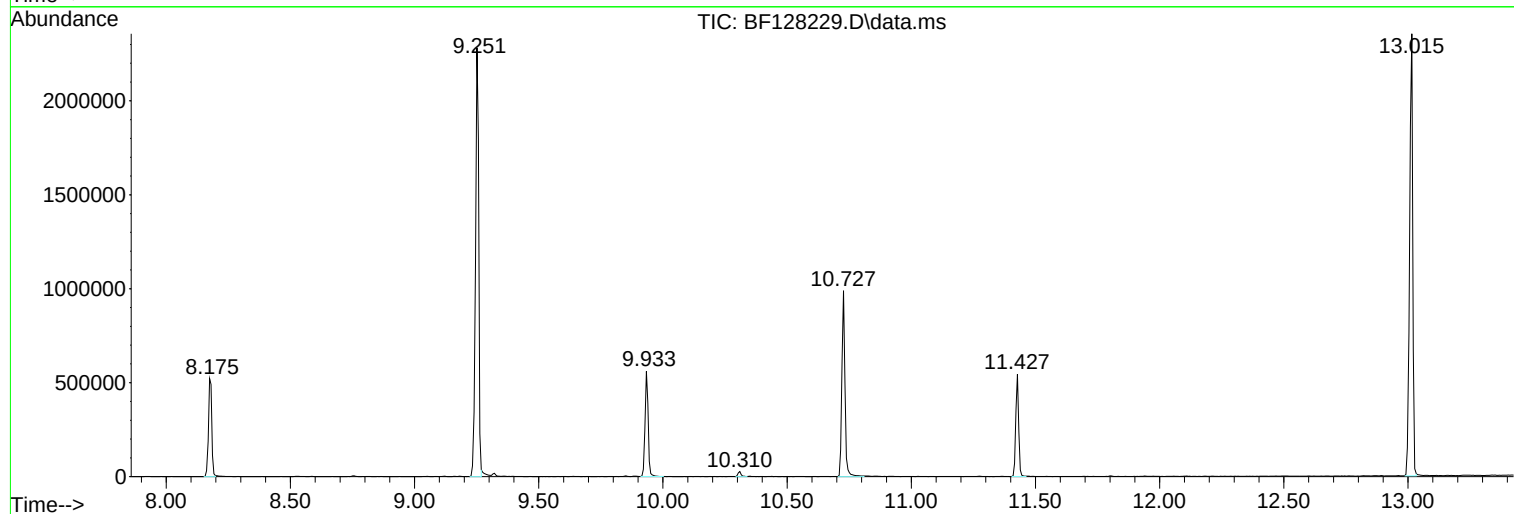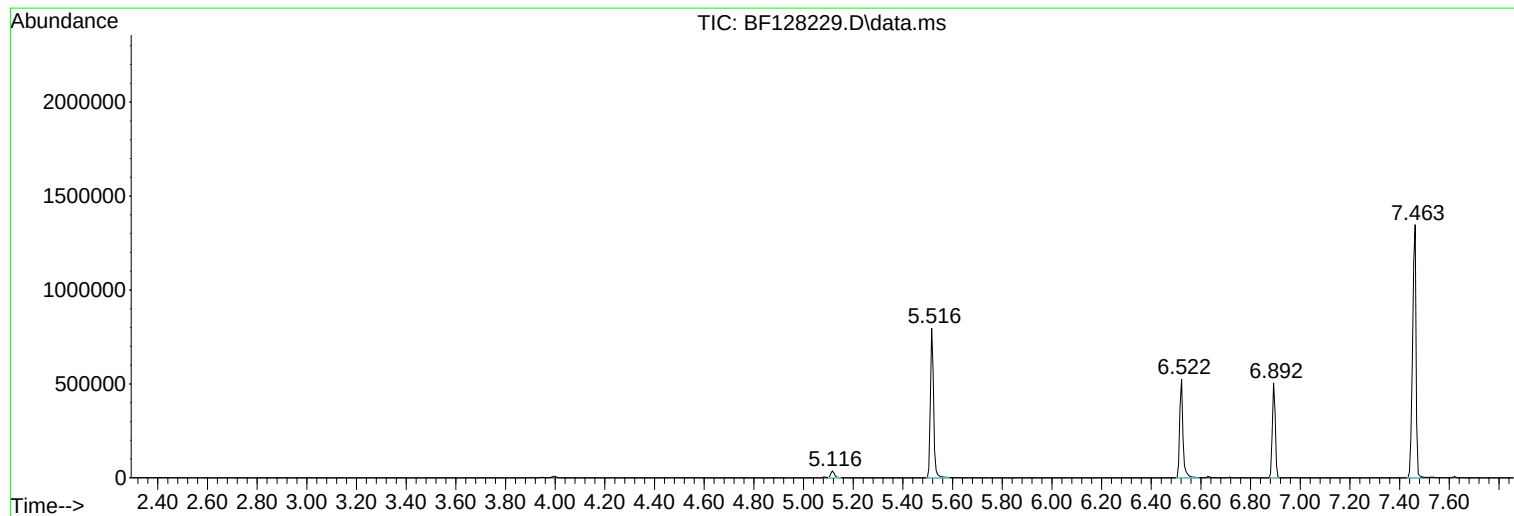

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051222\
Data File : BF128229.D
Acq On : 12 May 2022 21:57
Operator : CG\JU
Sample : N2804-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FEDUP










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1-Hexacosanol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.933	2.28 ng	48926	Chrysene-d12	14.074

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1-Hexacosanol	382	C26H54O	000506-52-5	80
2			Nonadecyl pentafluoropropionate	430	C22H39F5O2	1000351-88-8	64
3			1-Octadecanol	270	C18H38O	000112-92-5	62
4			1-Tetradecanol	214	C14H30O	000112-72-1	52
5			1-Tricosene	322	C23H46	018835-32-0	49

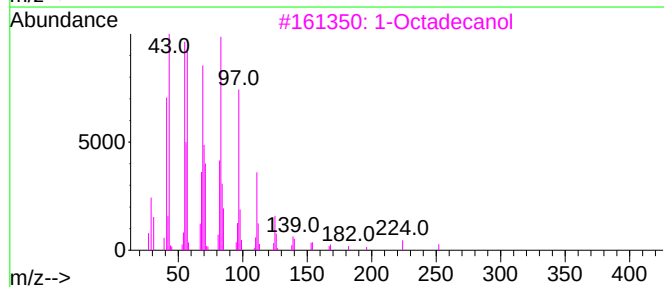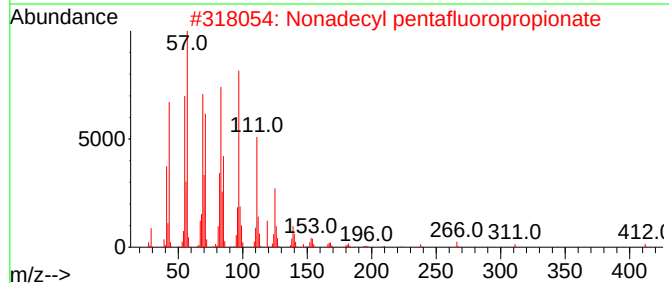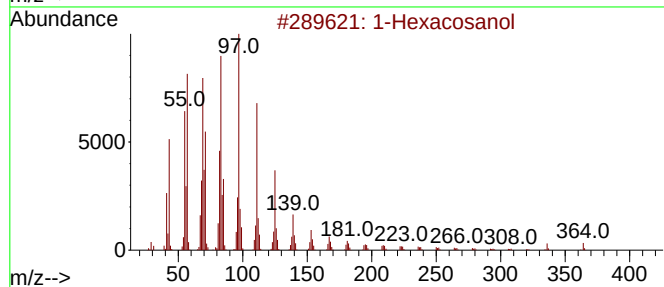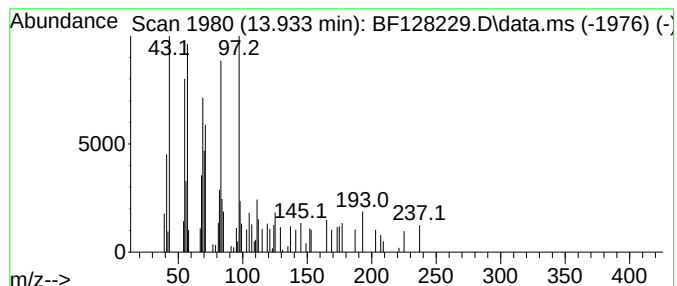

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051222\
Data File : BF128229.D
Acq On : 12 May 2022 21:57
Operator : CG\JU
Sample : N2804-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FEDUP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Hexacosanol	13.933	2.3	ng	48926	5	14.074	429943	20.0