

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051222\
 Data File : BF128230.D
 Acq On : 12 May 2022 22:26
 Operator : CG\JU
 Sample : N2804-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FE-FB-05112022

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128230.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.116	478	481	492	rVB	33604	36833	1.54%	0.334%
2	5.516	546	549	565	rBV	808485	728269	30.39%	6.597%
3	6.522	716	720	737	rBV	473145	442077	18.44%	4.005%
4	6.892	780	783	787	rBV	530622	432724	18.05%	3.920%
5	7.463	874	880	883	rBV	1583386	1543247	64.39%	13.980%
6	8.175	997	1001	1005	rBV	561937	502548	20.97%	4.553%
7	9.251	1179	1184	1187	rBV	2574534	2396736	100.00%	21.712%
8	9.933	1296	1300	1311	rBV	600883	490602	20.47%	4.444%
9	10.727	1431	1435	1449	rBV	1045891	923130	38.52%	8.363%
10	11.427	1550	1554	1561	rBV	557929	455435	19.00%	4.126%
11	13.016	1819	1824	1827	rBV	2671037	2292370	95.65%	20.766%
12	14.074	2000	2004	2010	rBV	510156	456583	19.05%	4.136%
13	15.574	2254	2259	2268	rBV	241849	338235	14.11%	3.064%




Sum of corrected areas: 11038789

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051222\
Data File : BF128230.D
Acq On : 12 May 2022 22:26
Operator : CG\JU
Sample : N2804-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FE-FB-05112022

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

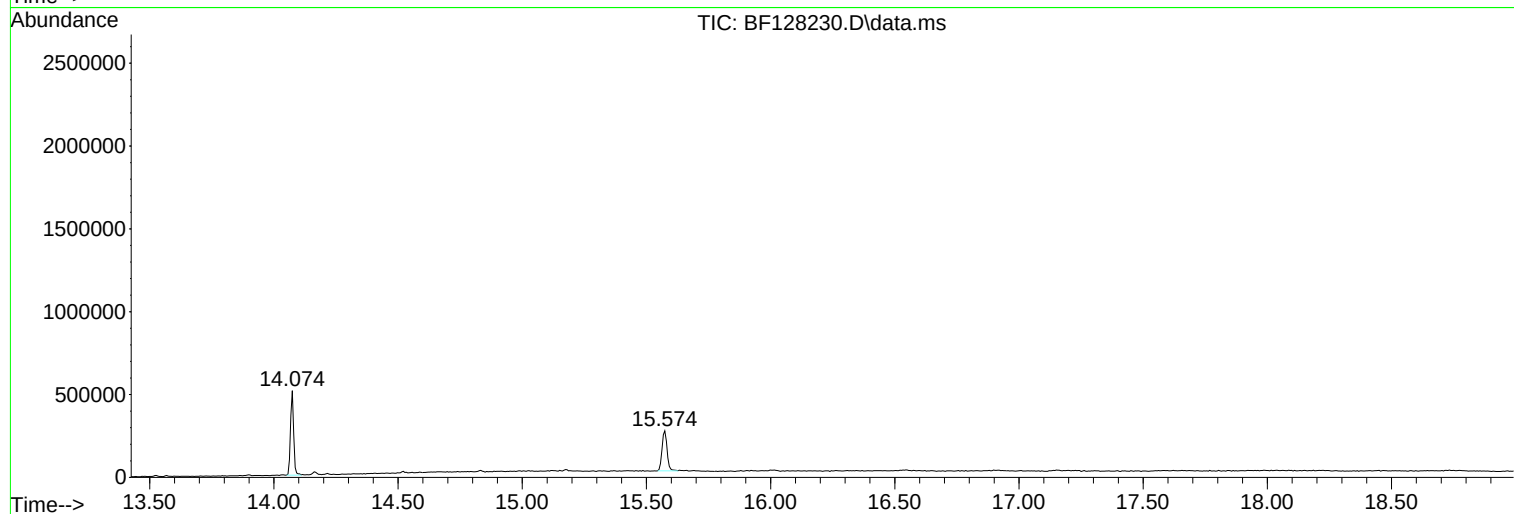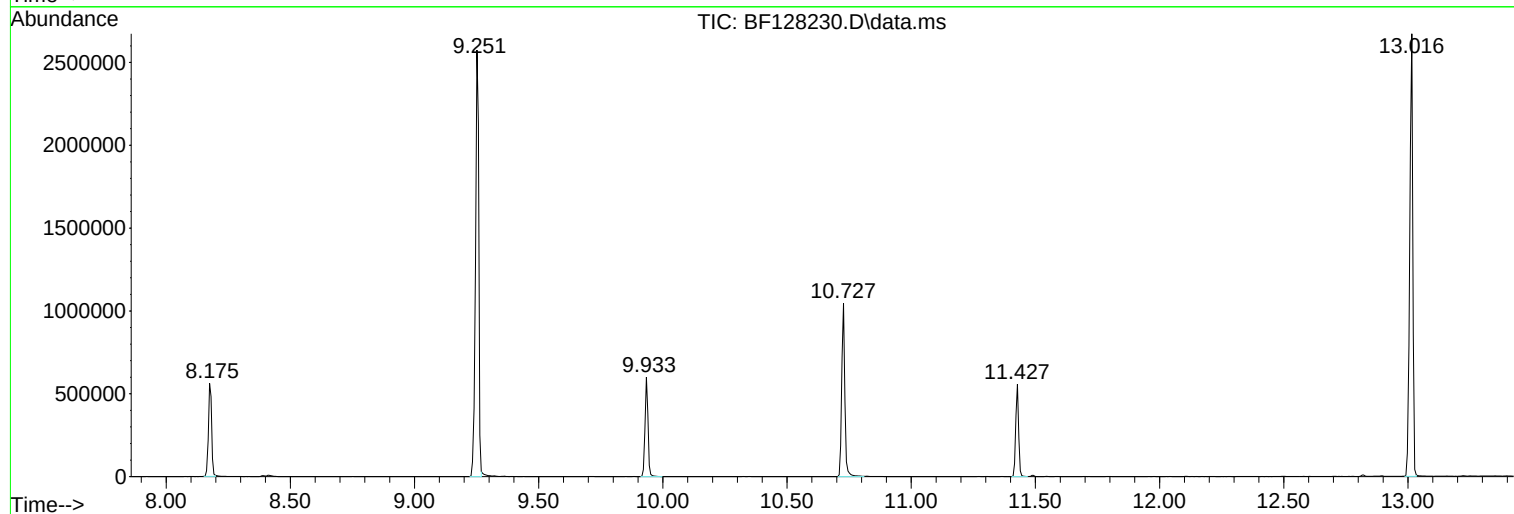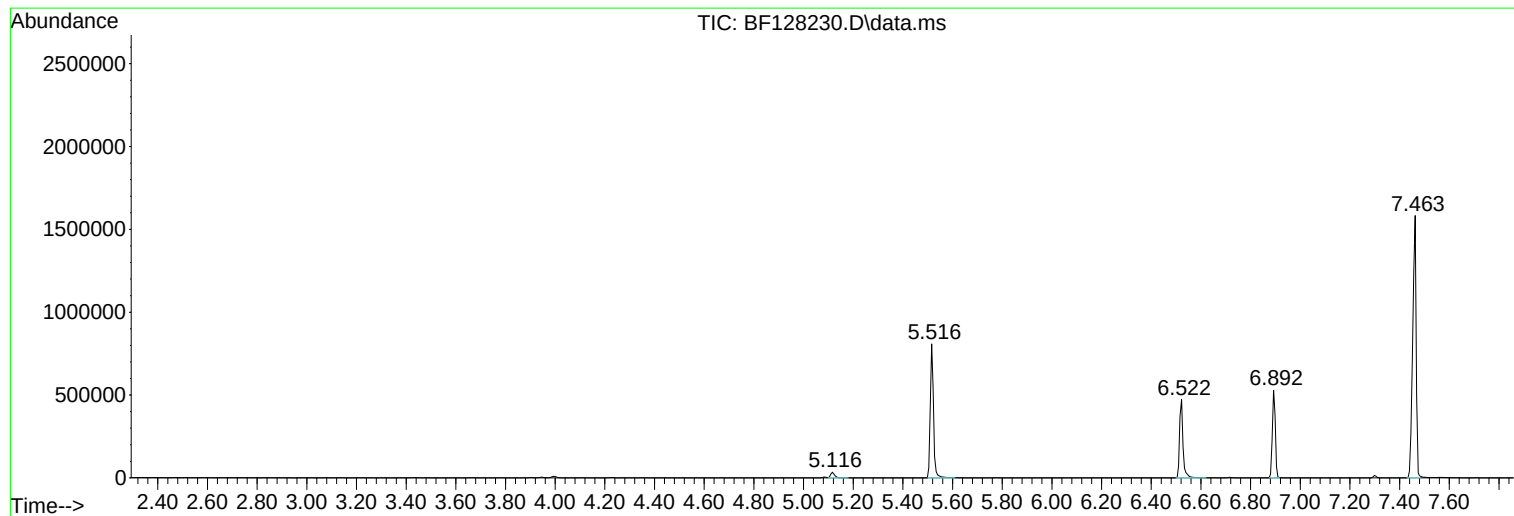

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051222\
Data File : BF128230.D
Acq On : 12 May 2022 22:26
Operator : CG\JU
Sample : N2804-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FE-FB-05112022

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051222\
Data File : BF128230.D
Acq On : 12 May 2022 22:26
Operator : CG\JU
Sample : N2804-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FE-FB-05112022

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------