
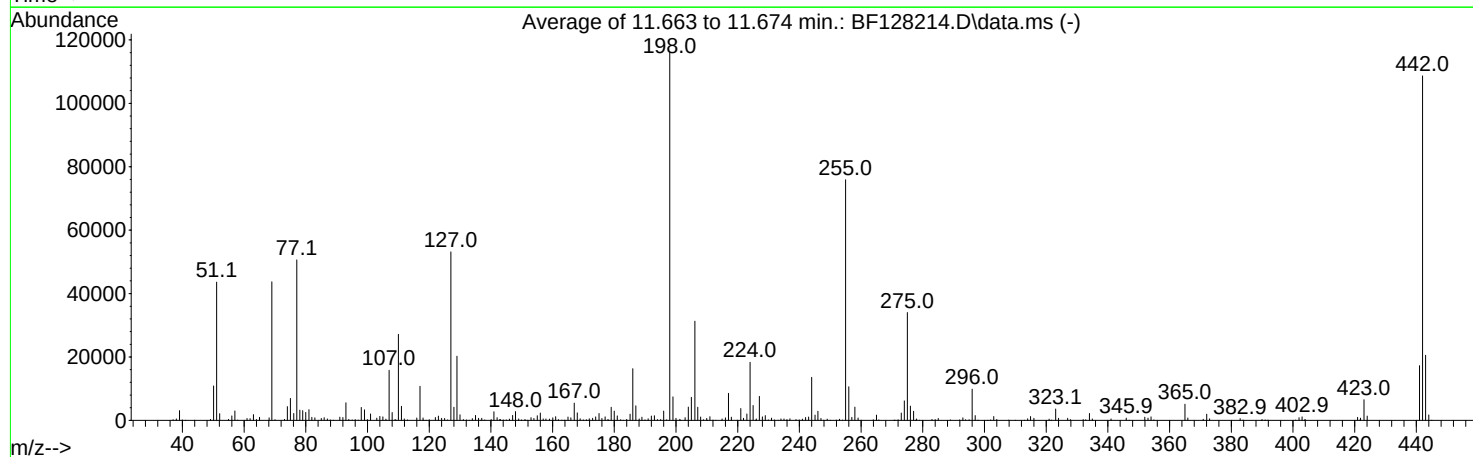


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051222\
 Data File : BF128214.D
 Acq On : 12 May 2022 11:47
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat May 14 00:51:21 2022

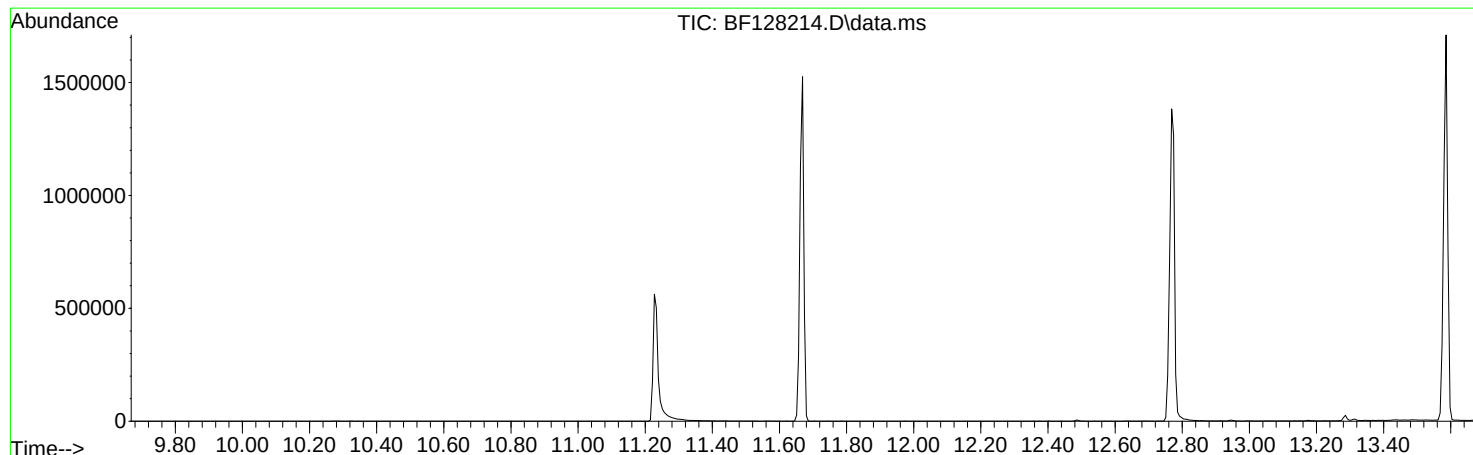

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	43598	PASS
68	69	0.00	2	1.8	800	PASS
69	198	0.00	100	37.7	43696	PASS
70	69	0.00	2	0.4	196	PASS
127	198	10	80	45.8	53134	PASS
197	198	0.00	2	0.2	187	PASS
198	198	100	100	100.0	116040	PASS
199	198	5	9	6.4	7410	PASS
275	198	10	60	29.3	34045	PASS
365	198	1	100	4.4	5084	PASS
441	198	0.01	100	14.9	17264	PASS
442	442	50	100	100.0	108677	PASS
443	442	15	24	18.9	20562	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/12/2022	BNA_F	<u>BF128214.D</u>
Compound Name	Response	Retention Time
DDT	278990	13.586
DDD	6086	13.286
DDE	684	12.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6770	285760	2.37

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051222\
Data File : BF128214.D
Acq On : 12 May 2022 11:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 13 07:25:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 09 15:30:11 2022
Response via : Initial Calibration

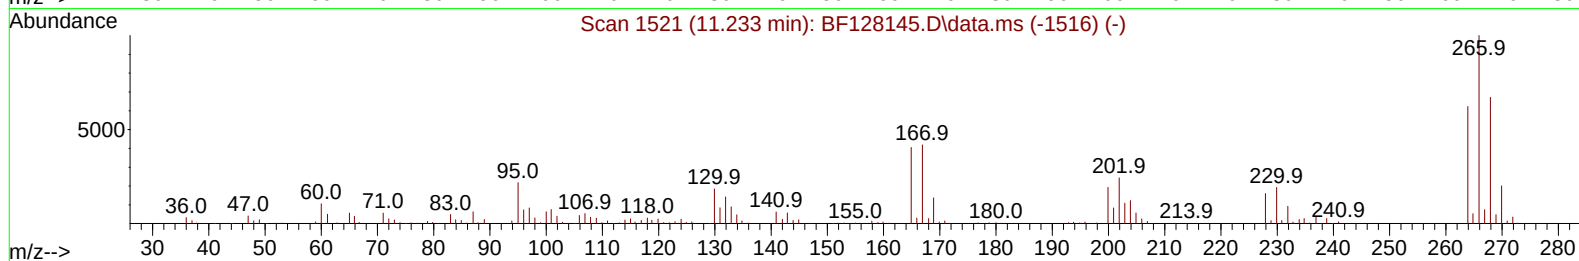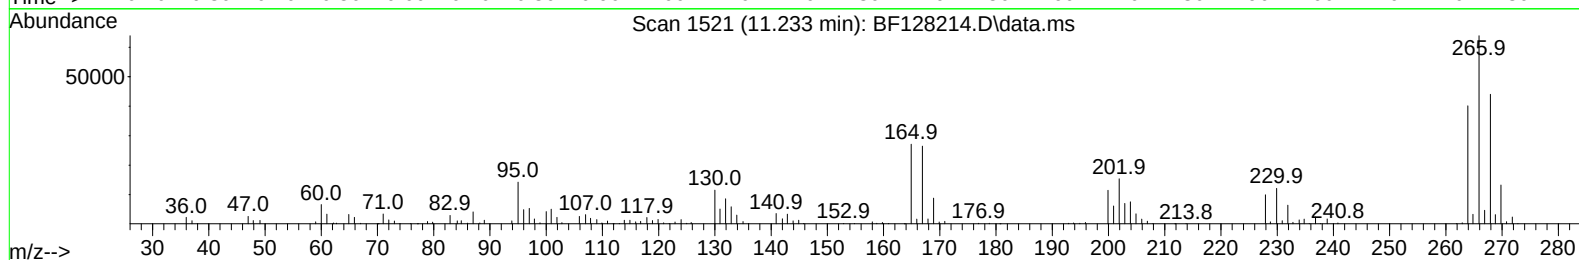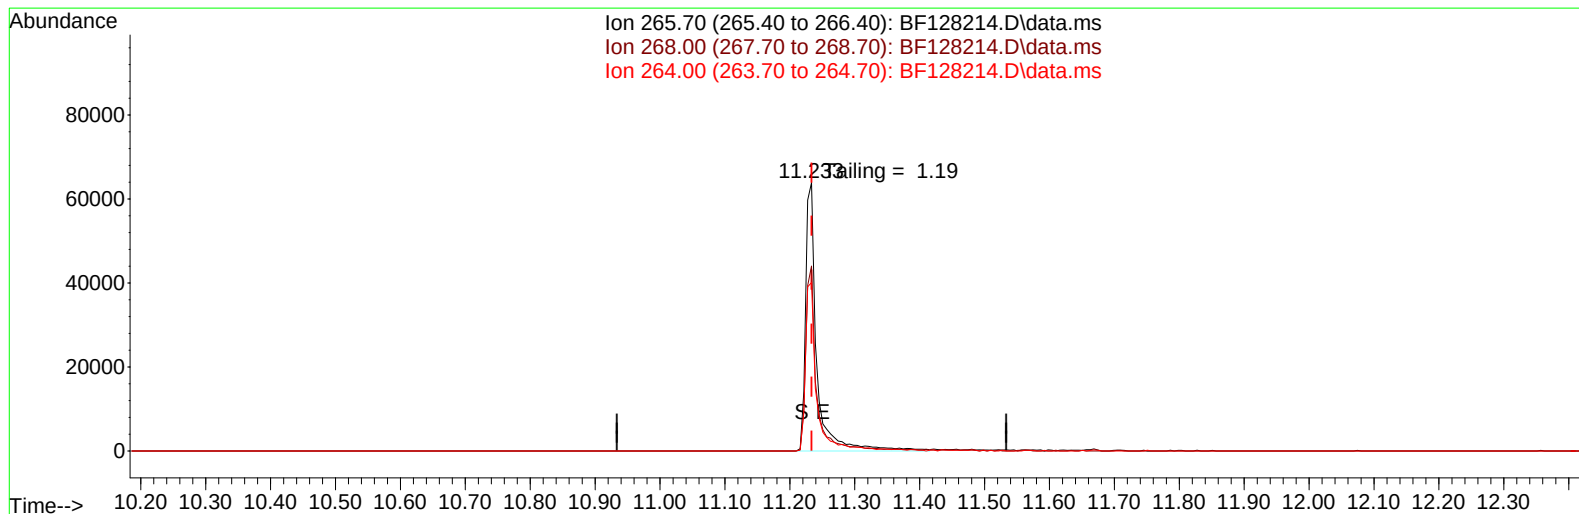

TIC: BF128214.D\data.ms

(70) Pentachlorophenol (C)

11.233min (-0.000) 24101.41 ng




response 77089

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.30	68.92
264.00	66.40	62.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051222\
Data File : BF128214.D
Acq On : 12 May 2022 11:47
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 13 07:25:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 09 15:30:11 2022
Response via : Initial Calibration

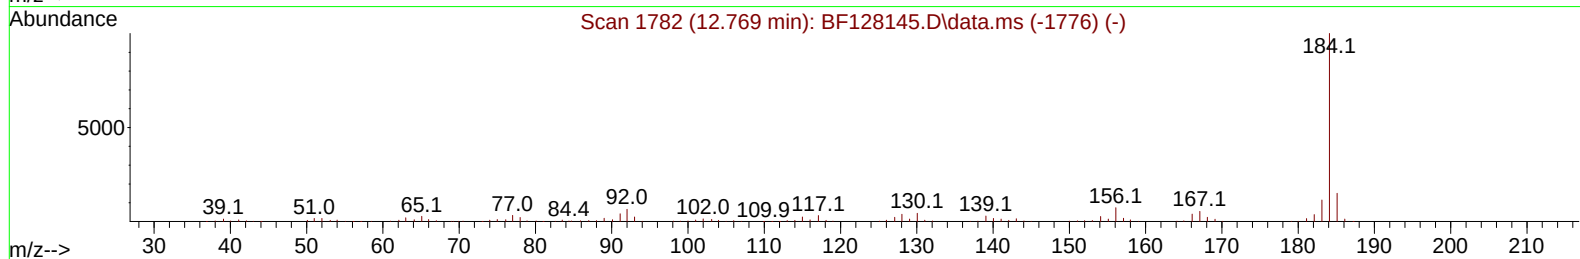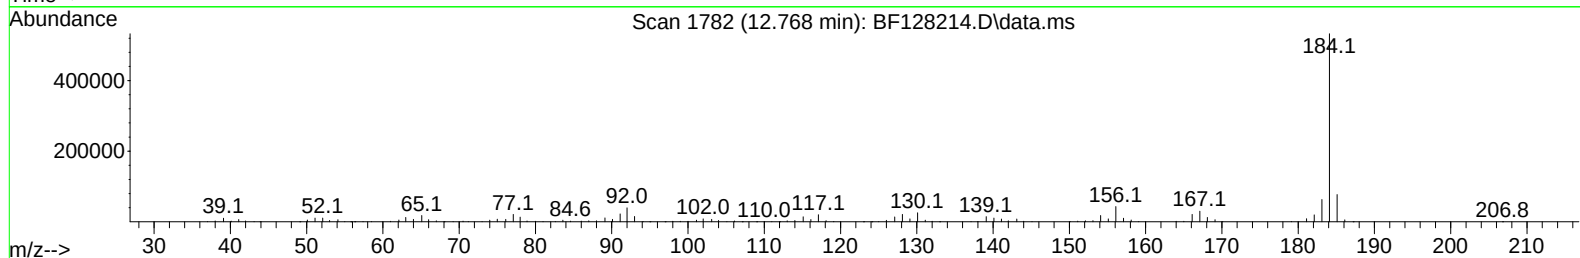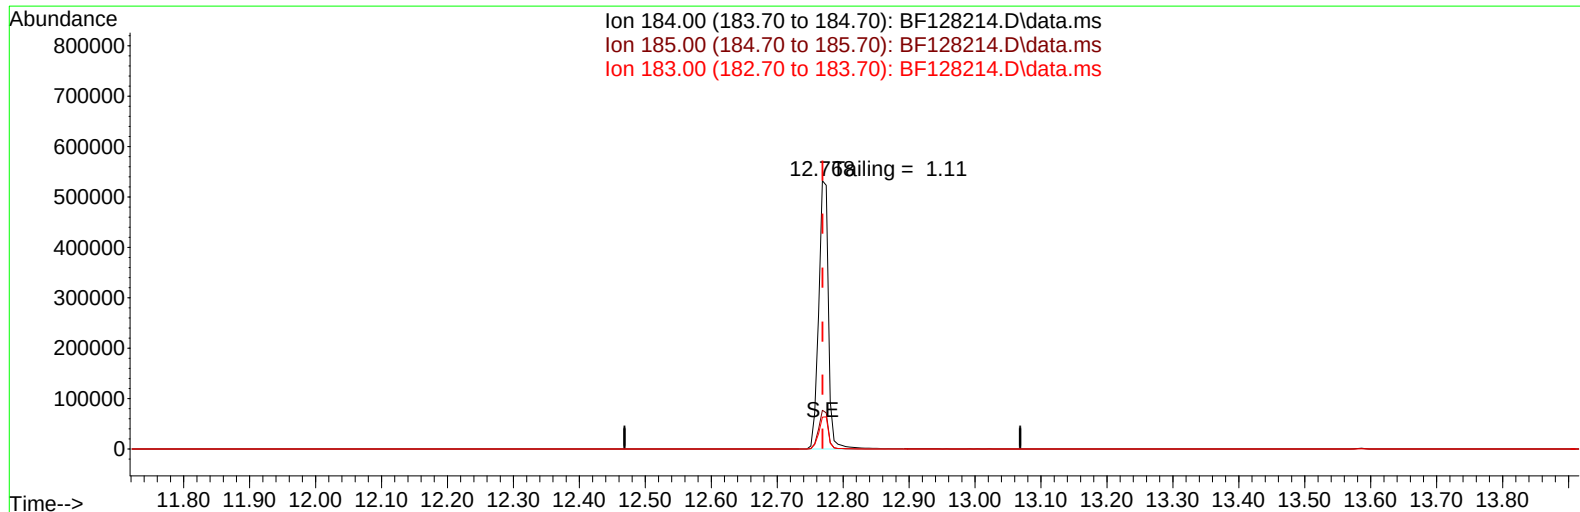

TIC: BF128214.D\data.ms

(77) Benzidine

12.768min (-0.000) 0.00 ng

response 549843

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.10	14.47
183.00	11.20	11.89
0.00	0.00	0.00