
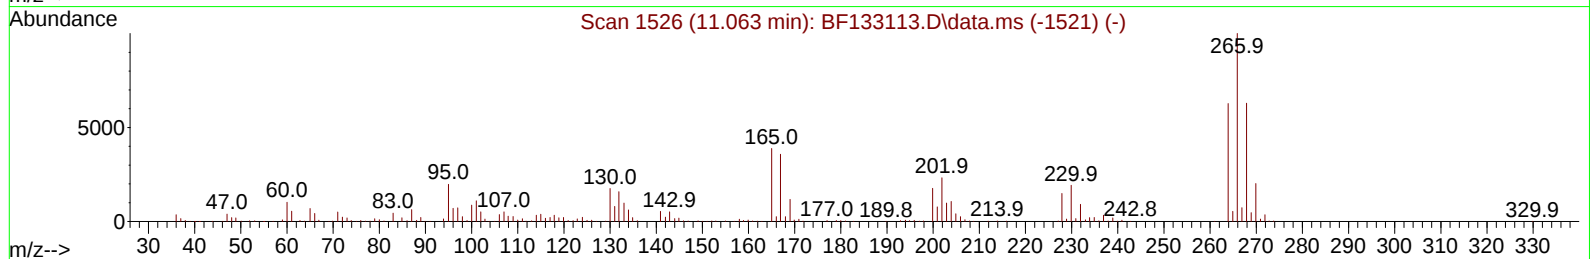
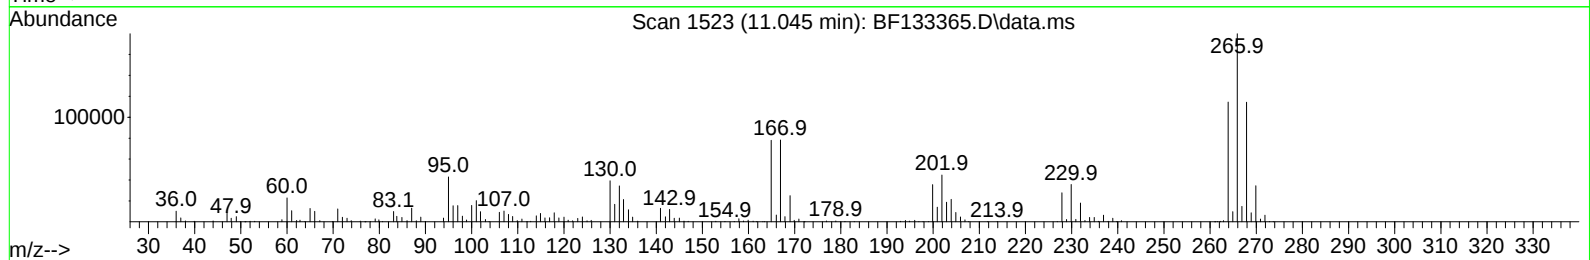


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051223\
Data File : BF133365.D
Acq On : 12 May 2023 12:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 14:23:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 11 16:40:17 2023
Response via : Initial Calibration

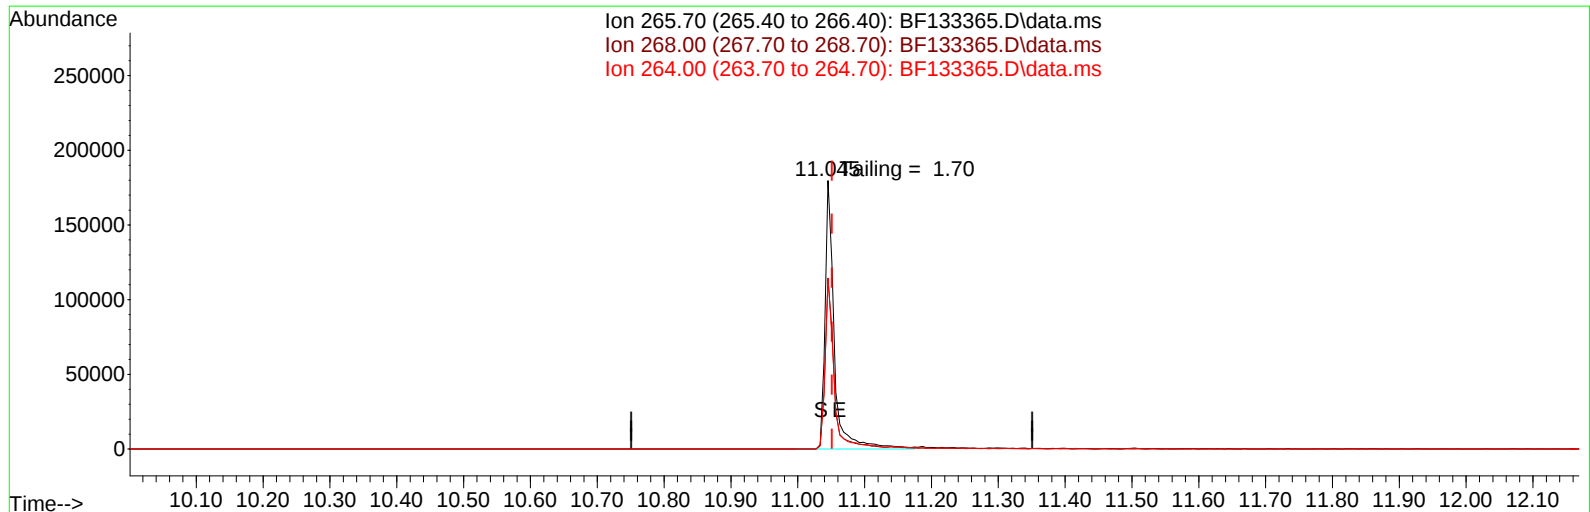

TIC: BF133365.D\data.ms

(70) Pentachlorophenol (C)




11.045min (-0.006) 24224.31 ng

response 172942

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	63.61
264.00	63.30	63.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051223\
Data File : BF133365.D
Acq On : 12 May 2023 12:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 12 14:23:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 11 16:40:17 2023
Response via : Initial Calibration

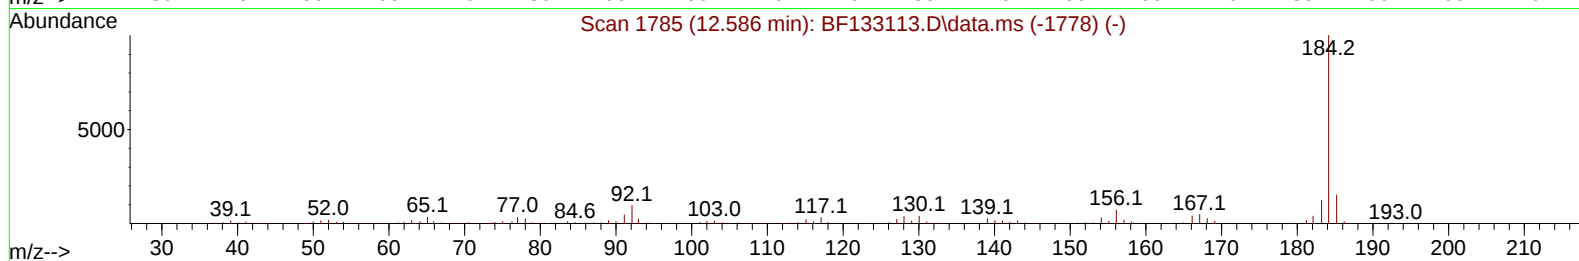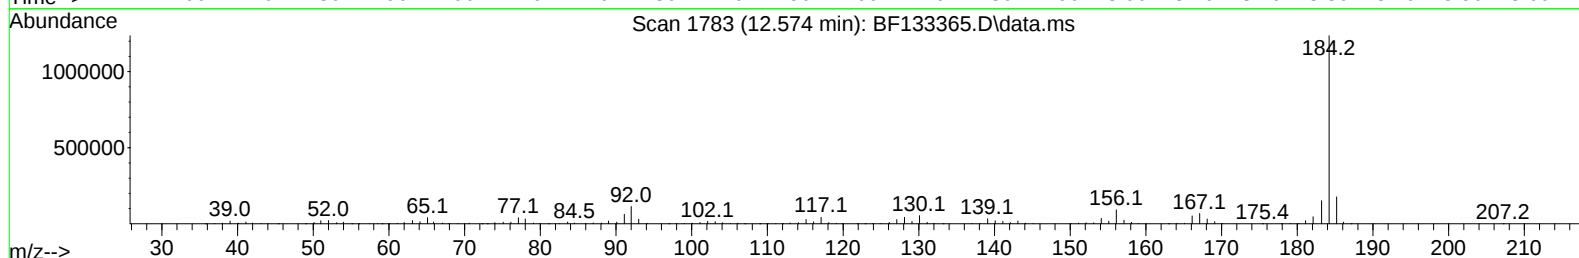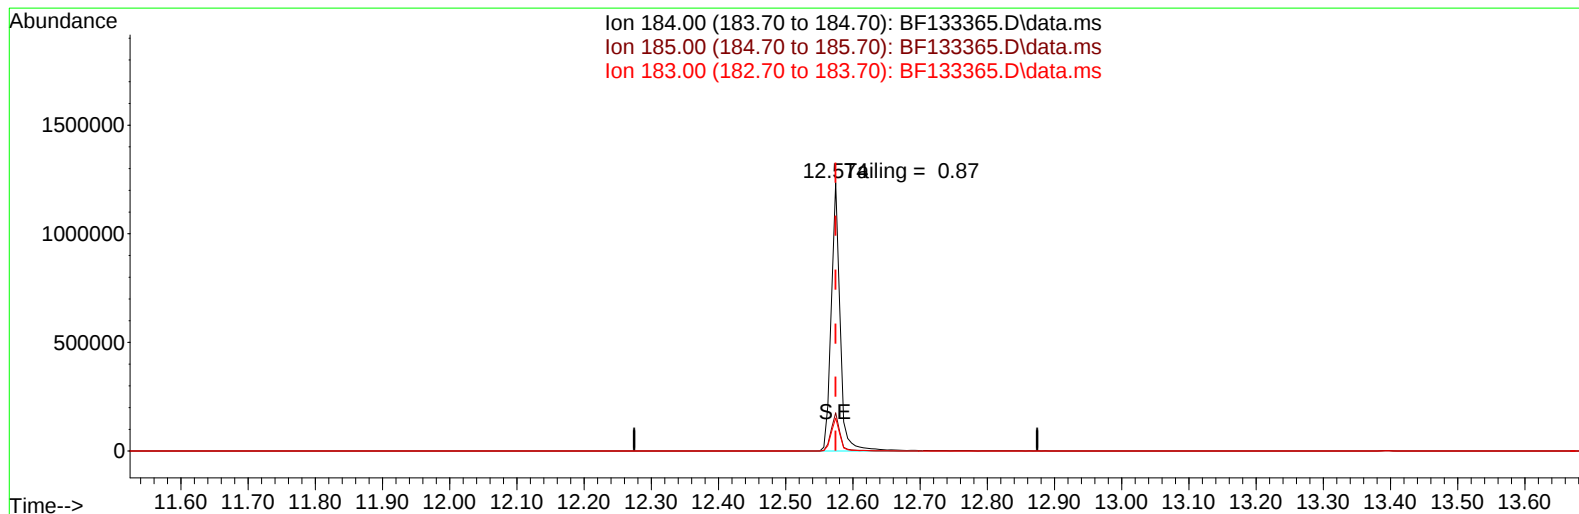

TIC: BF133365.D\data.ms

(77) Benzidine

12.574min (+ 0.000) 0.00 ng

response 1137703

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.28#
183.00	11.70	12.28
0.00	0.00	0.00