
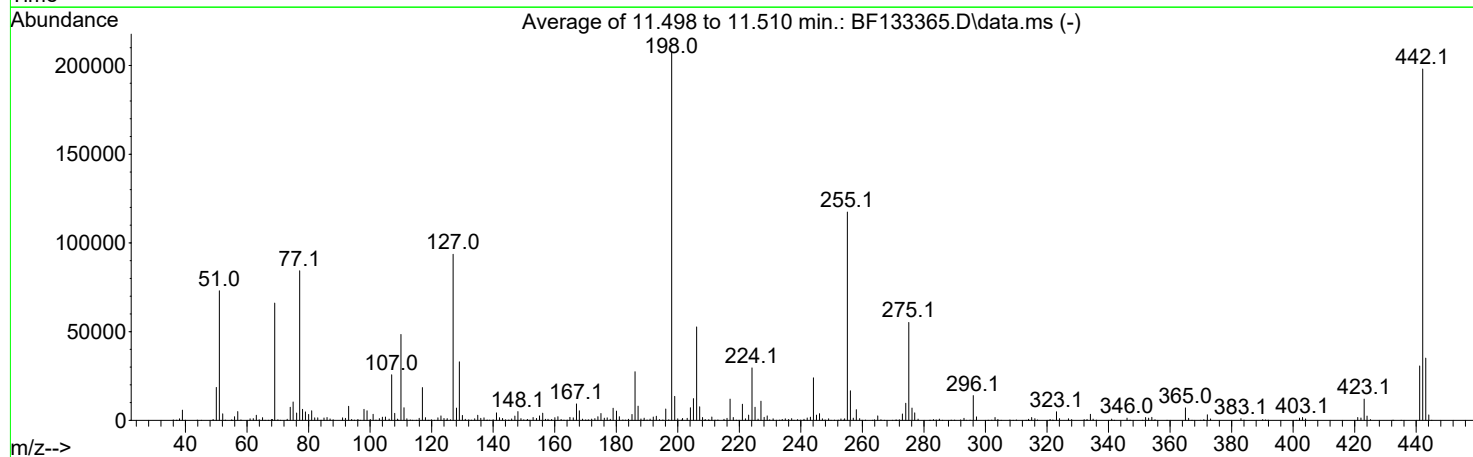


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051223\
Data File : BF133365.D
Acq On : 12 May 2023 12:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu May 11 16:40:17 2023

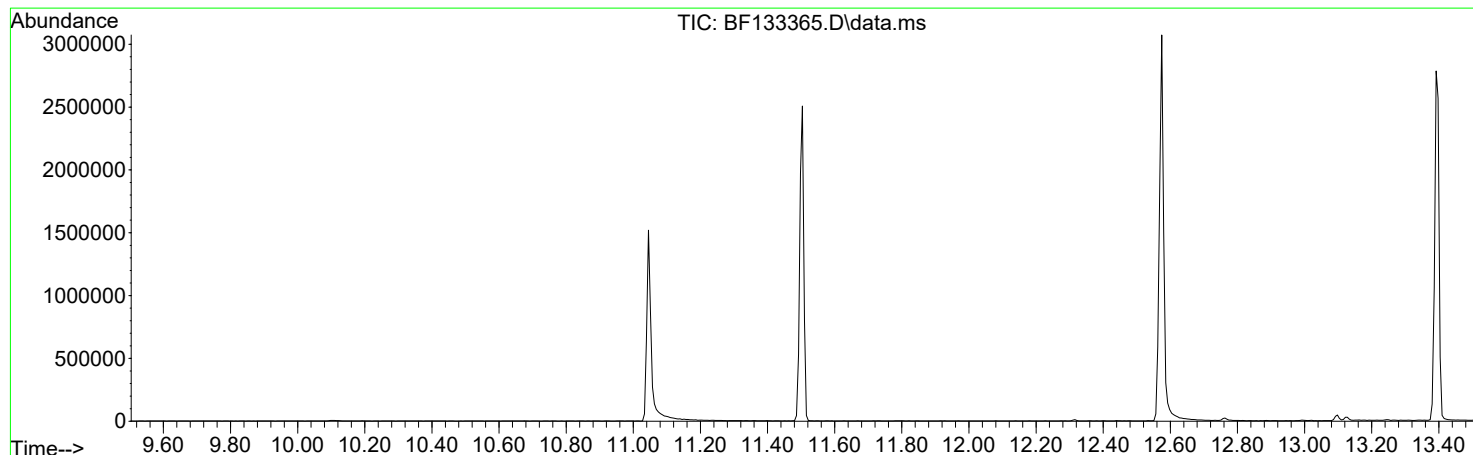

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	73019	PASS
68	69	0.00	2	0.8	559	PASS
69	198	0.00	100	31.9	66067	PASS
70	69	0.00	2	0.6	390	PASS
127	198	10	80	45.2	93640	PASS
197	198	0.00	2	0.2	394	PASS
198	198	100	100	100.0	207323	PASS
199	198	5	9	6.5	13569	PASS
275	198	10	60	26.6	55203	PASS
365	198	1	100	3.4	7085	PASS
441	198	0.01	100	14.8	30709	PASS
442	442	50	100	100.0	198067	PASS
443	442	15	24	17.7	35117	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/12/2023	BNA_F	<u>BF133365.D</u>
Compound Name	Response	Retention Time
DDT	490411	13.398
DDD	12956	13.098
DDE	2949	12.763
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15905	506316	3.14

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051223\
Data File : BF133365.D
Acq On : 12 May 2023 12:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 12 14:23:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 11 16:40:17 2023
Response via : Initial Calibration

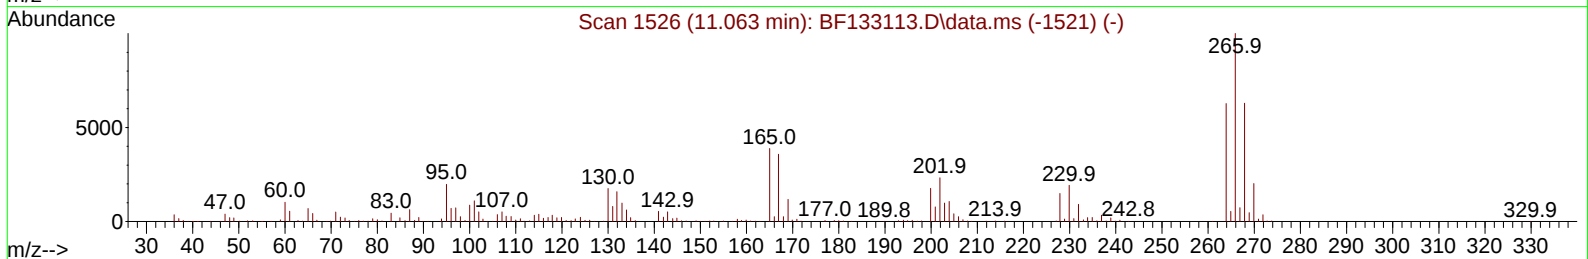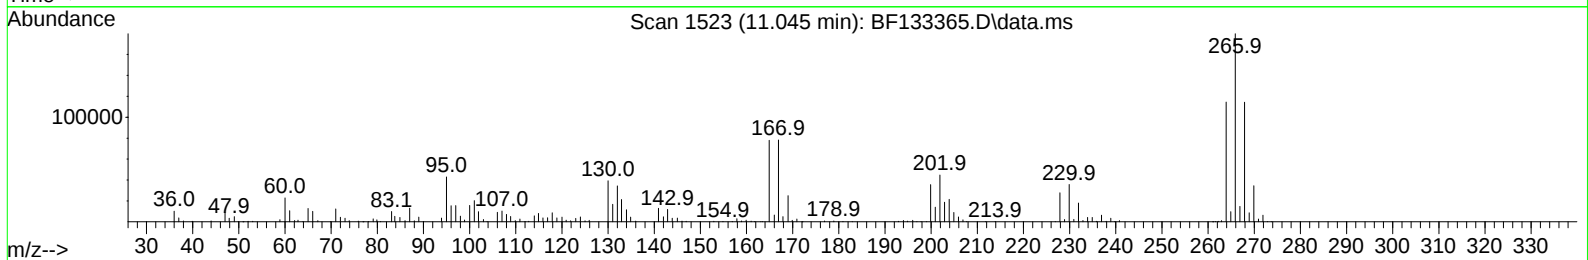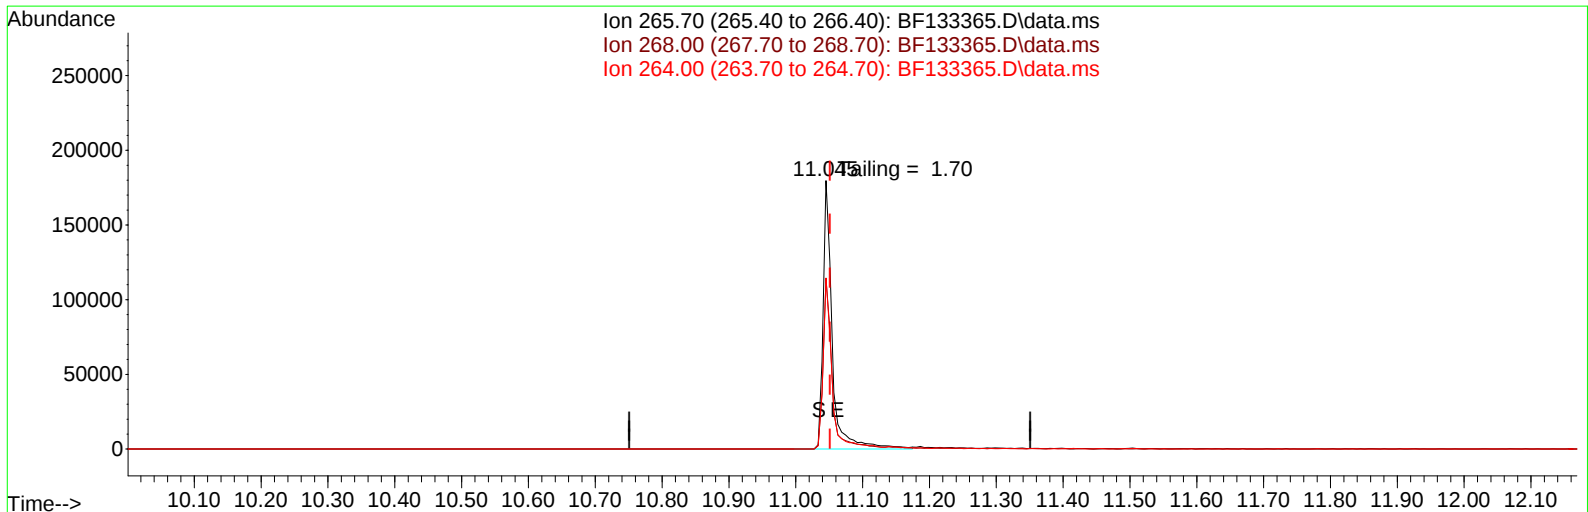

TIC: BF133365.D\data.ms

(70) Pentachlorophenol (C)

11.045min (-0.006) 24224.31 ng




response 172942

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	63.61
264.00	63.30	63.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051223\
Data File : BF133365.D
Acq On : 12 May 2023 12:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 12 14:23:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF042123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 11 16:40:17 2023
Response via : Initial Calibration

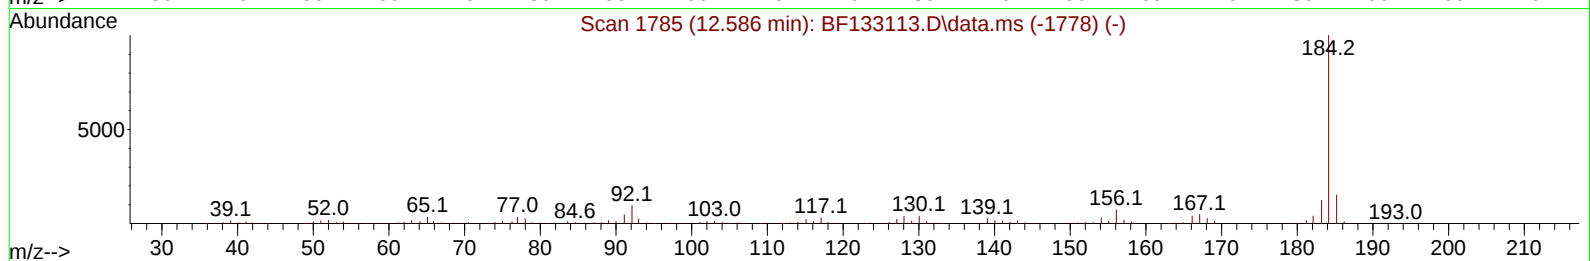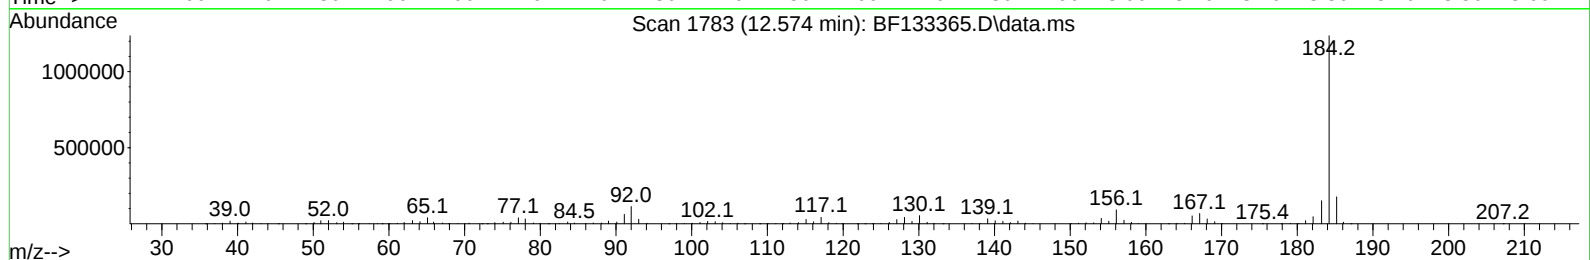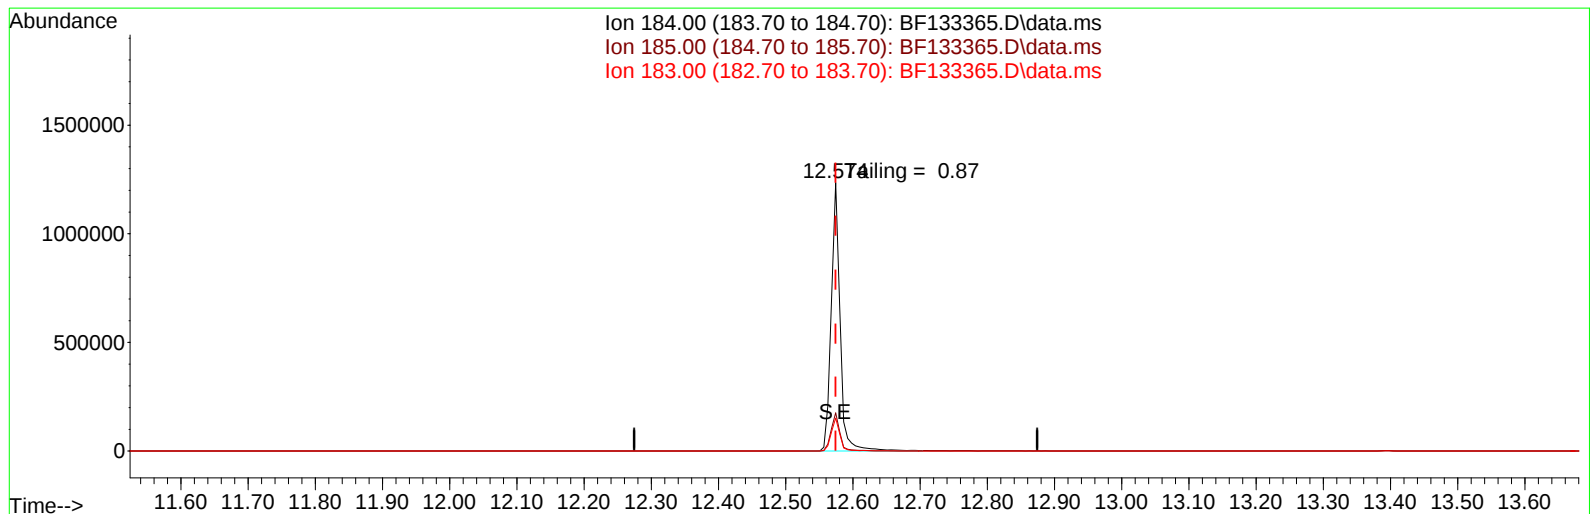

TIC: BF133365.D\data.ms

(77) Benzidine

12.574min (+ 0.000) 0.00 ng

response 1137703

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	19.30	14.28#
183.00	11.70	12.28
0.00	0.00	0.00