
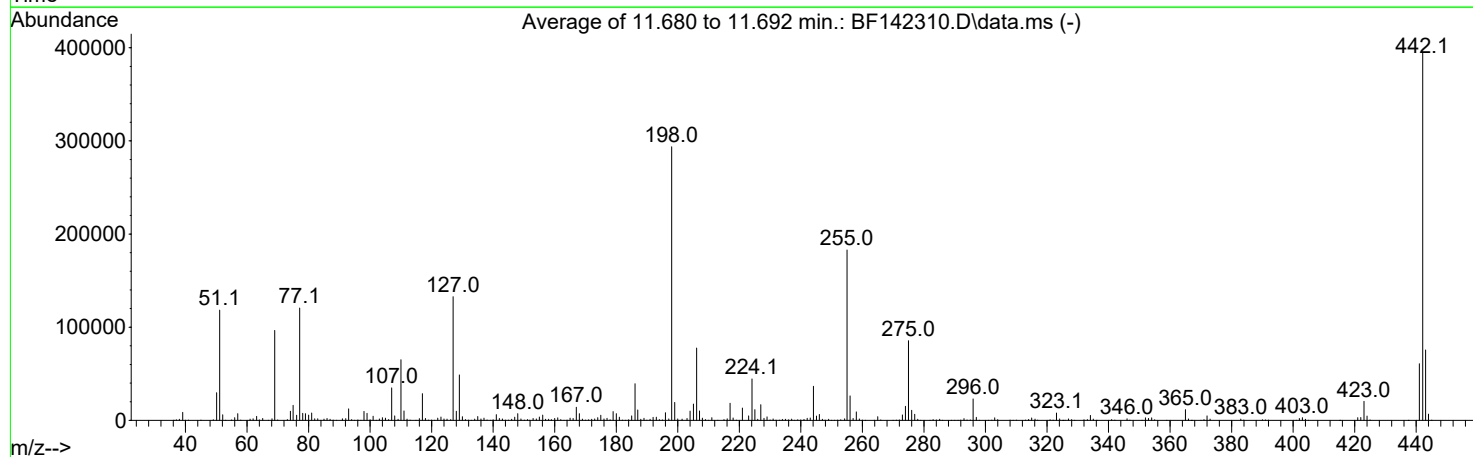


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051225\
Data File : BF142310.D
Acq On : 12 May 2025 10:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon May 05 18:41:44 2025

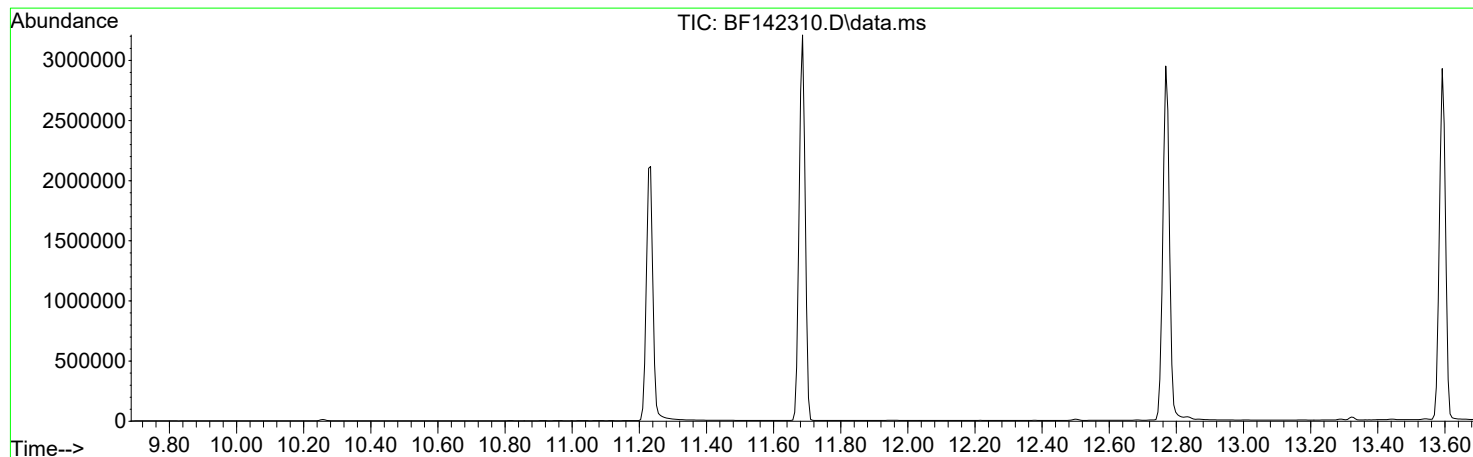

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	118373	PASS
68	69	0.00	2	1.9	1819	PASS
69	198	0.00	100	32.9	96499	PASS
70	69	0.00	2	0.6	555	PASS
127	198	10	80	45.2	132835	PASS
197	198	0.00	2	0.5	1490	PASS
198	198	100	100	100.0	293675	PASS
199	198	5	9	6.6	19341	PASS
275	198	10	60	29.1	85581	PASS
365	198	1	100	3.9	11453	PASS
441	198	0.01	100	20.7	60816	PASS
442	442	50	100	100.0	394880	PASS
443	442	15	24	19.1	75560	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/12/2025	BNA_F	<u>BF142310.D</u>
Compound Name	Response	Retention Time
DDT	594663	13.592
DDD	6529	13.322
DDE	451	12.957
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6980	601643	1.16

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051225\
Data File : BF142310.D
Acq On : 12 May 2025 10:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 12 12:07:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 05 18:41:44 2025
Response via : Initial Calibration

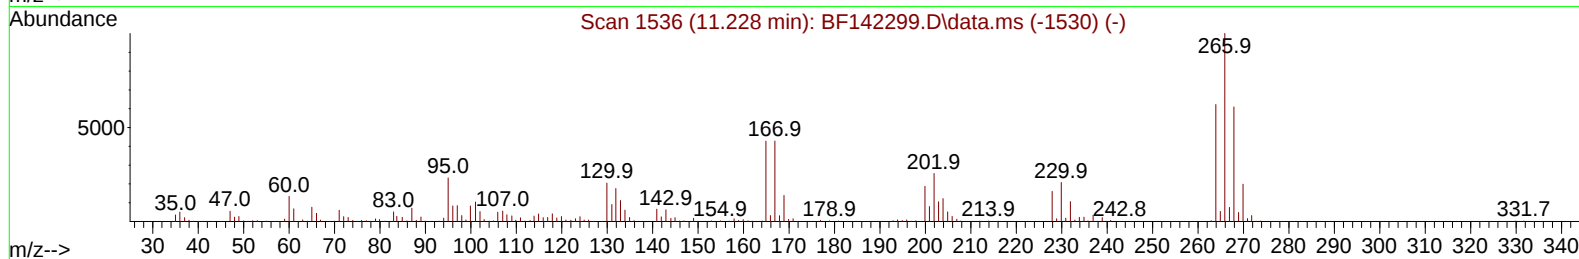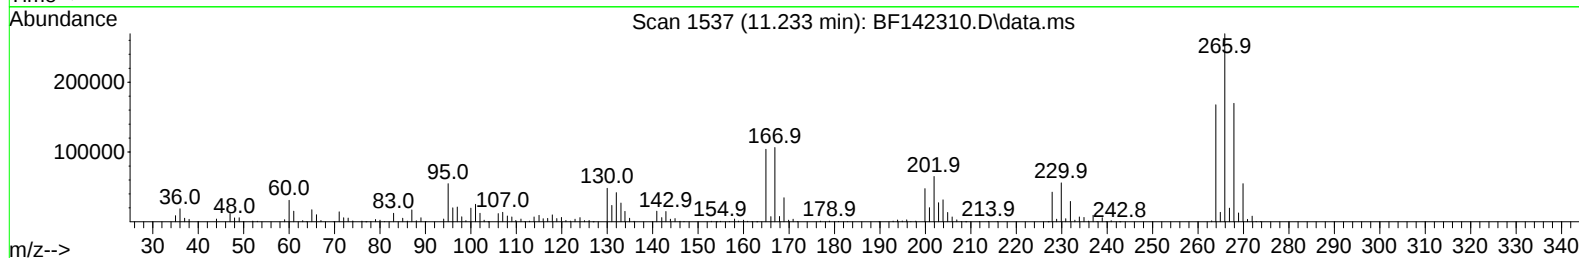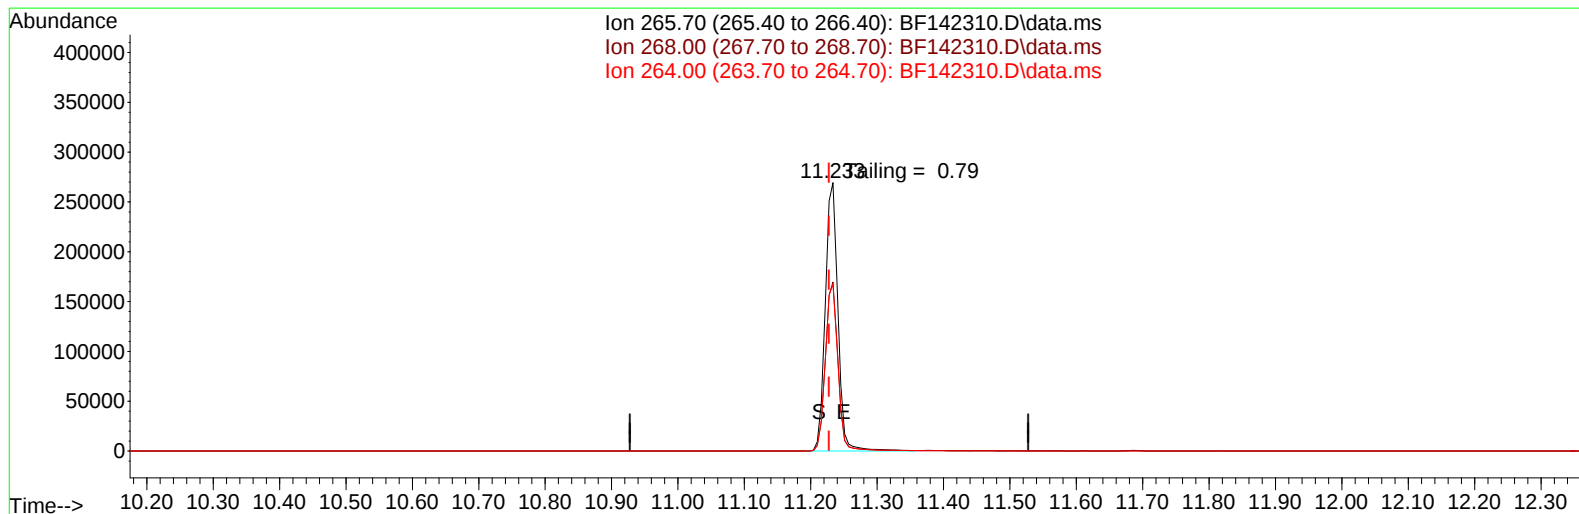

TIC: BF142310.D\data.ms

(70) Pentachlorophenol (C)

11.233min (+ 0.006) 470585.45 ng


response 358000

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	60.90	62.98
264.00	62.20	62.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF051225\
Data File : BF142310.D
Acq On : 12 May 2025 10:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 12 12:07:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF050525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 05 18:41:44 2025
Response via : Initial Calibration

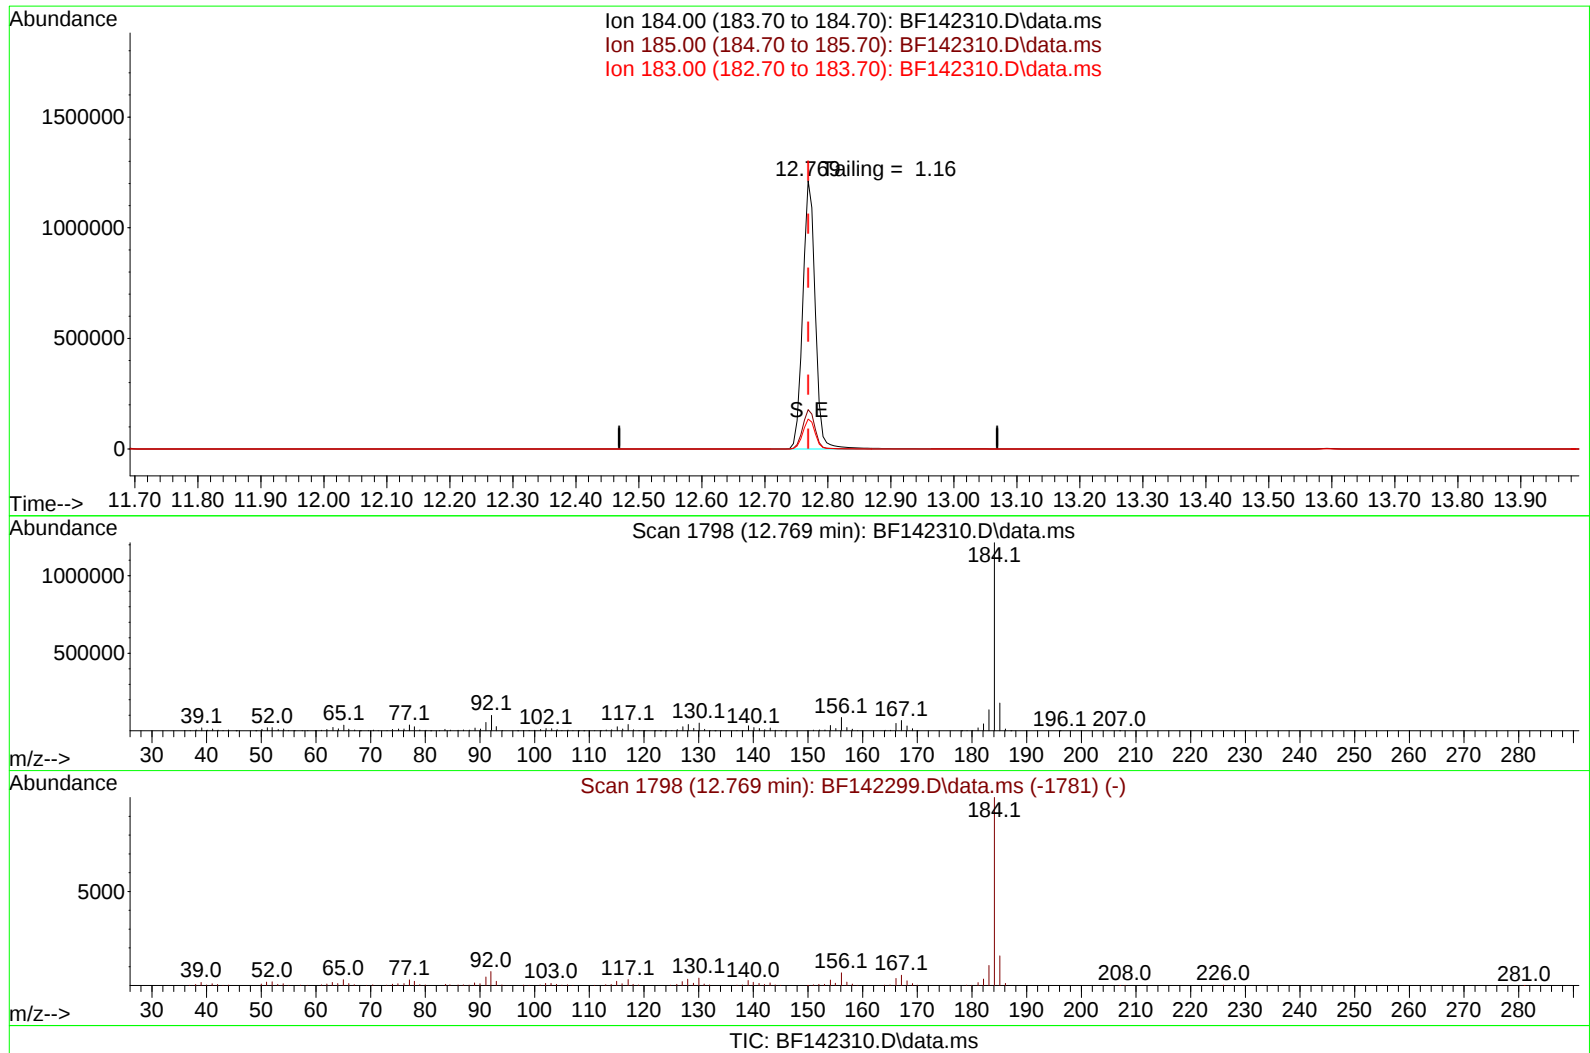

(77) Benzidine

12.769min (-0.000) 0.00 ng

response 1686596

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.71
183.00	10.70	11.17
0.00	0.00	0.00