


Data Path : Z:\HPCHEM1\BNA\_F\Data\BF051315\  
 Data File : BF079196.D  
 Acq On : 13 May 2015 15:03  
 Operator : TP/IZ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF043015.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Apr 30 19:07:47 2015

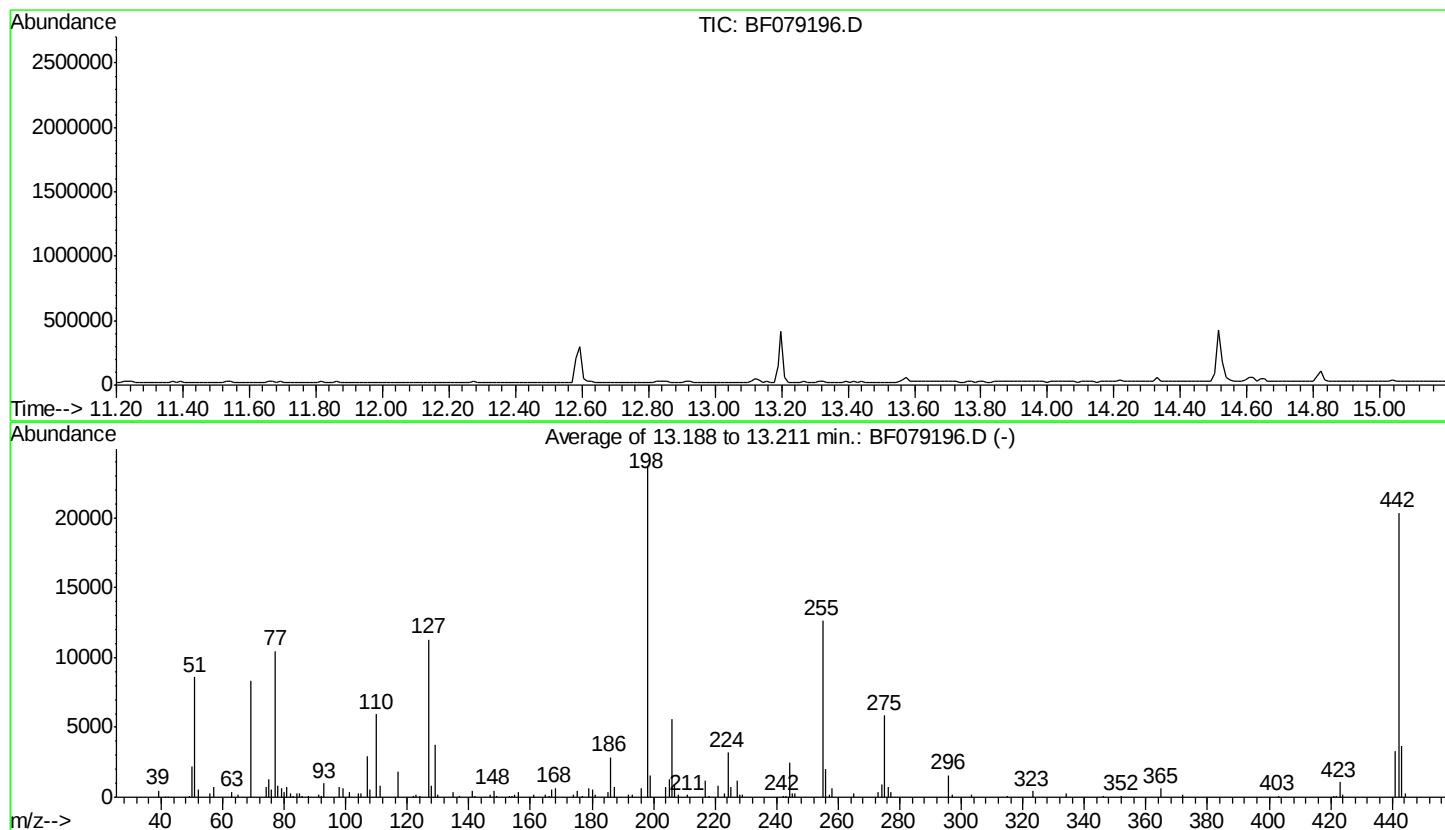

AutoFind: Scans 1050, 1051, 1052; Background Corrected with Scan 1047

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 36.1         | 8572       | PASS                |
| 68             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 69             | 198             | 0.00            | 100             | 35.3         | 8370       | PASS                |
| 70             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 127            | 198             | 10              | 80              | 47.7         | 11321      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 23741      | PASS                |
| 199            | 198             | 5               | 9               | 6.5          | 1545       | PASS                |
| 275            | 198             | 10              | 60              | 24.7         | 5857       | PASS                |
| 365            | 198             | 1               | 100             | 2.5          | 599        | PASS                |
| 441            | 442             | 0.01            | 24              | 16.4         | 3345       | PASS                |
| 442            | 198             | 50              | 100             | 85.8         | 20367      | PASS                |
| 443            | 442             | 15              | 24              | 18.0         | 3667       | PASS                |