
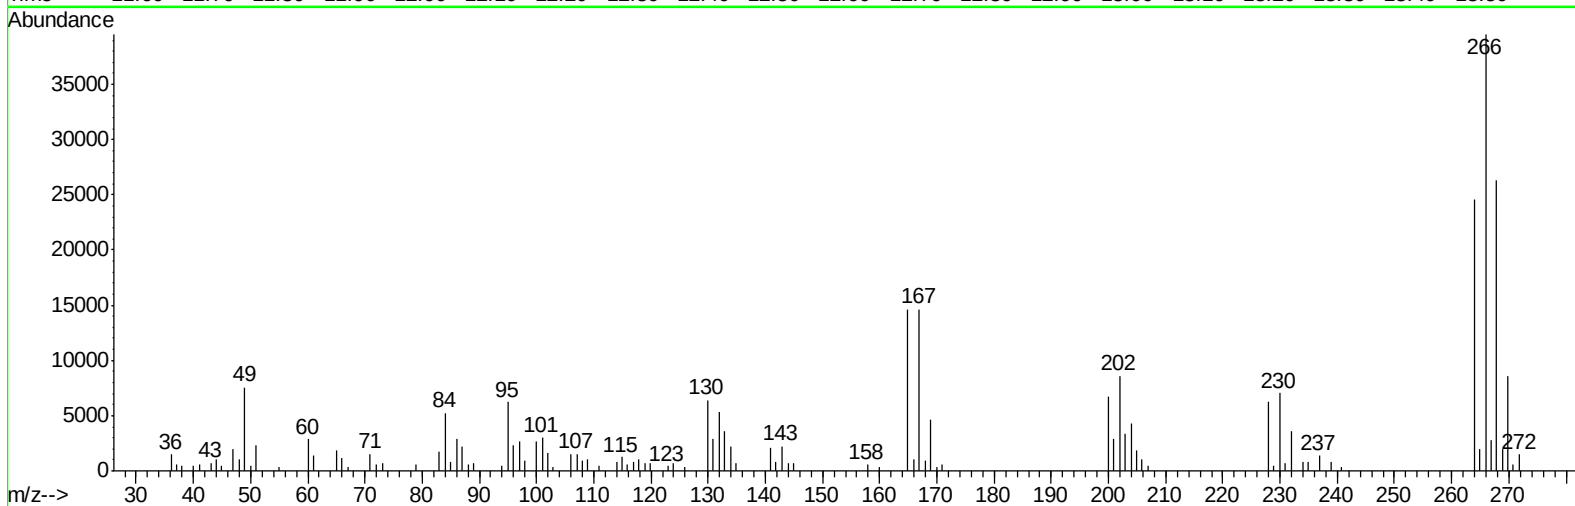


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051315\
Data File : BF079196.D
Acq On : 13 May 2015 15:03
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 14 05:41:15 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 14 00:58:22 2015
Response via : Initial Calibration

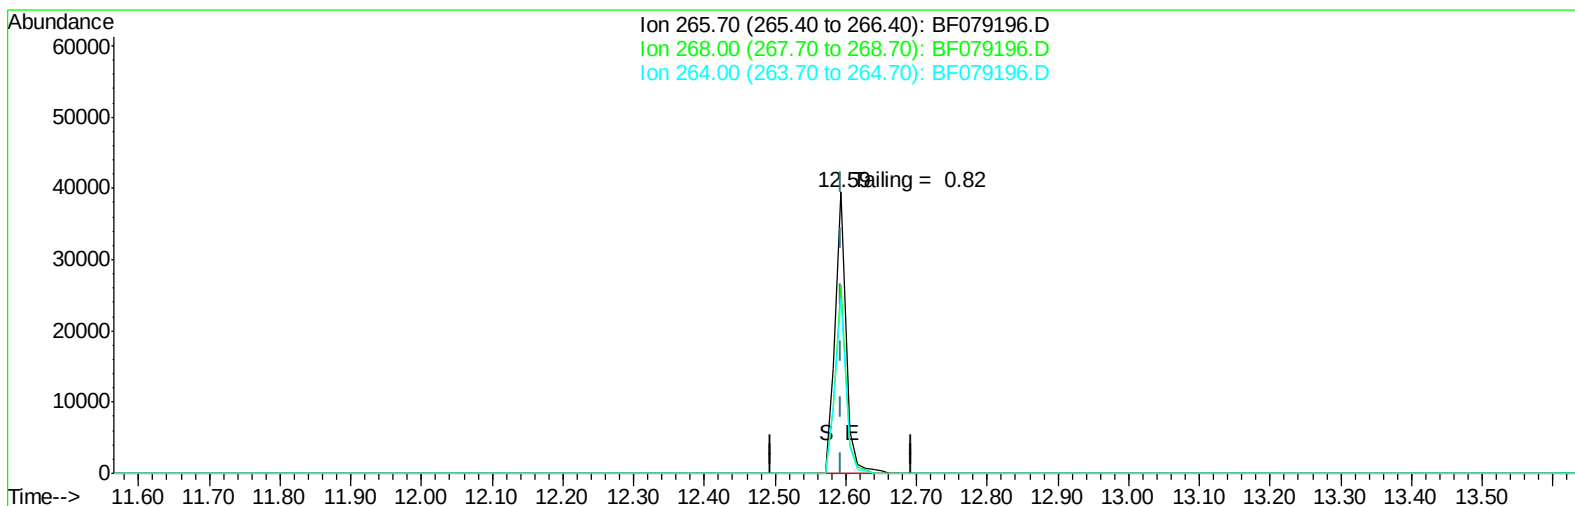

TIC: BF079196.D

(69) Pentachlorophenol (C)



12.594min (+0.000) 2157.77ng

response 42888

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	66.70
264.00	60.20	62.21
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051315\
Data File : BF079196.D
Acq On : 13 May 2015 15:03
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 14 05:41:15 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 14 00:58:22 2015
Response via : Initial Calibration

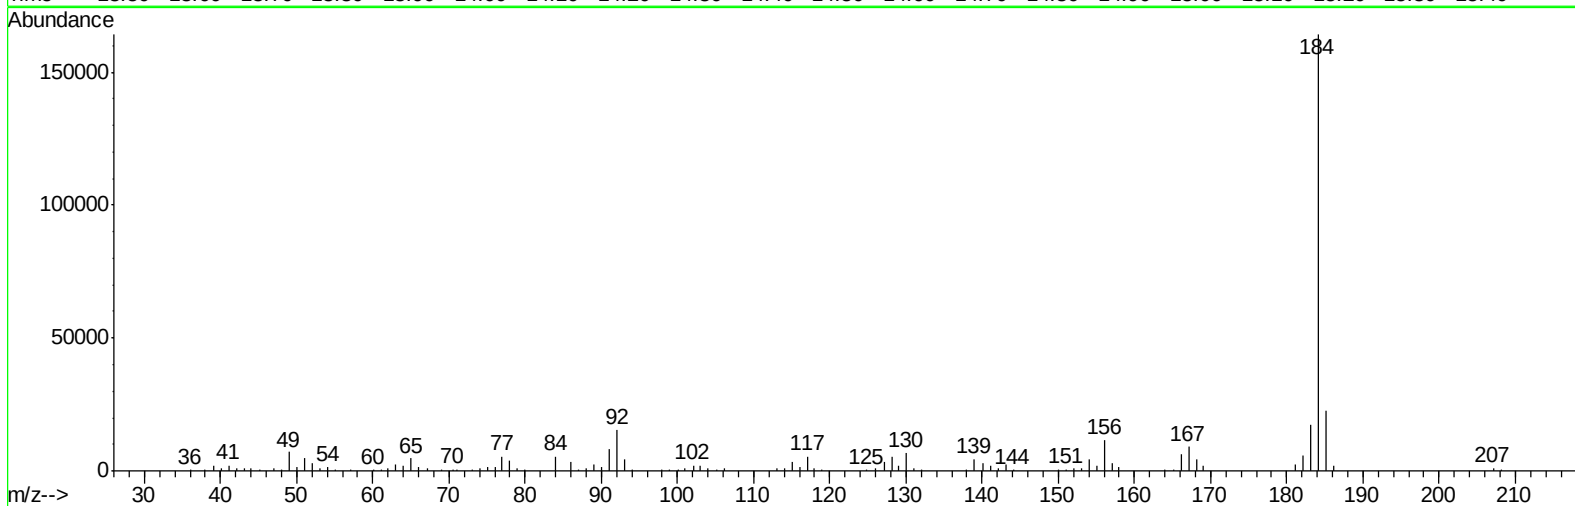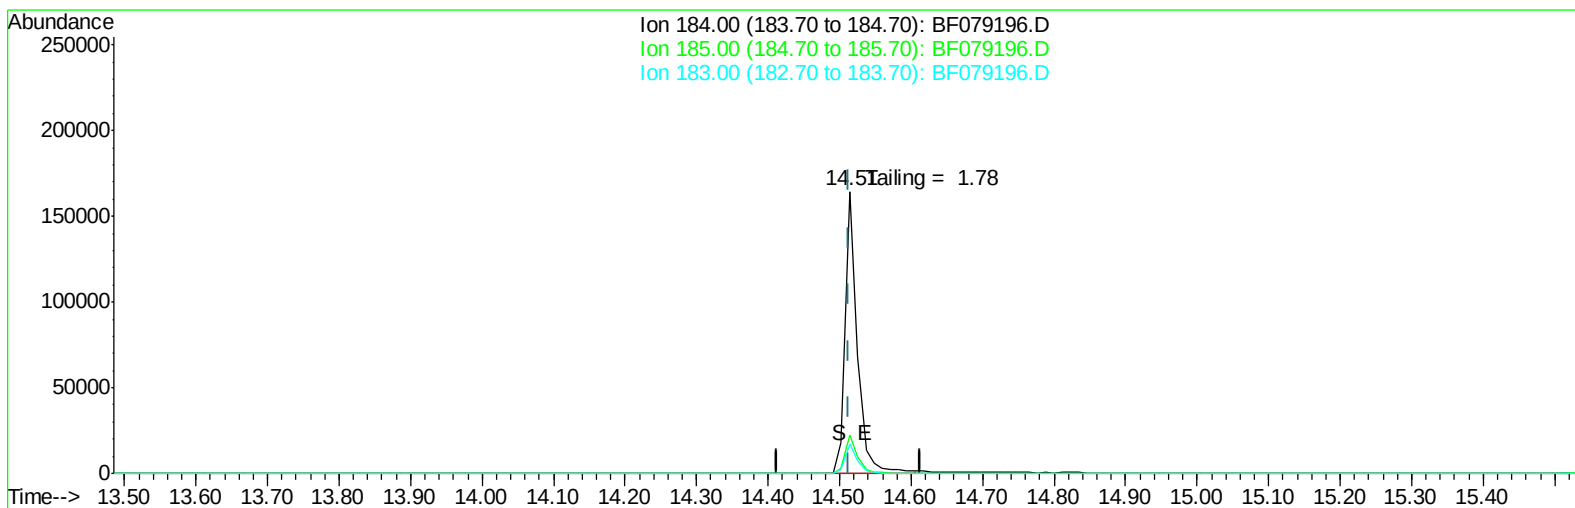

TIC: BF079196.D

(76) Benzidine

14.514min (+0.000) 474.97ng

response 181134

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	13.85
183.00	10.50	10.68
0.00	0.00	0.00