
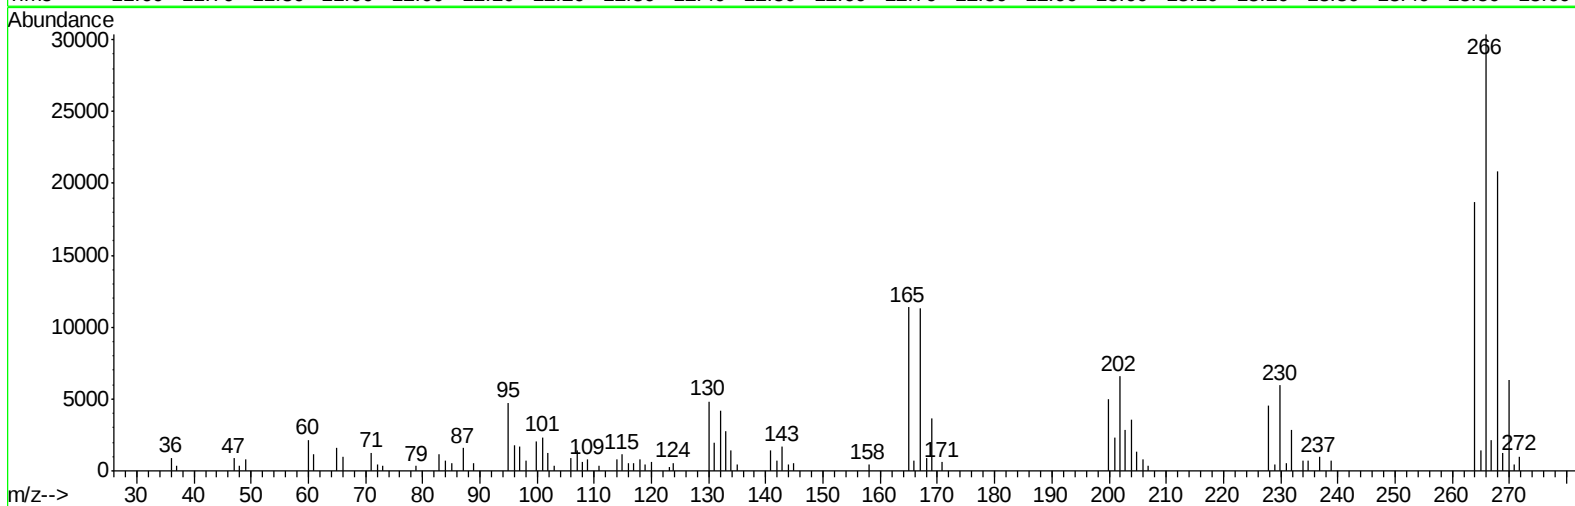


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051315\
Data File : BF079220.D
Acq On : 14 May 2015 4:52
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 14 05:42:11 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 14 00:58:22 2015
Response via : Initial Calibration

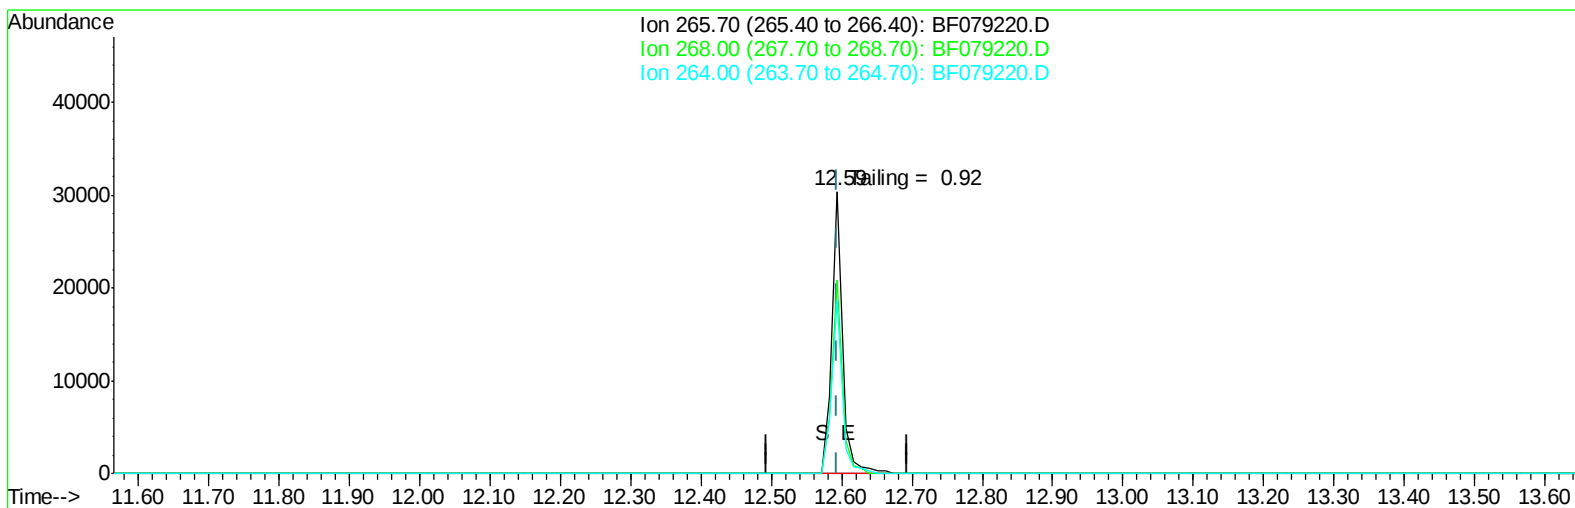

TIC: BF079220.D

(69) Pentachlorophenol (C)



12.594min (+0.000) 0.00ng

response 31573

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	68.55
264.00	60.20	61.51
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051315\
 Data File : BF079220.D
 Acq On : 14 May 2015 4:52
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 14 05:42:11 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 14 00:58:22 2015
 Response via : Initial Calibration

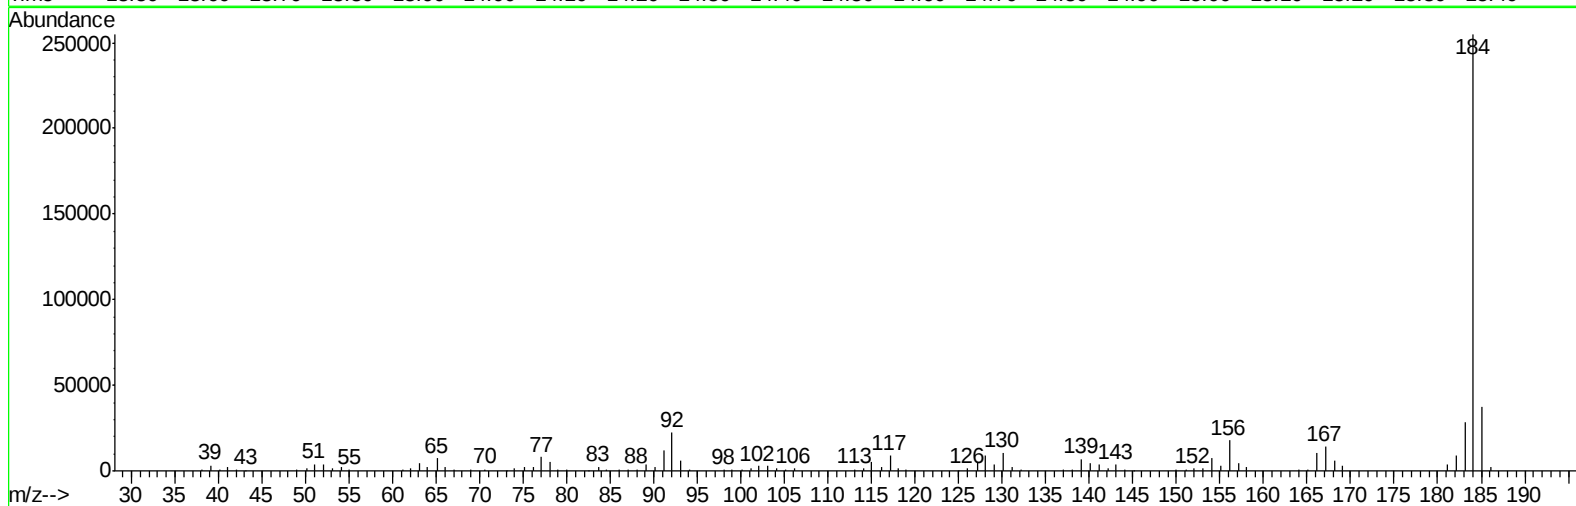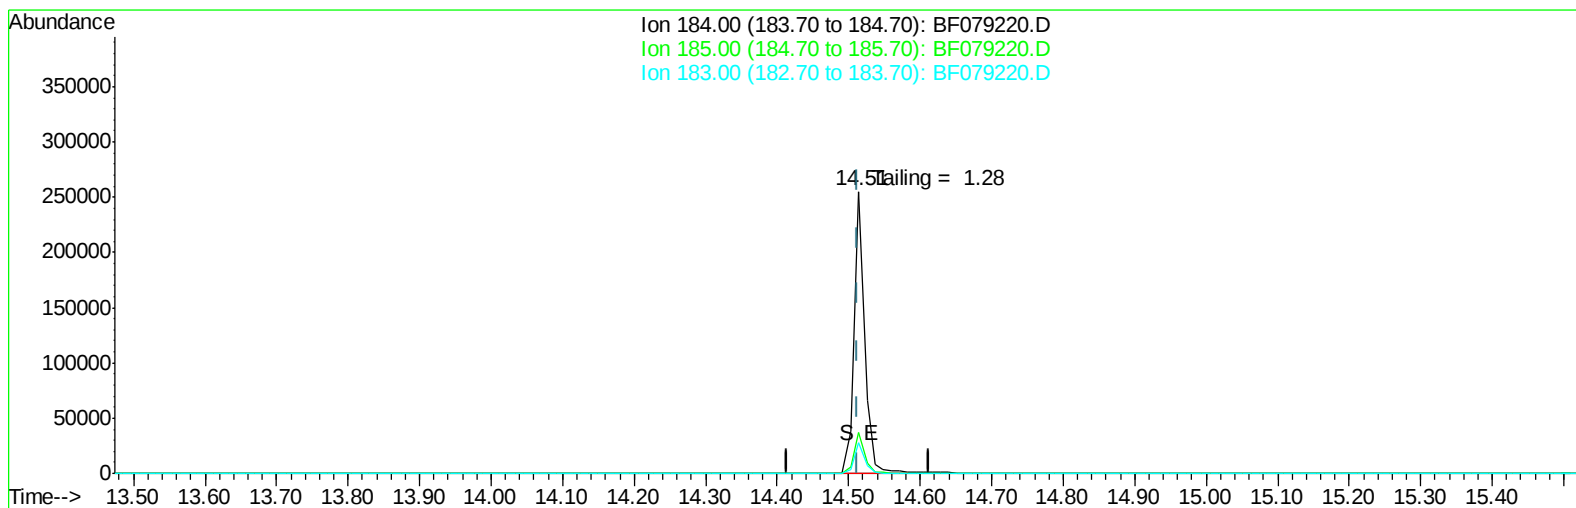

TIC: BF079220.D

(76) Benzidine

14.514min (+0.000) 7953.61ng

response 246511

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	14.59
183.00	10.50	11.02
0.00	0.00	0.00