

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051315\
 Data File : BF079230.D
 Acq On : 14 May 2015 9:39
 Operator : TP/IZ
 Sample : G2176-25
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PS-26(0-25)

Manual Integrations
 APPROVED

apatel
 5/14/2015 5:00:42 PM

Quant Time: May 14 15:43:14 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF043015.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 14 15:23:47 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.23	152	64843	20.00	ng	0.00
21) Naphthalene-d8	8.81	136	246832	20.00	ng	0.00
38) Acenaphthene-d10	10.98	164	118083	20.00	ng	0.00
63) Phenanthrene-d10	12.82	188	220663	20.00	ng	-0.01
75) Chrysene-d12	16.16	240	231513m	20.00	ng	0.03
86) Perylene-d12	18.02	264	243840	20.00	ng	0.17
System Monitoring Compounds						
5) 2-Fluorophenol	5.53	112	468090	124.26	ng	0.00
7) Phenol-d6	6.80	99	551245	110.71	ng	0.00
23) Nitrobenzene-d5	7.93	82	345960	80.55	ng	0.00
41) 2,4,6-Tribromophenol	11.97	330	171074	133.92	ng	0.00
44) 2-Fluorobiphenyl	10.16	172	718722	84.80	ng	0.00
78) Terphenyl-d14	14.82	244	786877	81.37	ng	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA F\DATA\BF051315\
Data File : BF079230.D
Acq On : 14 May 2015 9:39
Operator : TP/IZ
Sample : G2176-25
Misc :
ALS Vial : 32 Sample Multiplier: 1


Instrument :
BNA_F
ClientSampleId :
PS-26(0-25)

Manual Integrations
APPROVED

apatel
5/14/2015 5:00:42 PM

Quant Time: May 14 15:43:14 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 14 15:23:47 2015
Response via : Initial Calibration

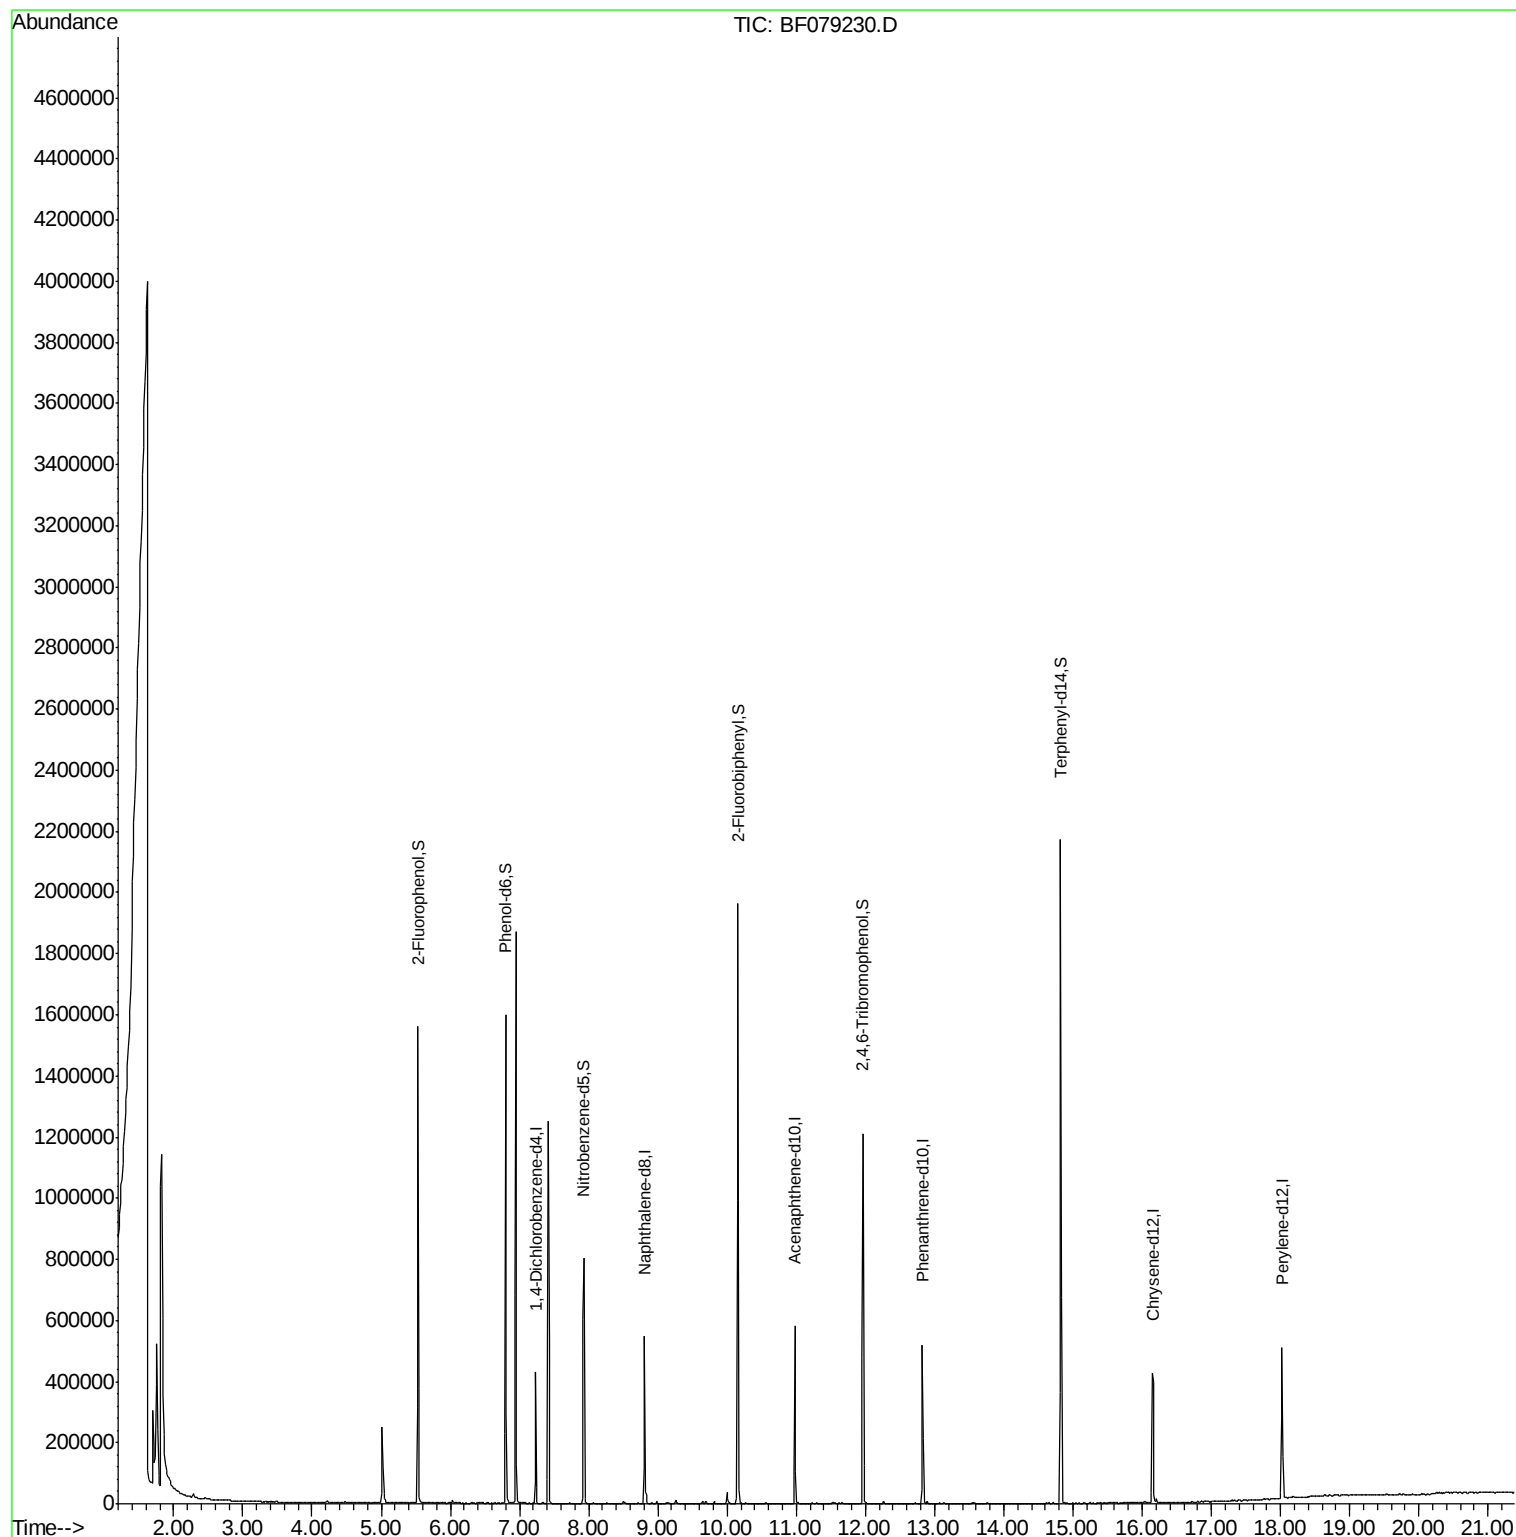

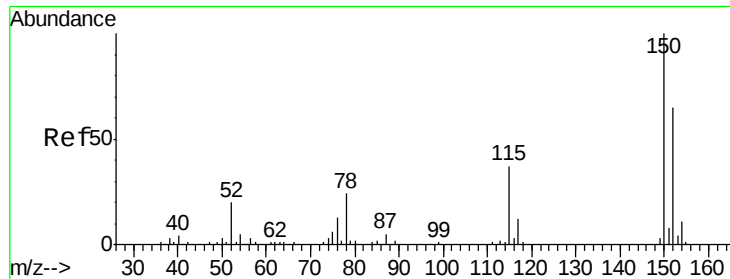





#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 7.23 min Scan# 529
 Delta R.T. 0.00 min
 Lab File: BF079230.D
 Acq: 14 May 2015 9:39

Instrument :
 BNA_F
 ClientSampleId :
 PS-26(0-25)

Tot Ion:	152	Resp:	64843
Ion Ratio	Lower	Upper	
152	100		
150	156.5	122.0	183.0
115	60.9	46.3	69.5




Manual Integrations
 APPROVED


apatel
 5/14/2015 5:00:42 PM

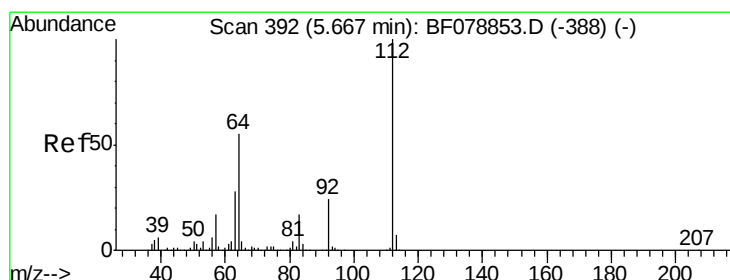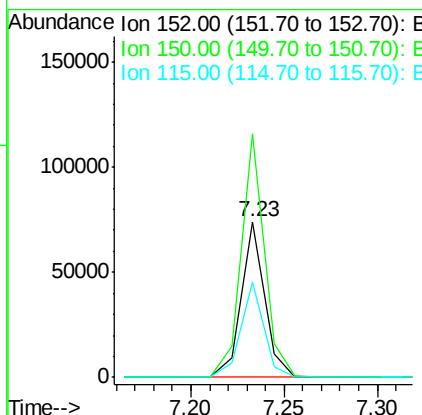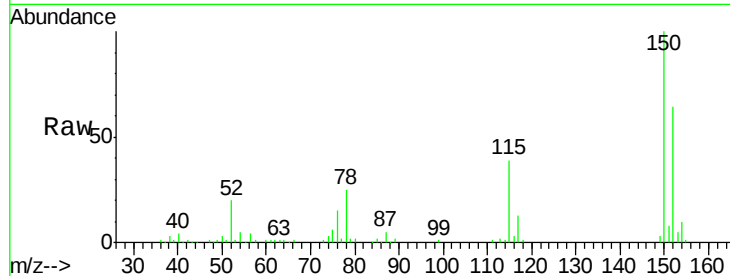

#5
 2-Fluorophenol
 Concen: 124.26 ng
 RT: 5.53 min Scan# 380
 Delta R.T. 0.00 min
 Lab File: BF079230.D
 Acq: 14 May 2015 9:39

Tgt Ion:	112	Resp:	468090
Ion Ratio	Lower	Upper	
112	100		
64	59.0	53.5	80.3
63	29.7	27.5	41.3

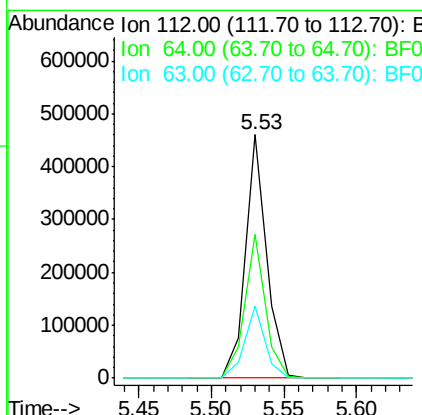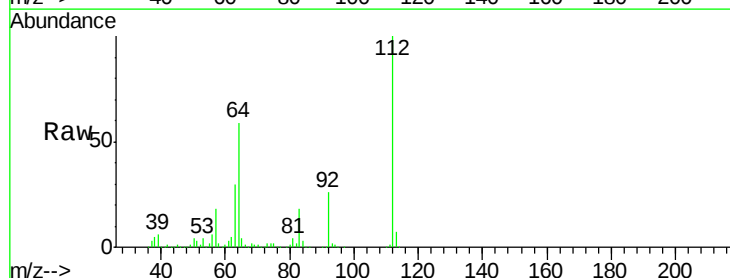



#7

Phenol-d6

Concen: 110.71 ng

RT: 6.80 min Scan# 491

Delta R.T. 0.00 min

Lab File: BF079230.D

Acq: 14 May 2015 9:39

Instrument :

BNA_F





ClientSampleId :

PS-26(0-25)

Tot Ion:	99	Resp:	551245
Ion Ratio	Lower	Upper	
99	100		
42	18.3	12.8	19.2
71	31.6	23.4	35.2

Manual Integrations
APPROVED

apatel
5/14/2015 5:00:42 PM

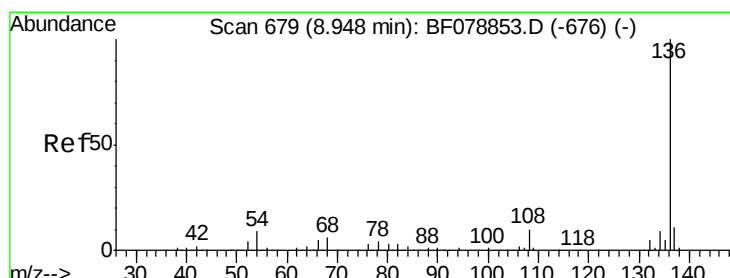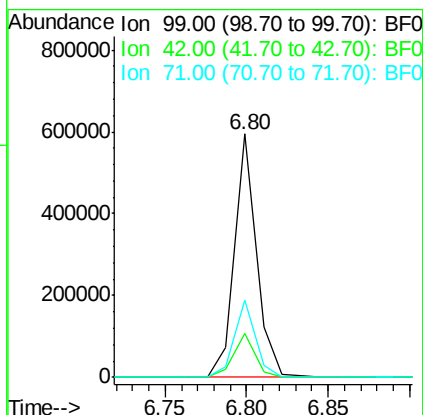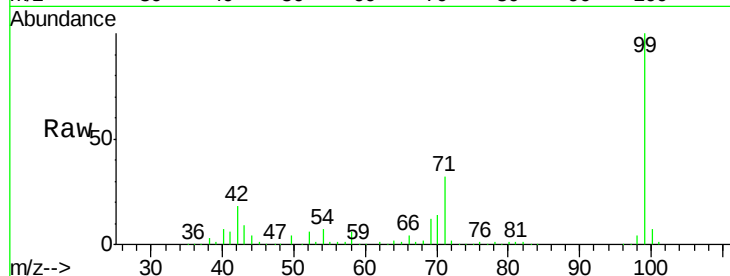

#21

Naphthalene-d8

Concen: 20.00 ng




RT: 8.81 min Scan# 667

Delta R.T. 0.00 min

Lab File: BF079230.D

Acq: 14 May 2015 9:39

Tgt Ion:	136	Resp:	246832
Ion Ratio	Lower	Upper	
136	100		
137	10.8	8.7	13.1
54	6.8	5.8	8.8
68	5.5	4.2	6.4

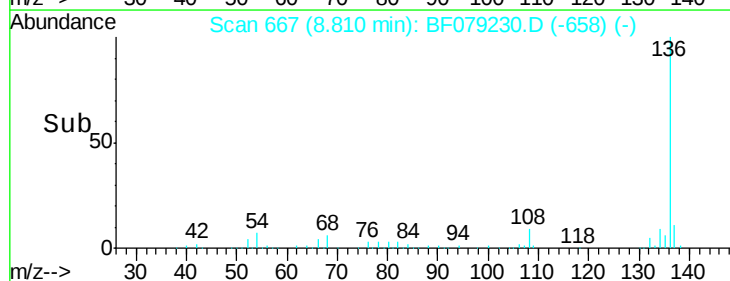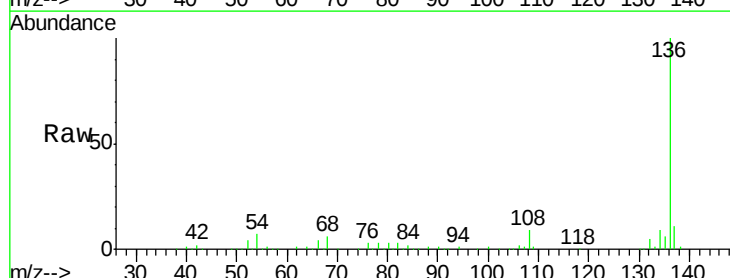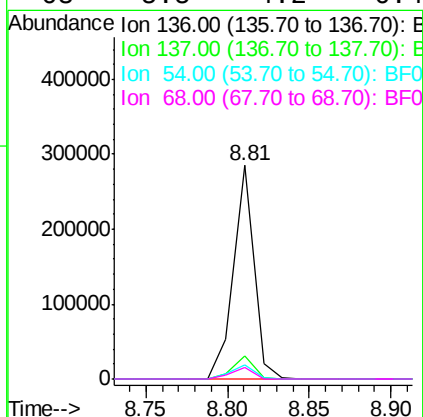







#23
 Nitrobenzene-d5
 Concen: 80.55 ng
 RT: 7.93 min Scan# 590
 Delta R.T. 0.00 min
 Lab File: BF079230.D
 Acq: 14 May 2015 9:39

Instrument :
 BNA_F
 ClientSampled :
 PS-26(0-25)

Tot Ion	Ratio	Resp	Lower	Upper
82	100			
128	54.3	30.0	45.0#	
54	45.2	46.4	69.6#	




Manual Integrations
 APPROVED

apatel
 5/14/2015 5:00:42 PM

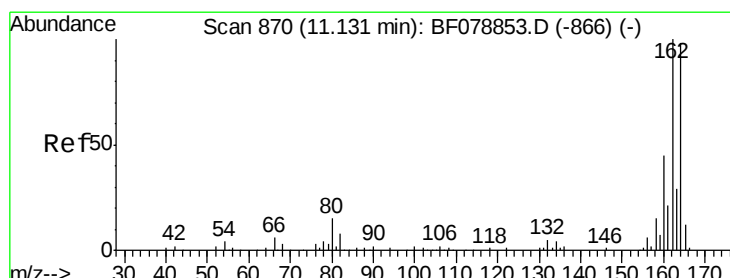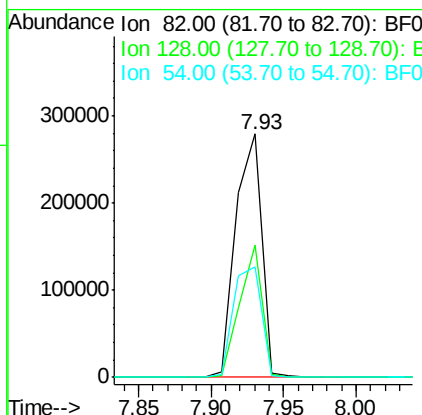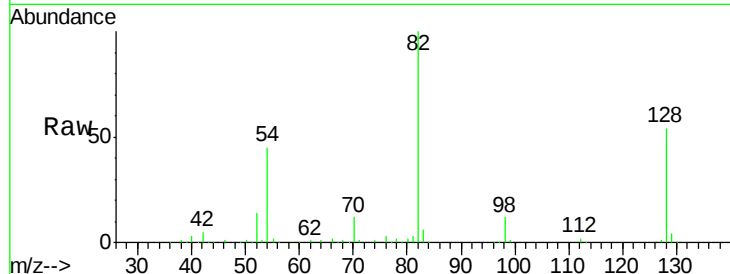

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.98 min Scan# 857
 Delta R.T. 0.00 min
 Lab File: BF079230.D
 Acq: 14 May 2015 9:39

Tgt Ion	Ratio	Resp	Lower	Upper
164	100			
162	102.7	82.7	124.1	
160	45.6	35.8	53.8	

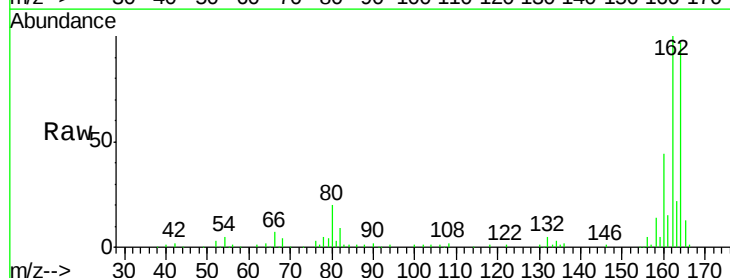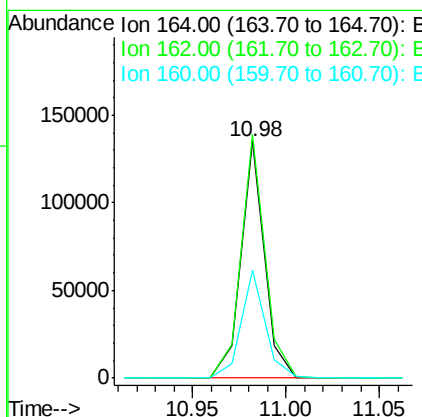







#41
 2,4,6-Tribromophenol
 Concen: 133.92 ng
 RT: 11.97 min Scan# 943
 Delta R.T. 0.00 min
 Lab File: BF079230.D
 Acq: 14 May 2015 9:39

Instrument :
 BNA_F
 ClientSampled :
 PS-26(0-25)

Tot Ion	Ratio	Resp Lower	Upper
330	100		
332	96.9	0.0	0.0#
141	33.4	0.0	0.0#




Manual Integrations
 APPROVED


apatel
 5/14/2015 5:00:42 PM

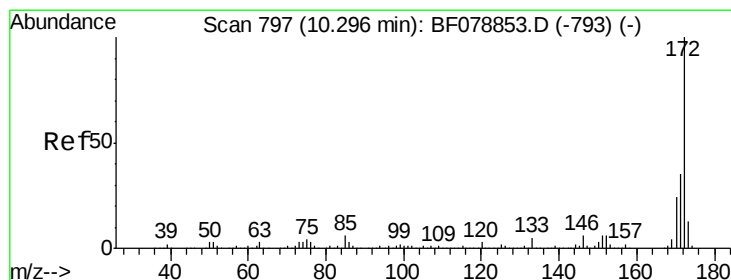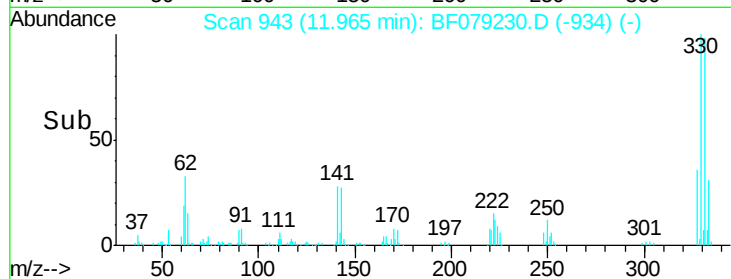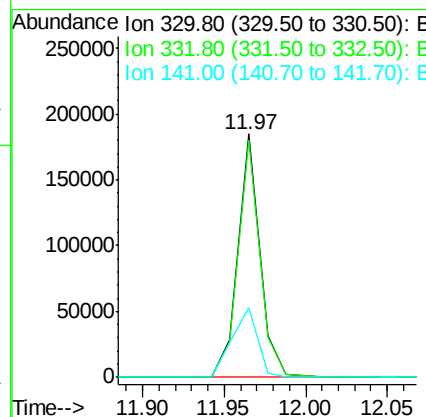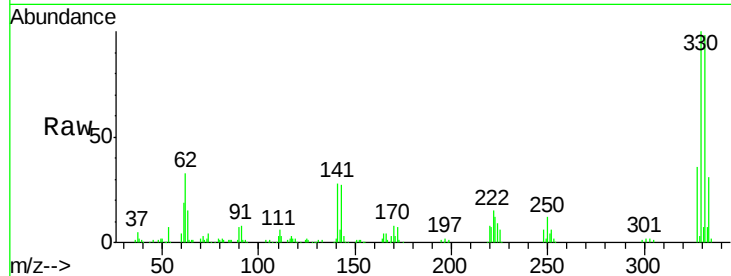

#44
 2-Fluorobiphenyl
 Concen: 84.80 ng
 RT: 10.16 min Scan# 785
 Delta R.T. 0.00 min
 Lab File: BF079230.D
 Acq: 14 May 2015 9:39

Tgt Ion	Ratio	Resp Lower	Upper
172	100		
171	34.6	27.9	41.9
170	23.8	19.4	29.0

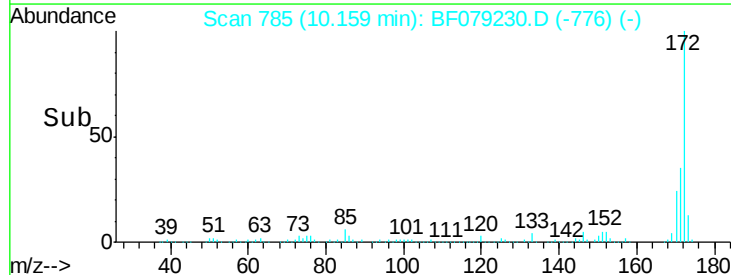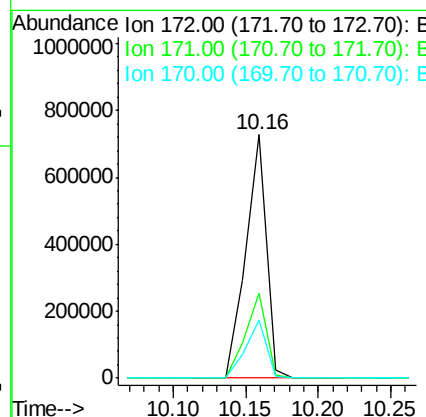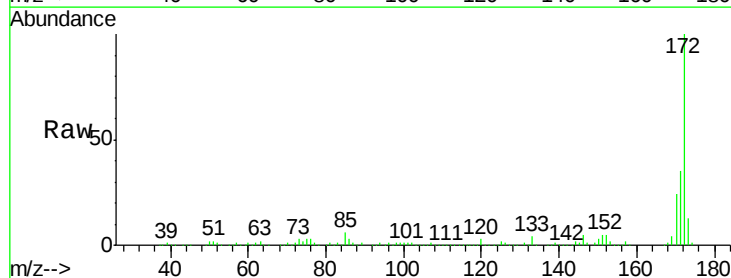

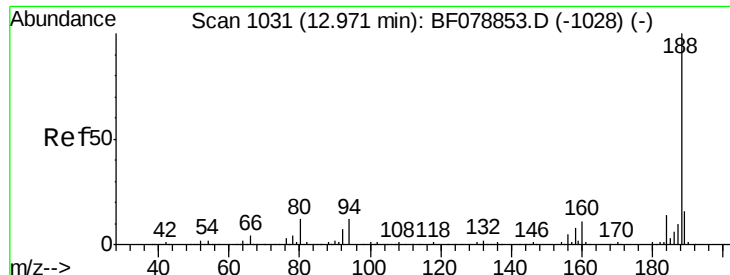





#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 12.82 min Scan# 1018
Delta R.T. -0.01 min
Lab File: BF079230.D
Acq: 14 May 2015 9:39

Instrument :
BNA_F
ClientSampleId :
PS-26(0-25)

Tot Ion	Ratio	Resp Lower	Upper
188	100		
94	11.6	8.2	12.2
80	12.3	8.9	13.3




Manual Integrations
APPROVED


apatel
5/14/2015 5:00:42 PM

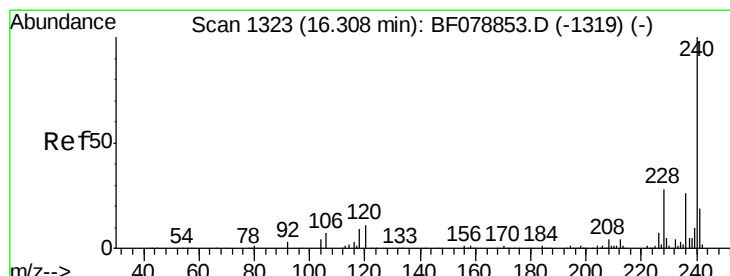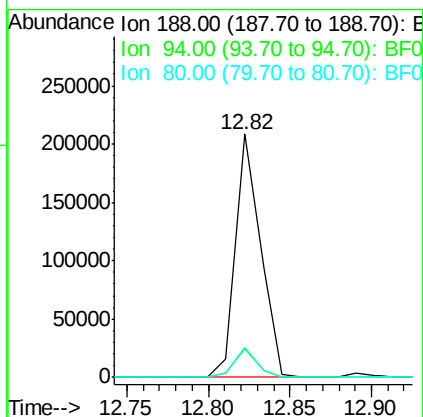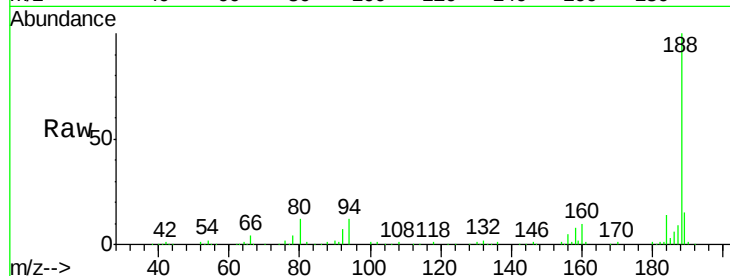

#75
Chrysene-d12
Concen: 20.00 ng m
RT: 16.16 min Scan# 1310
Delta R.T. 0.03 min
Lab File: BF079230.D
Acq: 14 May 2015 9:39

Tgt Ion	Ratio	Resp Lower	Upper
240	100		
120	9.0	9.7	14.5#
236	25.2	20.2	30.4

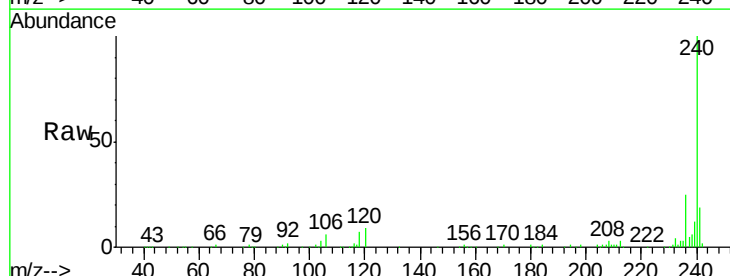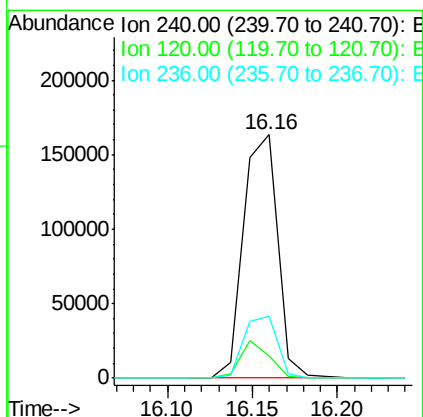







#78
 Terphenyl-d14
 Concen: 81.37 ng
 RT: 14.82 min Scan# 1193
 Delta R.T. 0.00 min
 Lab File: BF079230.D
 Acq: 14 May 2015 9:39

Instrument :
 BNA_F
 ClientSampleId :
 PS-26(0-25)

Tot Ion	Ratio	Lower	Upper
244	100		
212	6.9	5.6	8.4
122	14.1	10.3	15.5

Manual Integrations
 APPROVED

apatel
 5/14/2015 5:00:42 PM

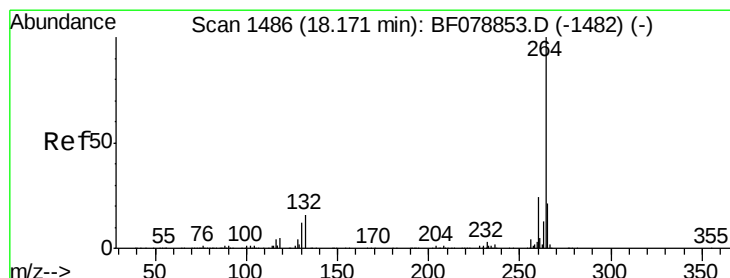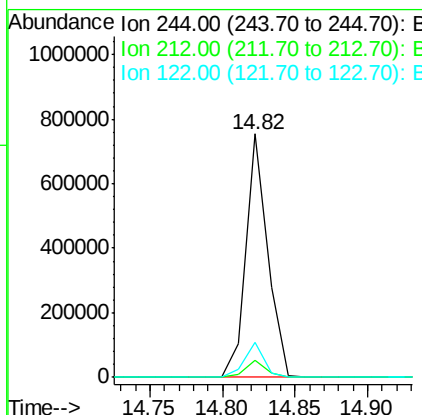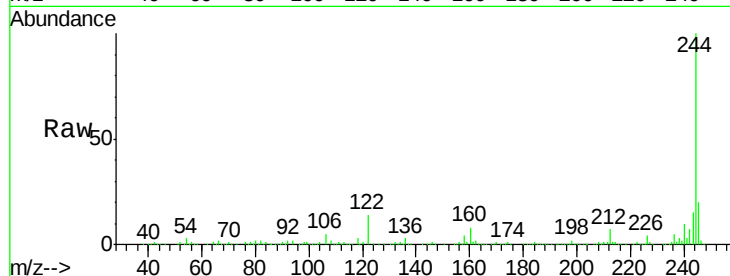

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 18.02 min Scan# 1473
 Delta R.T. 0.17 min
 Lab File: BF079230.D
 Acq: 14 May 2015 9:39

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.1	19.4	29.2
265	21.0	18.3	27.5

