

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051315\
 Data File : BF079212.D
 Acq On : 14 May 2015 00:05
 Operator : TP/IZ
 Sample : G2202-09
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 A-COMP

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.381	14	17	19	rVB	1095034	1413050	39.69%	8.378%
2	1.507	25	28	38	rVB3	67305	198310	5.57%	1.176%
3	1.701	41	45	51	rVV2	187455	419459	11.78%	2.487%
4	1.827	54	56	90	rVB	1471007	3560348	100.00%	21.109%
5	5.016	333	335	340	rBV	66378	84459	2.37%	0.501%
6	5.530	377	380	383	rBV	875762	926181	26.01%	5.491%
7	6.799	489	491	494	rBV	1070339	958587	26.92%	5.684%
8	6.947	501	504	506	rBV	1044717	1018152	28.60%	6.037%
9	7.233	527	529	532	rVB	363081	319621	8.98%	1.895%
10	7.416	543	545	548	rVB	744074	744600	20.91%	4.415%
11	7.930	587	590	592	rBV	441767	591546	16.61%	3.507%
12	8.810	665	667	669	rBV	506166	444614	12.49%	2.636%
13	10.159	782	785	787	rBV	1130288	1158451	32.54%	6.869%
14	10.662	827	829	831	rBV	79272	66542	1.87%	0.395%
15	10.982	855	857	860	rVB	526381	505264	14.19%	2.996%
16	11.965	940	943	945	rBV	897657	883408	24.81%	5.238%
17	12.822	1016	1018	1021	rBV	467481	564862	15.87%	3.349%
18	13.542	1078	1081	1083	rBV3	32960	46180	1.30%	0.274%
19	14.822	1190	1193	1196	rBV	1275984	1287036	36.15%	7.631%
20	15.565	1253	1258	1259	rBV4	17850	49441	1.39%	0.293%
21	15.988	1293	1295	1300	rBV	112432	198478	5.57%	1.177%
22	16.114	1303	1306	1308	rBV	604469	667143	18.74%	3.956%
23	16.800	1364	1366	1370	rVB	32107	55180	1.55%	0.327%
24	17.840	1454	1457	1461	rVB	568620	705186	19.81%	4.181%


Sum of corrected areas: 16866098

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051315\
Data File : BF079212.D
Acq On : 14 May 2015 00:05
Operator : TP/IZ
Sample : G2202-09
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
A-COMP

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

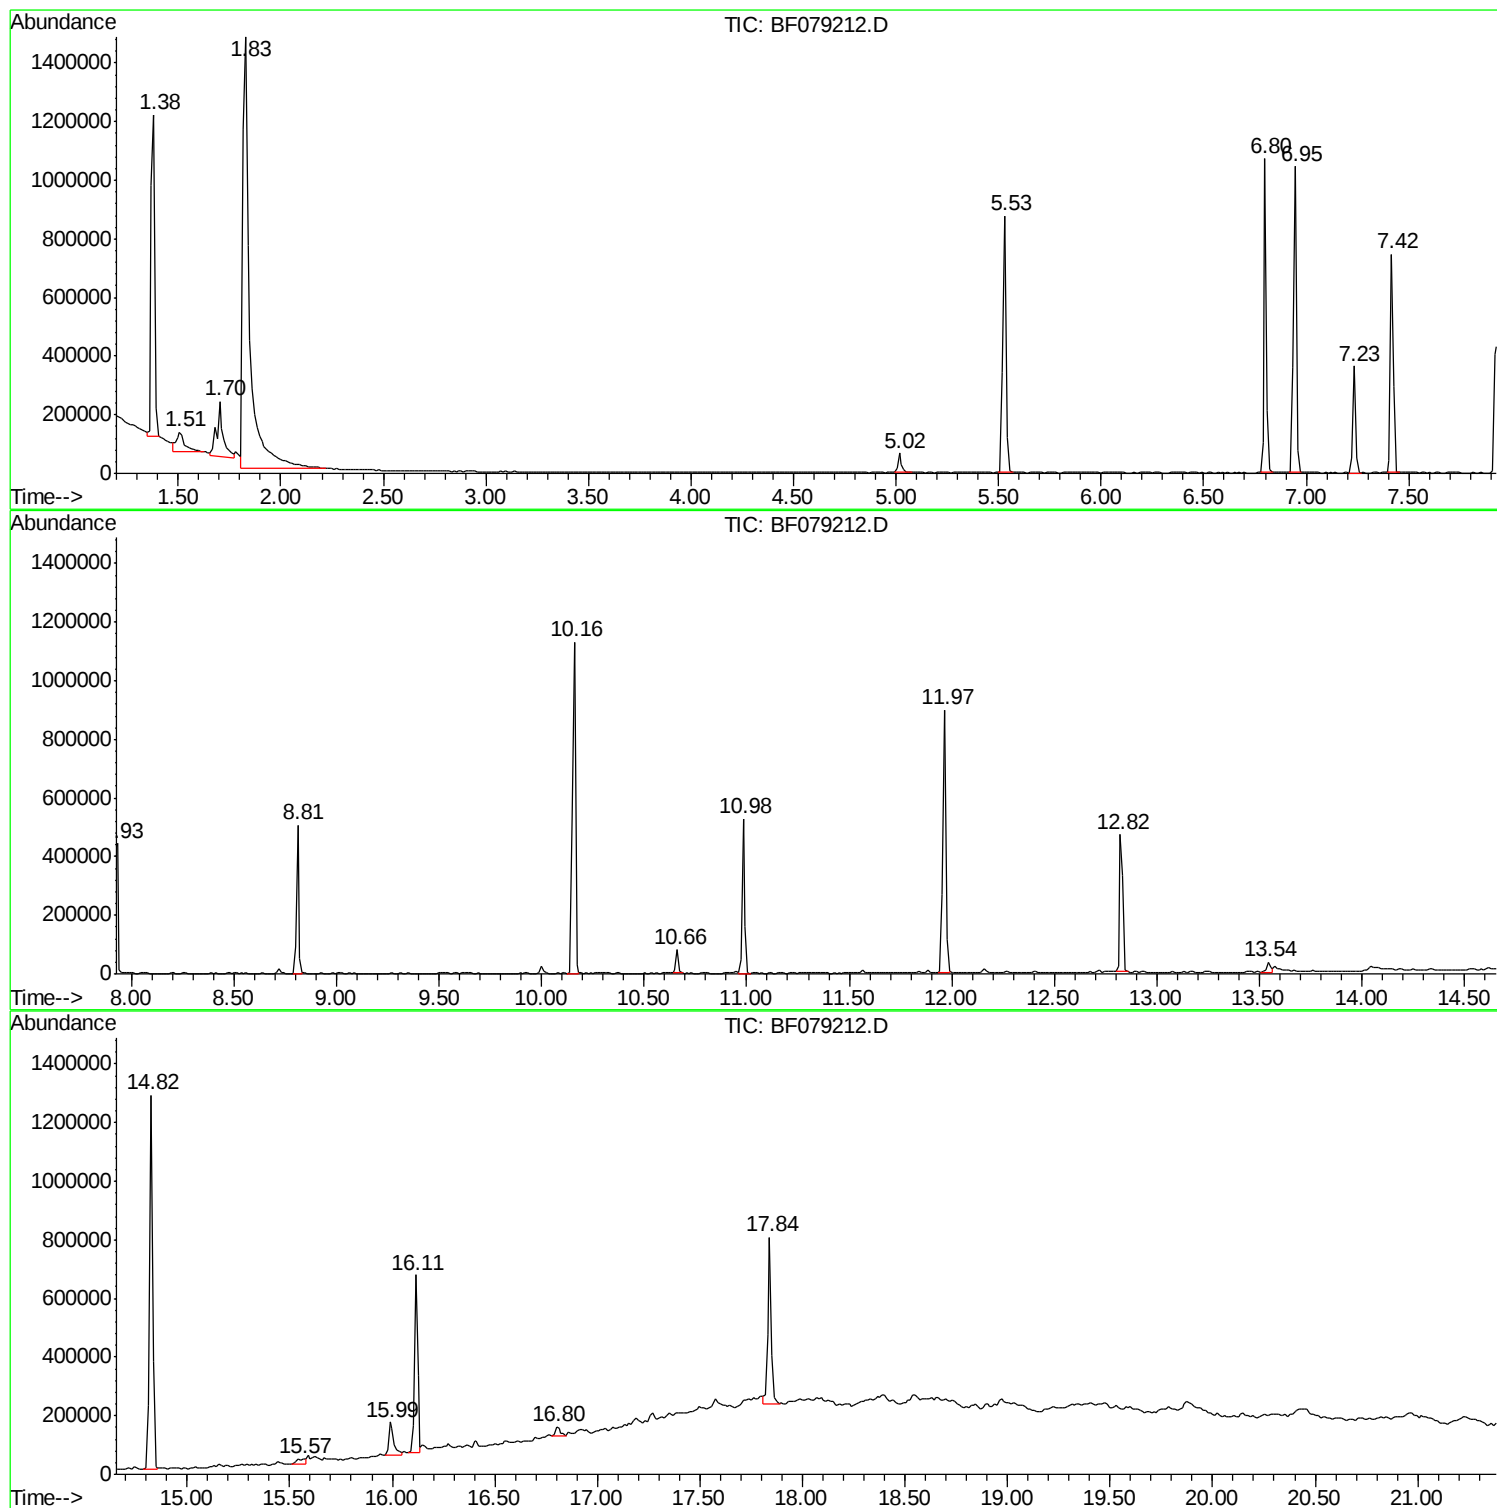

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF051315\
Data_File : BF079212.D
Acq_On : 14 May, 2015 00:055
Operator : TP/IZZ
Sample : G2202-099
Misc :
ALS_Vial : 17 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
A-COMP

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
