


Data Path : Z:\HPCHEM1\BNA F\DATA\BF051315\
 Data File : BF079196.D
 Acq On : 13 May 2015 15:03
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 14 15:23:47 2015

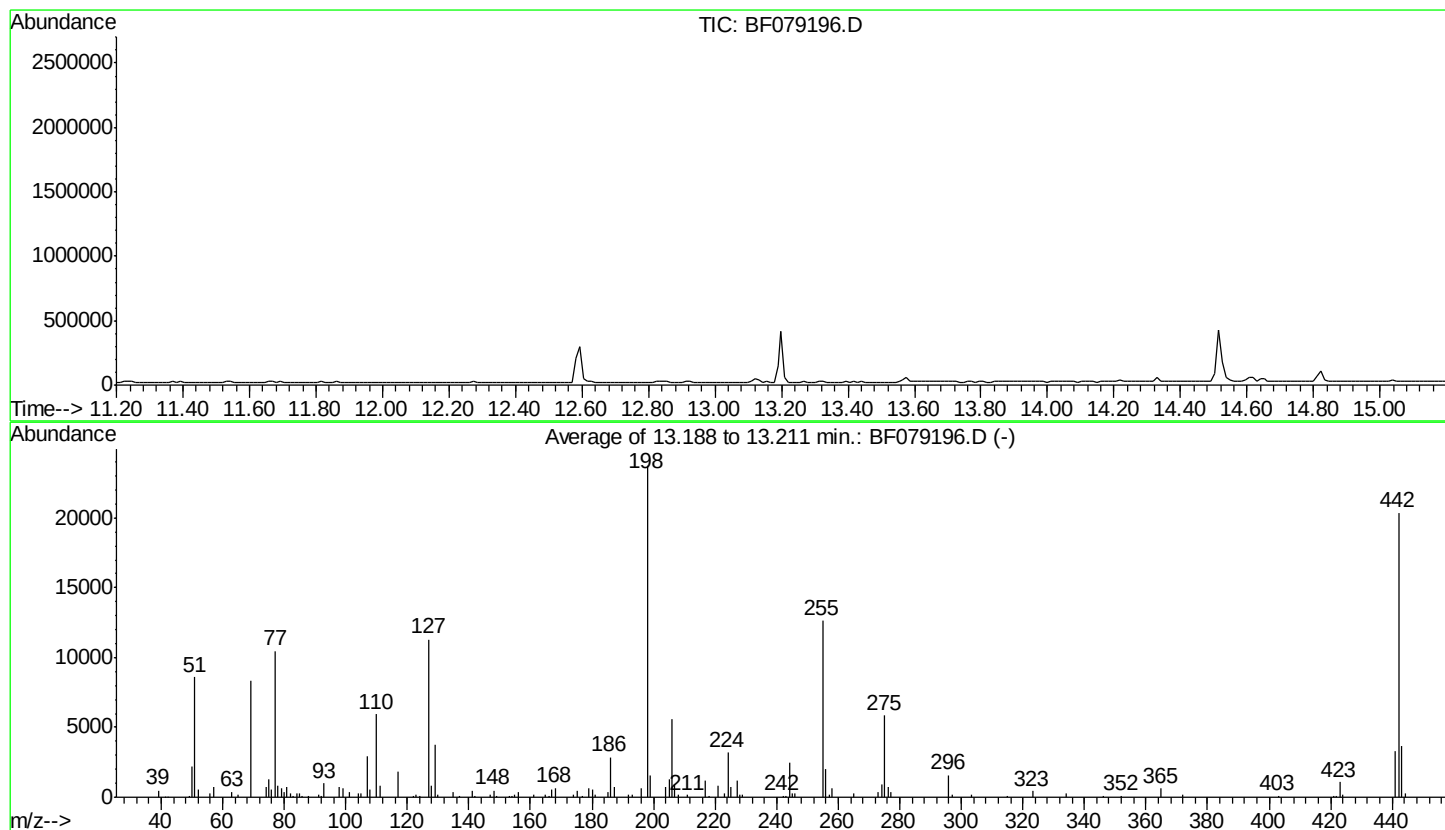

AutoFind: Scans 1050, 1051, 1052; Background Corrected with Scan 1047

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	8572	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.3	8370	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.7	11321	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	23741	PASS
199	198	5	9	6.5	1545	PASS
275	198	10	60	24.7	5857	PASS
365	198	1	100	2.5	599	PASS
441	442	0.01	24	16.4	3345	PASS
442	198	50	100	85.8	20367	PASS
443	442	15	24	18.0	3667	PASS