


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051315\
 Data File : BF079220.D
 Acq On : 14 May 2015 4:52
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 14 15:23:47 2015

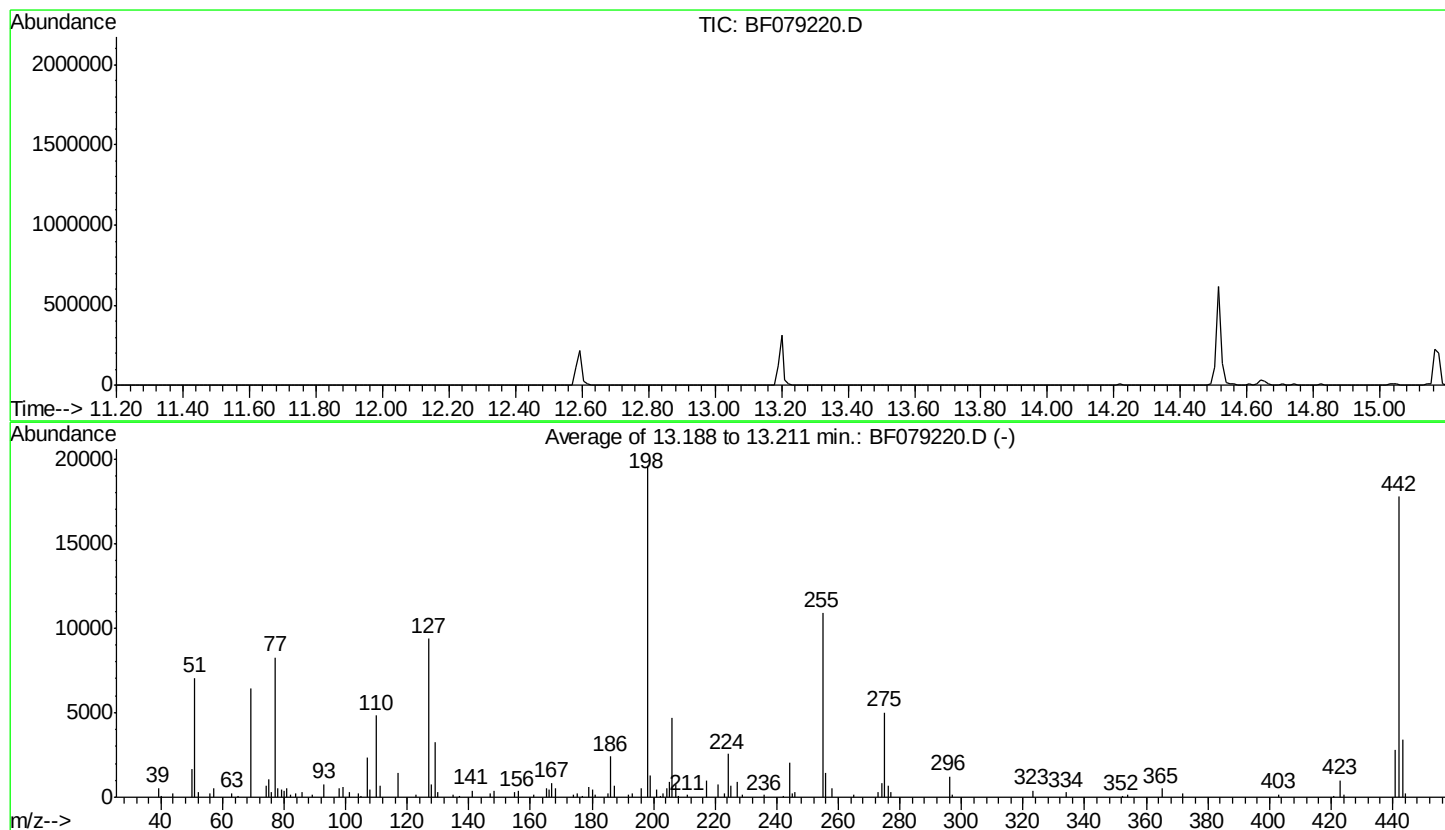

AutoFind: Scans 1050, 1051, 1052; Background Corrected with Scan 1047

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	7064	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	32.8	6431	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.9	9374	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	19587	PASS
199	198	5	9	6.7	1321	PASS
275	198	10	60	25.6	5022	PASS
365	198	1	100	2.7	525	PASS
441	442	0.01	24	15.8	2812	PASS
442	198	50	100	90.6	17751	PASS
443	442	15	24	19.0	3374	PASS