
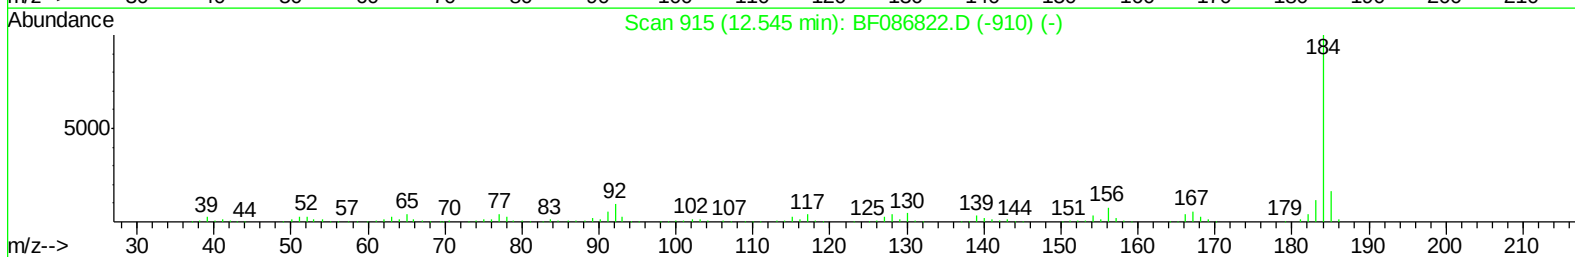
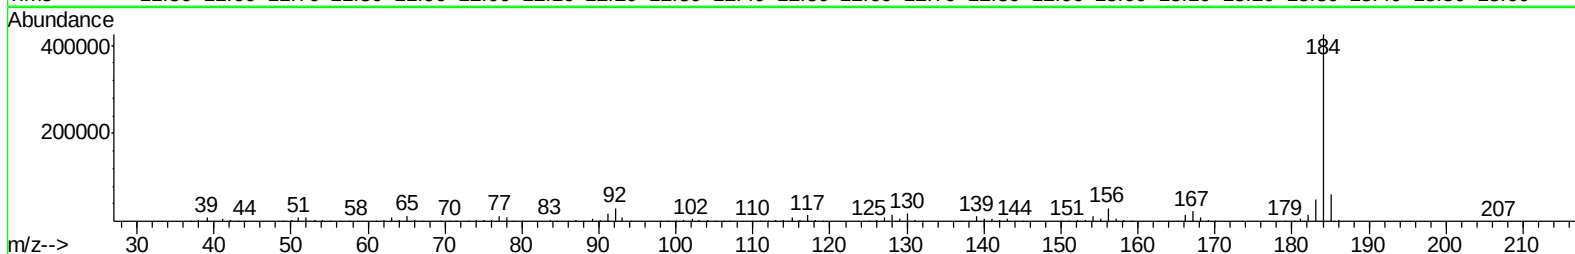


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051316\
 Data File : BF087001.D
 Acq On : 14 May 2016 6:05
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 03:14:01 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 16 01:11:12 2016
 Response via : Initial Calibration

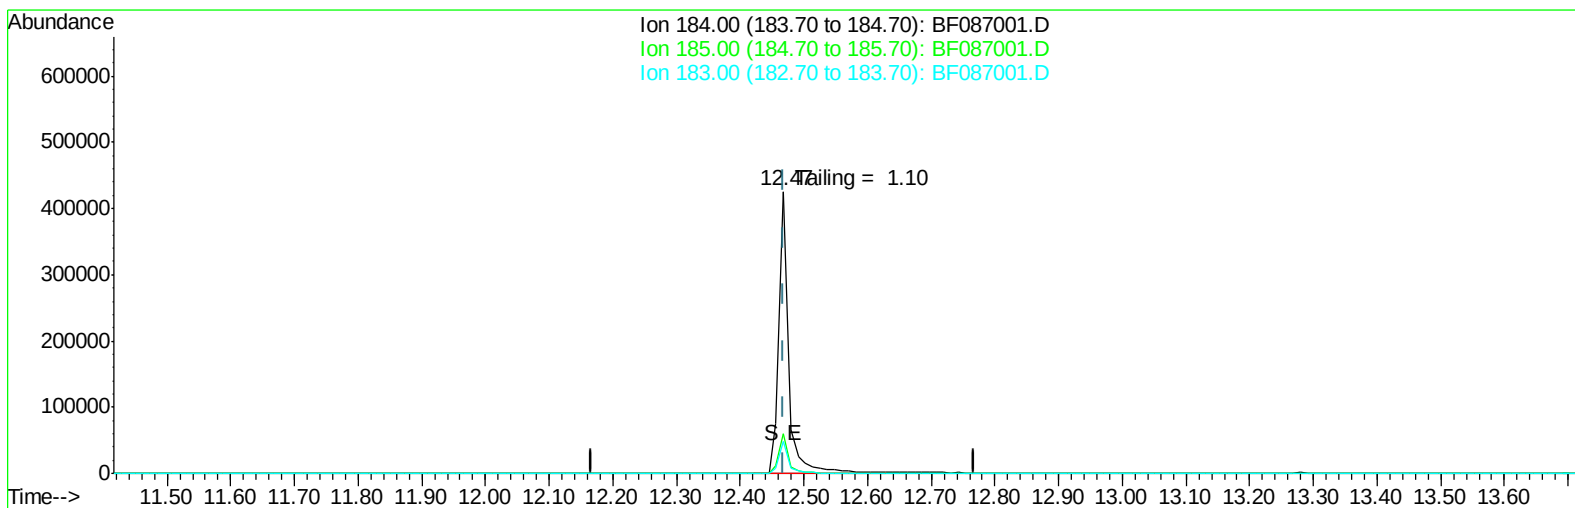

TIC: BF087001.D

(76) Benzidine




12.468min (0.000) 83266.62ng

response 456392

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	14.20
183.00	12.20	11.48
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF051316\
Data File : BF087001.D
Acq On : 14 May 2016 6:05
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 03:14:01 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 16 01:11:12 2016
Response via : Initial Calibration

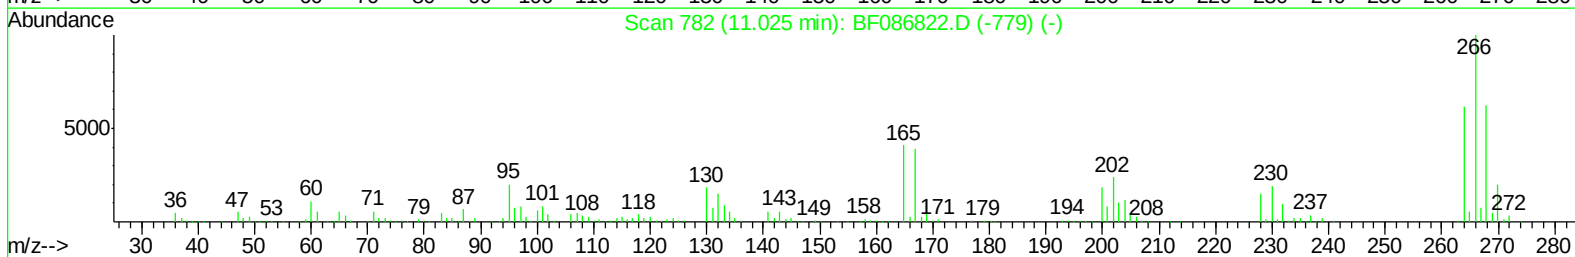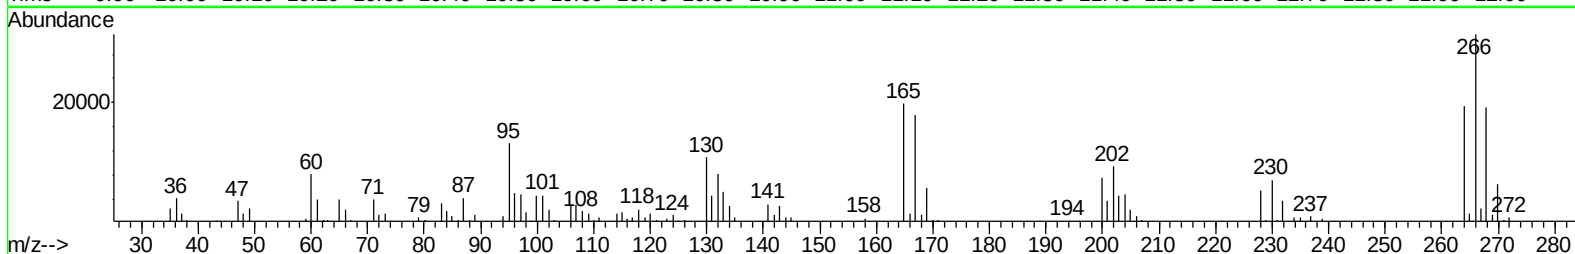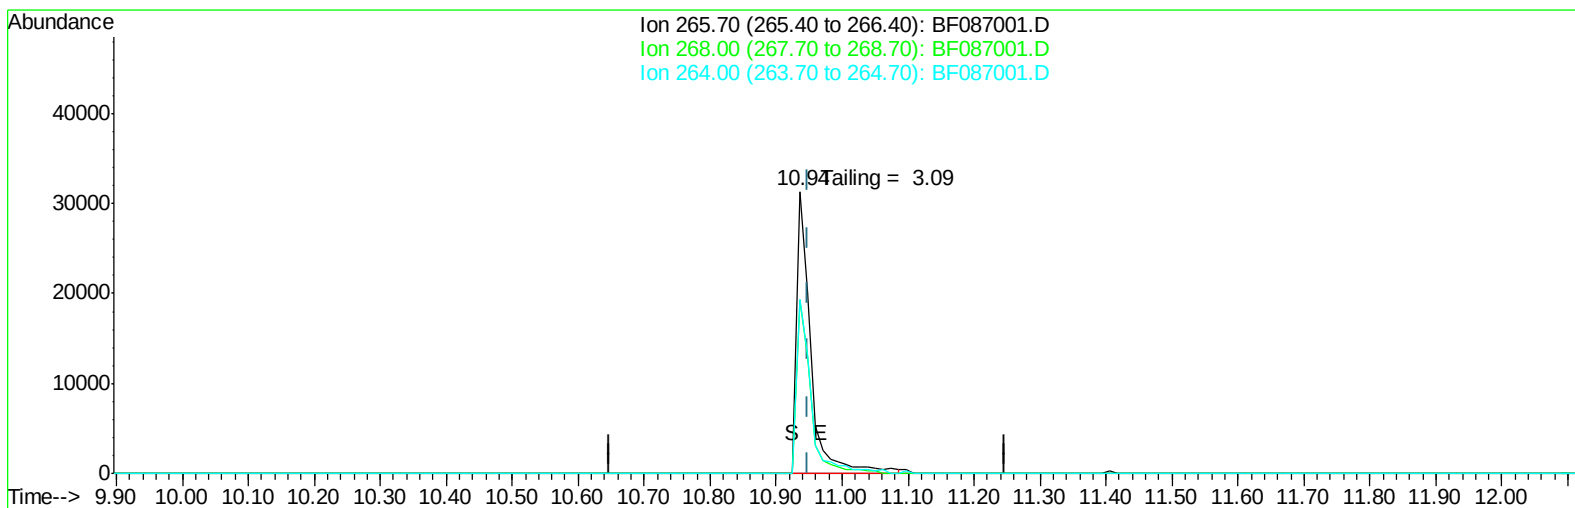

TIC: BF087001.D

(69) Pentachlorophenol (C)

10.936min (-0.011) 0.00ng

response 46323

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	61.18
264.00	66.10	62.05
0.00	0.00	0.00