

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051316\
 Data File : BF086994.D
 Acq On : 14 May 2016 2:42
 Operator : UM/SJ
 Sample : H2895-14
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP14-2FT

Quant Time: May 14 03:39:59 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 13 23:02:21 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.62	152	144758	20.00	ng	0.00
21) Naphthalene-d8	7.90	136	594365	20.00	ng	-0.01
38) Acenaphthene-d10	9.64	164	289330	20.00	ng	-0.01
63) Phenanthrene-d10	11.12	188	542622	20.00	ng	-0.01
75) Chrysene-d12	13.75	240	455572	20.00	ng	-0.01
86) Perylene-d12	15.11	264	332379	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.22	112	1106094	129.40	ng	0.02
7) Phenol-d6	6.28	99	1468197	128.52	ng	0.00
23) Nitrobenzene-d5	7.19	82	1059441	89.50	ng	-0.01
41) 2,4,6-Tribromophenol	10.44	330	416171	135.87	ng	0.00
44) 2-Fluorobiphenyl	8.98	172	1669512	96.98	ng	0.00
78) Terphenyl-d14	12.71	244	1652285	76.95	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF051316\
Data File : BF086994.D
Acq On : 14 May 2016 2:42
Operator : UM/SJ
Sample : H2895-14
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP14-2FT

Quant Time: May 14 03:39:59 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 13 23:02:21 2016
Response via : Initial Calibration

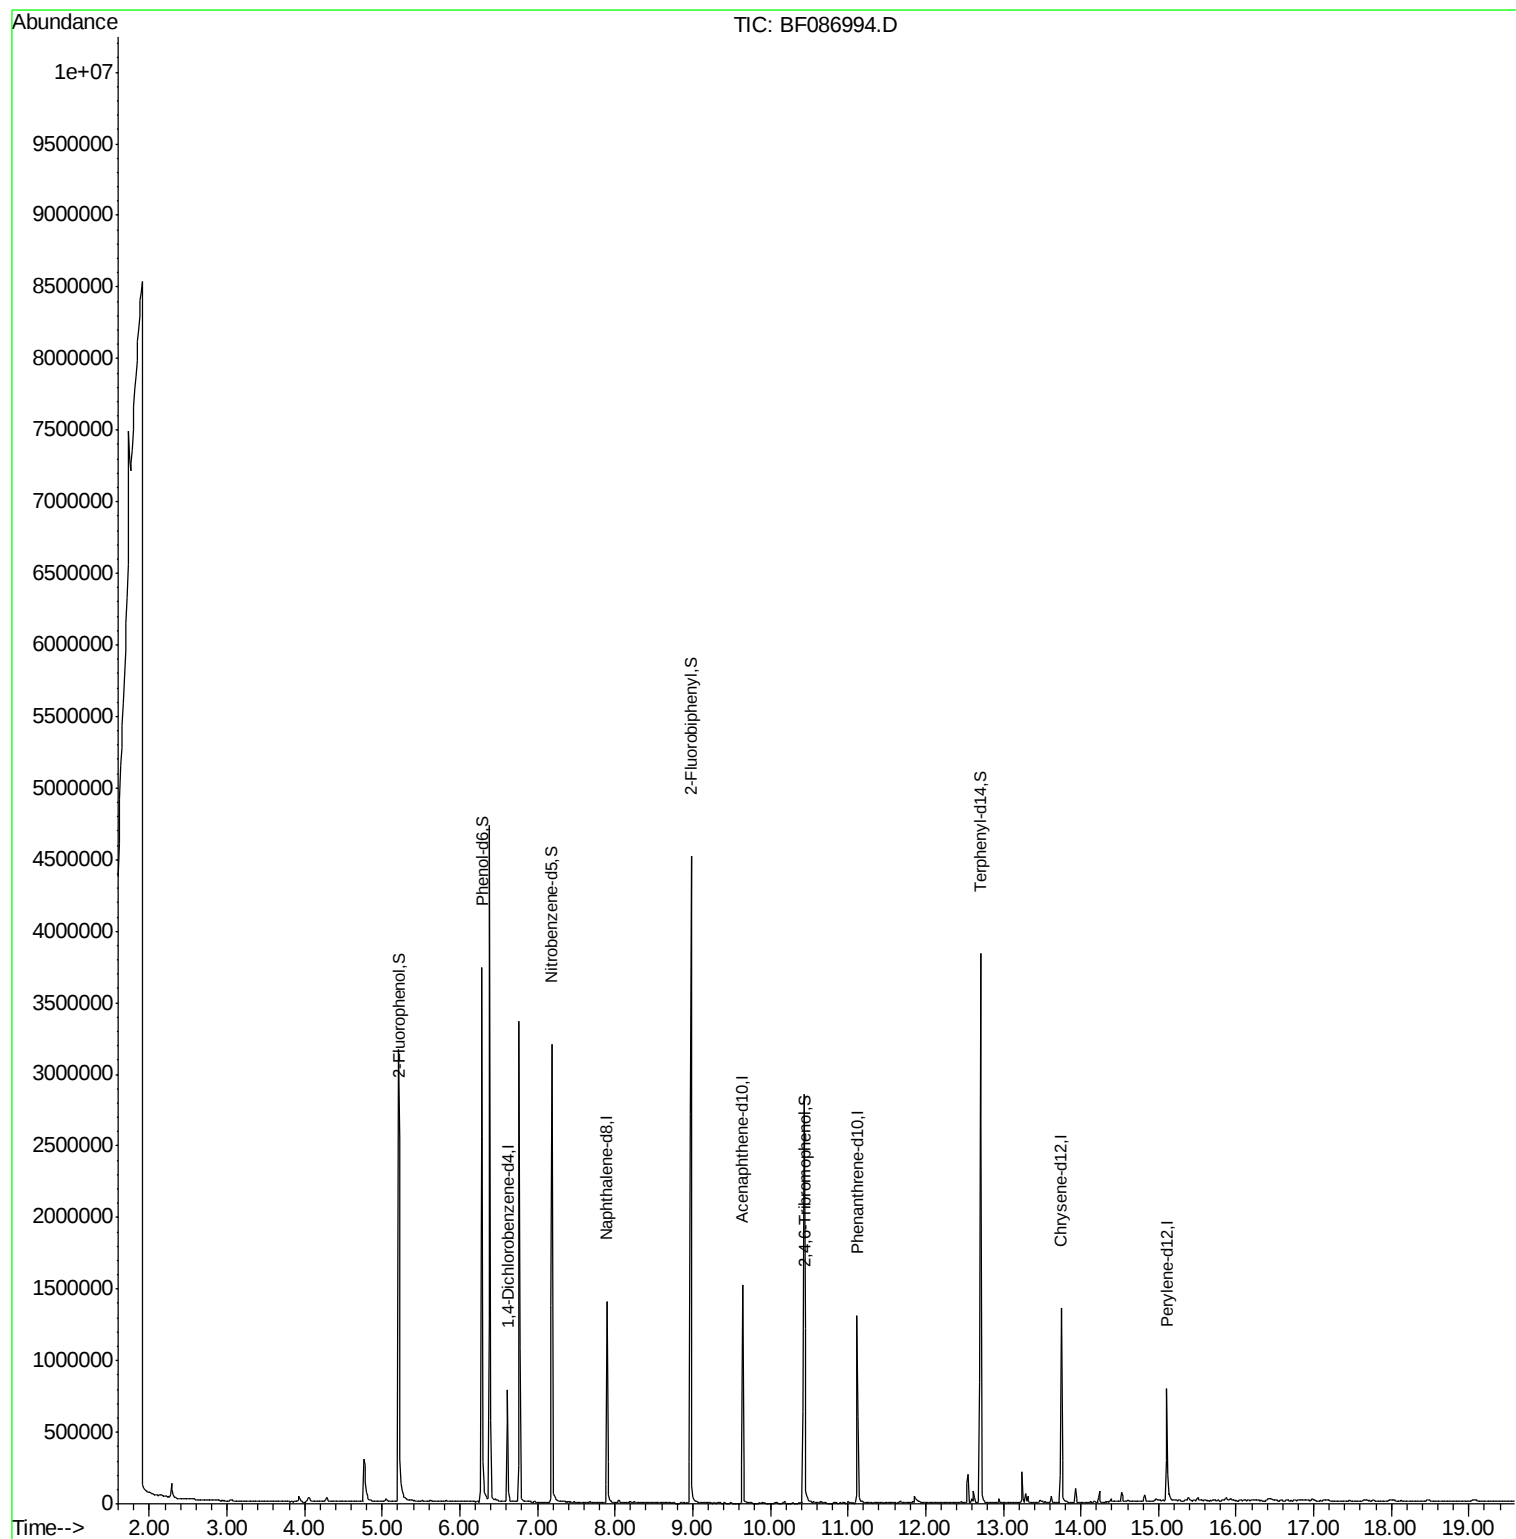

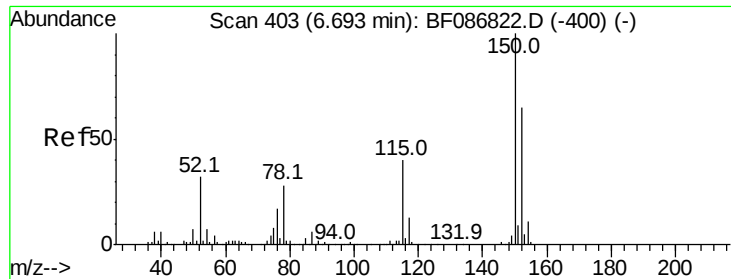

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.62 min Scan# 440

Delta R.T. 0.00 min

Lab File: BF086994.D

Acq: 14 May 2016 2:42

Instrument :

BNA_F

ClientSampleId :

TP14-2FT


Tot Ion:152 Resp: 144758

Ion Ratio Lower Upper

152 100

150 152.9 125.8 188.6




115 57.6 51.5 77.3



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

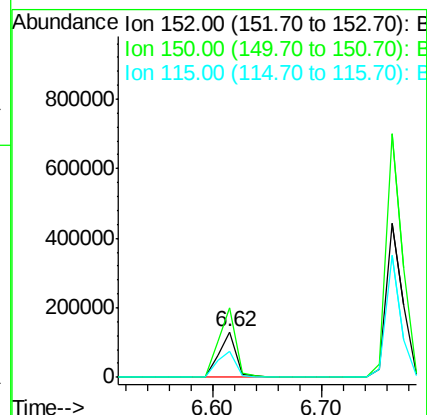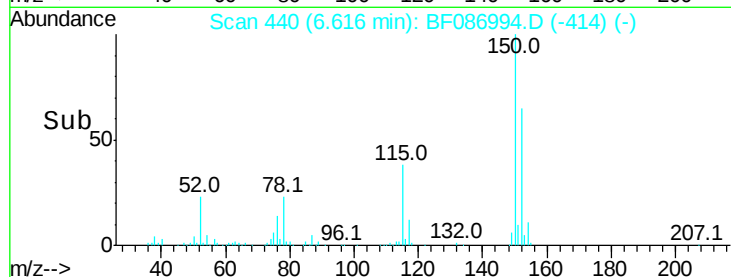

#5

2-Fluorophenol

Concen: 129.40 ng

RT: 5.22 min Scan# 318

Delta R.T. 0.02 min

Lab File: BF086994.D

Acq: 14 May 2016 2:42


Tgt Ion:112 Resp: 1106094

Ion Ratio Lower Upper

112 100

64 58.9 52.1 78.1



63 31.7 25.7 38.5




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

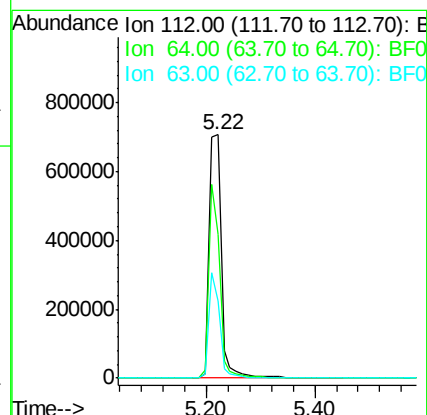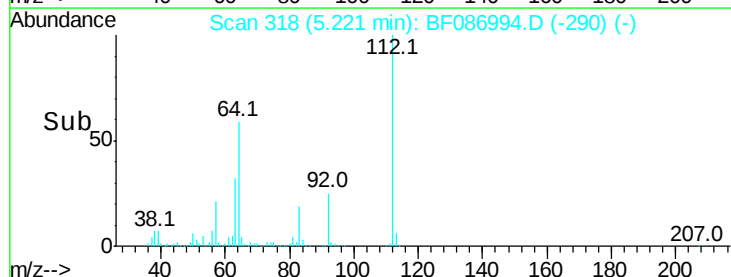

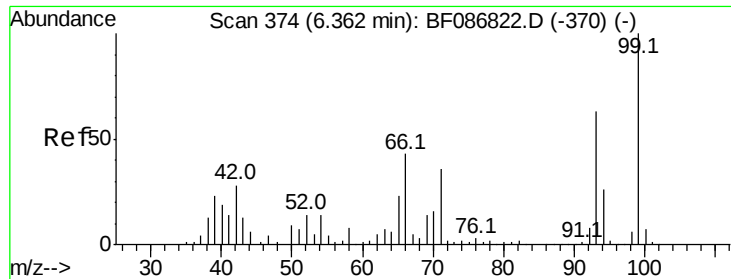

#7

Phenol-d6

Concen: 128.52 ng

RT: 6.28 min Scan# 411

Delta R.T. 0.00 min

Lab File: BF086994.D

Acq: 14 May 2016 2:42

Instrument :


BNA_F

ClientSampleId :

TP14-2FT

Tot Ion: 99 Resp: 1468197




Ion	Ratio	Lower	Upper
99	100		
42	25.9	13.6	20.4#
71	36.7	24.6	36.8

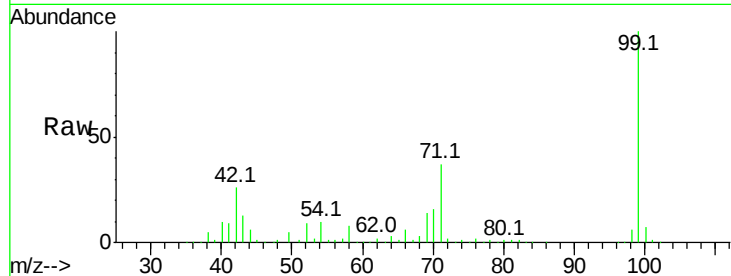

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

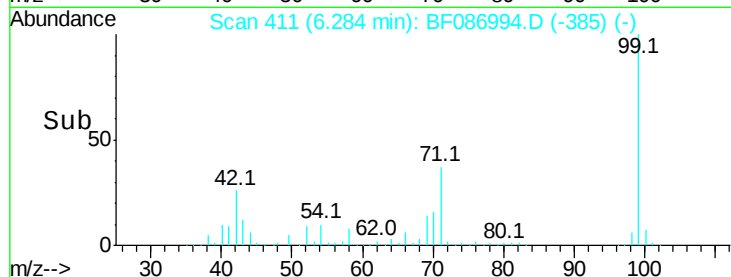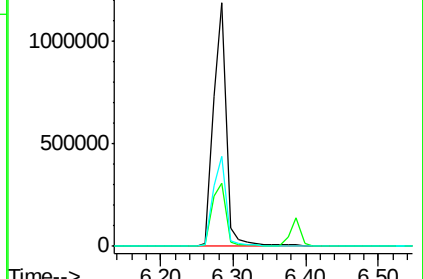

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.90 min Scan# 552


Delta R.T. -0.01 min

Lab File: BF086994.D

Acq: 14 May 2016 2:42

Tgt Ion: 136 Resp: 594365

Ion	Ratio	Lower	Upper
136	100		
137	11.2	8.8	13.2
54	12.9	5.0	7.4#
68	6.8	4.4	6.6#






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

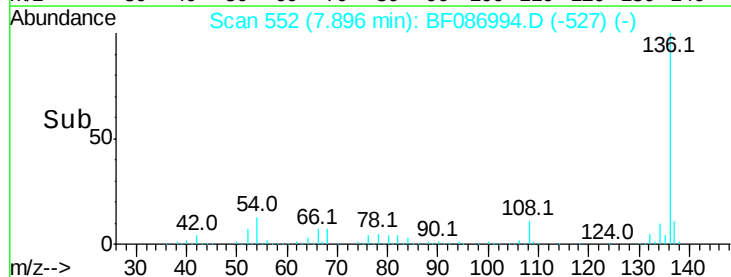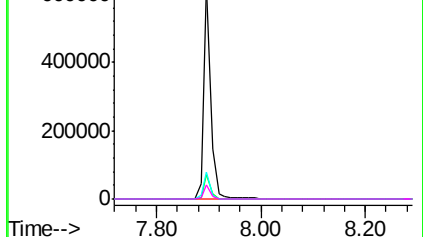

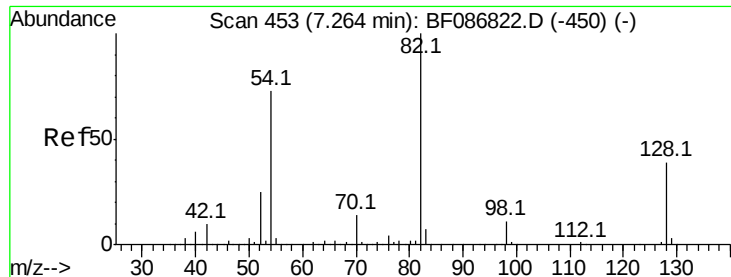

#23

Nitrobenzene-d5

Concen: 89.50 ng

RT: 7.19 min Scan# 490

Delta R.T. -0.01 min

Lab File: BF086994.D

Acq: 14 May 2016 2:42

Instrument :

BNA_F

ClientSampled :

TP14-2FT


Tot Ion: 82 Resp: 1059441

Ion Ratio Lower Upper

82 100

128 39.7 40.6 61.0#




54 69.7 38.1 57.1#

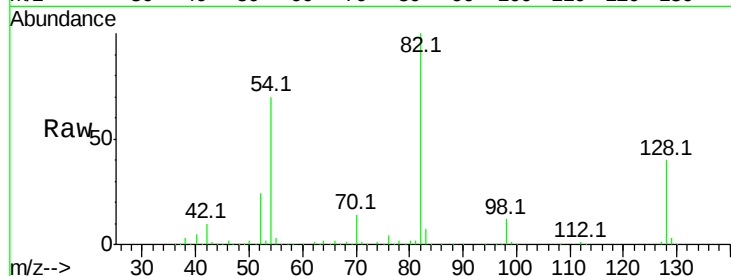

Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

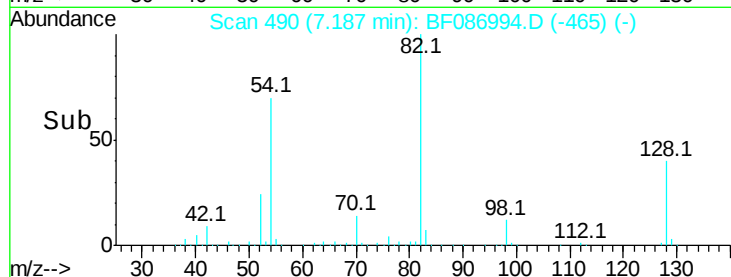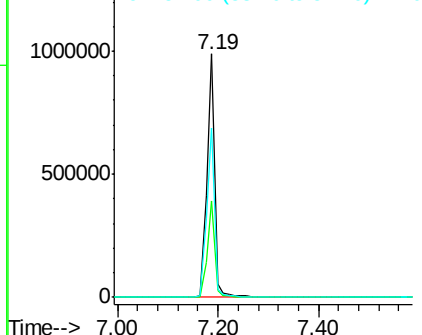

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.64 min Scan# 705

Delta R.T. -0.01 min

Lab File: BF086994.D

Acq: 14 May 2016 2:42


Tgt Ion: 164 Resp: 289330

Ion Ratio Lower Upper

164 100

162 102.2 82.8 124.2



160 46.6 36.9 55.3




Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

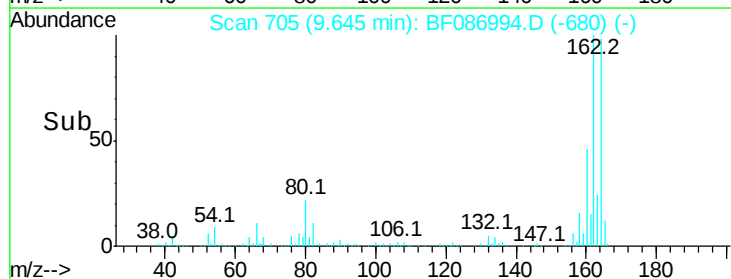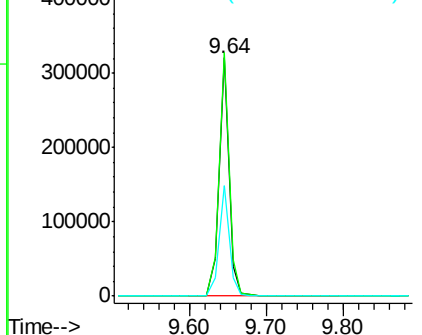


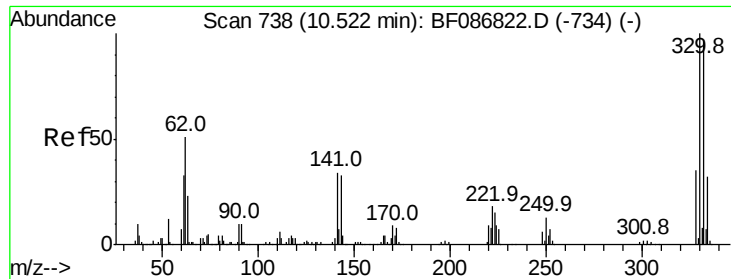




#41
 2,4,6-Tribromophenol
 Concen: 135.87 ng
 RT: 10.44 min Scan# 775
 Delta R.T. 0.00 min
 Lab File: BF086994.D
 Acq: 14 May 2016 2:42

Instrument :
 BNA_F
 ClientSampleId :
 TP14-2FT

Tot Ion:330 Resp: 416171
 Ion Ratio Lower Upper
 330 100
 332 96.8 79.0 118.4
 141 33.1 31.2 46.8

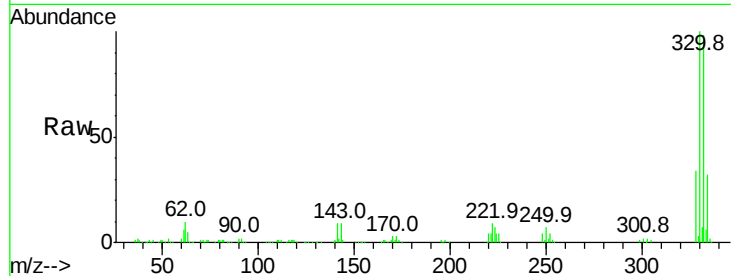


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

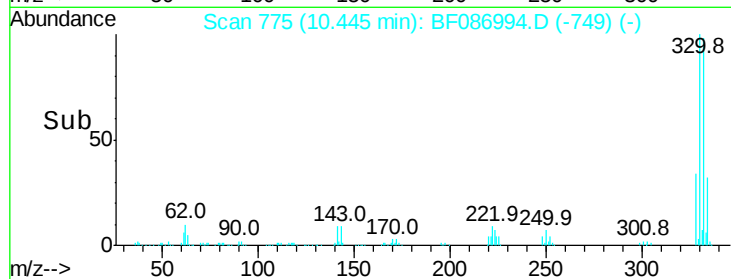
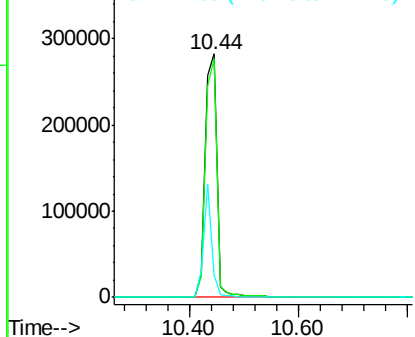



#44
 2-Fluorobiphenyl
 Concen: 96.98 ng
 RT: 8.98 min Scan# 647
 Delta R.T. 0.00 min
 Lab File: BF086994.D
 Acq: 14 May 2016 2:42

Tgt Ion:172 Resp: 1669512
 Ion Ratio Lower Upper
 172 100
 171 36.4 29.0 43.6
 170 24.8 19.8 29.8



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

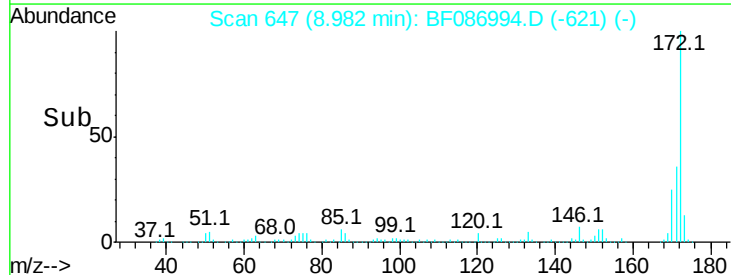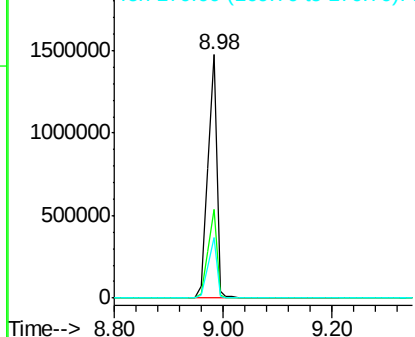


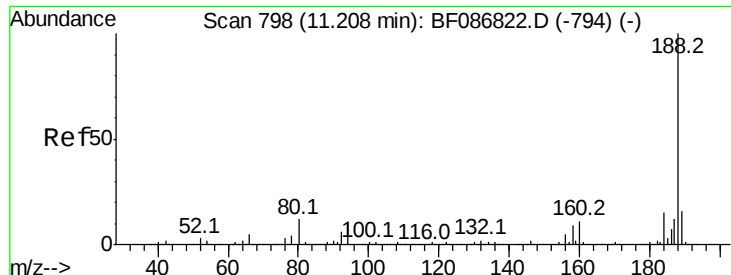




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.12 min Scan# 834
Delta R.T. -0.01 min
Lab File: BF086994.D
Acq: 14 May 2016 2:42

Instrument :
BNA_F
ClientSampleId :
TP14-2FT

Tot Ion:188 Resp: 542622
Ion Ratio Lower Upper
188 100
94 13.0 6.8 10.2#
80 14.9 7.1 10.7#

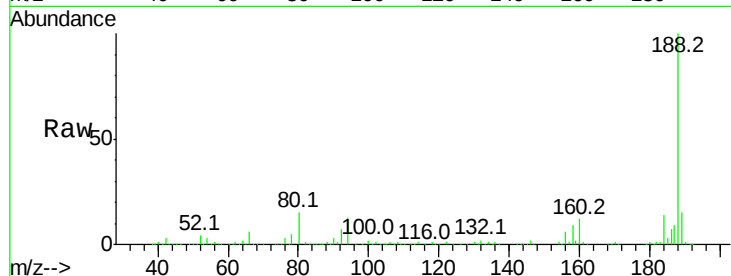


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

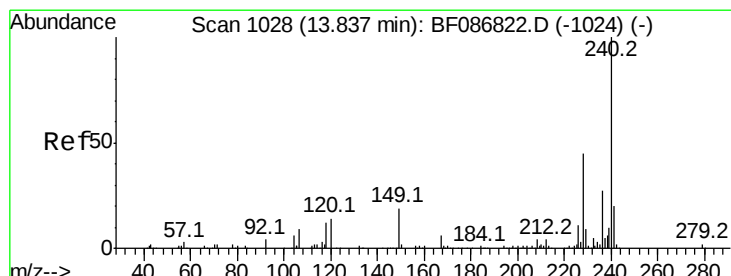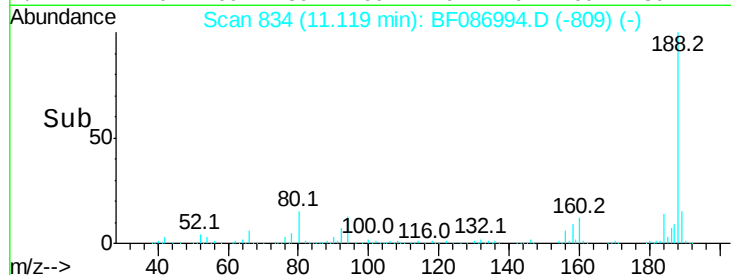
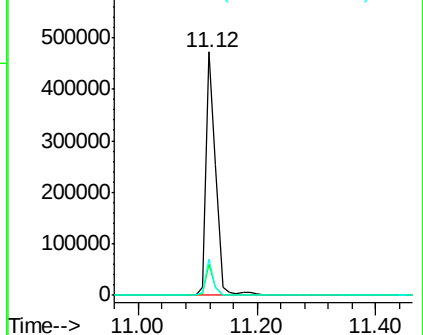



#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.75 min Scan# 1064
Delta R.T. -0.01 min
Lab File: BF086994.D
Acq: 14 May 2016 2:42

Tgt Ion:240 Resp: 455572
Ion Ratio Lower Upper
240 100
120 13.7 11.2 16.8
236 26.1 21.2 31.8

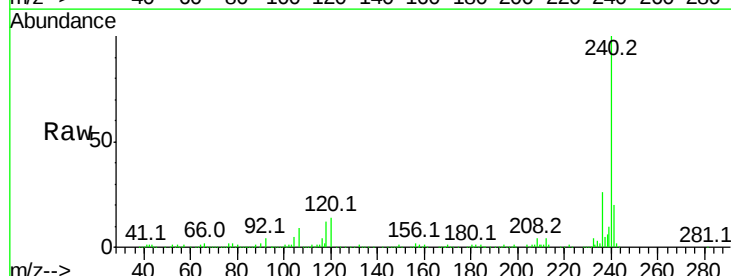

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

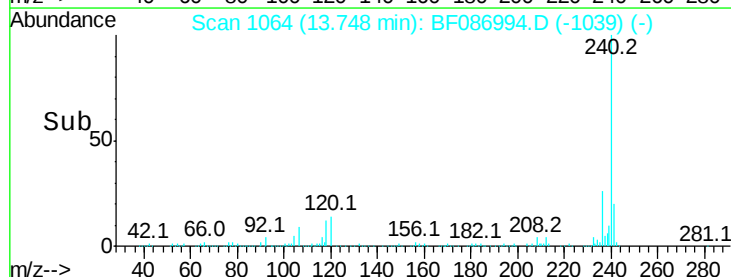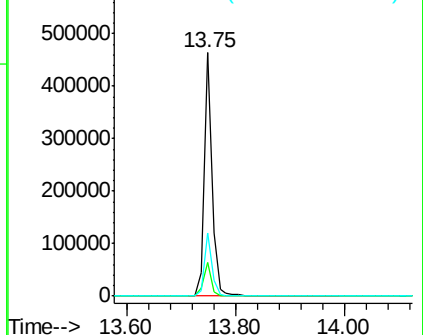

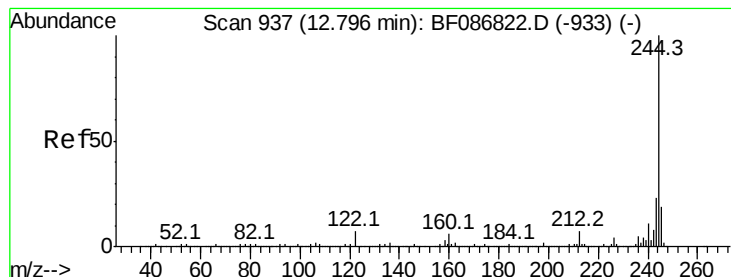

#78

Terphenyl-d14

Concen: 76.95 ng

RT: 12.71 min Scan# 973

Delta R.T. -0.01 min

Lab File: BF086994.D

Acq: 14 May 2016 2:42

Instrument :

BNA_F

ClientSampleId :

TP14-2FT


Tot Ion:244 Resp: 1652285

Ion Ratio Lower Upper

244 100

212 8.1 6.2 9.2




122 14.8 12.0 18.0



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

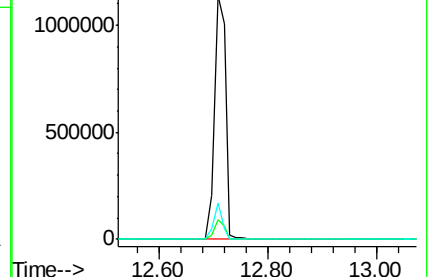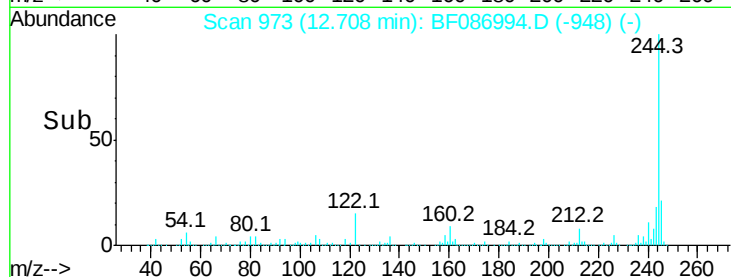

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.11 min Scan# 1183

Delta R.T. -0.01 min

Lab File: BF086994.D

Acq: 14 May 2016 2:42


Tgt Ion:264 Resp: 332379

Ion Ratio Lower Upper

264 100

260 24.3 19.5 29.3

265 21.2 17.3 25.9



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

