


Data Path : Z:\HPCHEM1\BNA F\Data\BF051316\
 Data File : BF086975.D
 Acq On : 13 May 2016 17:09
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 13 14:55:23 2016

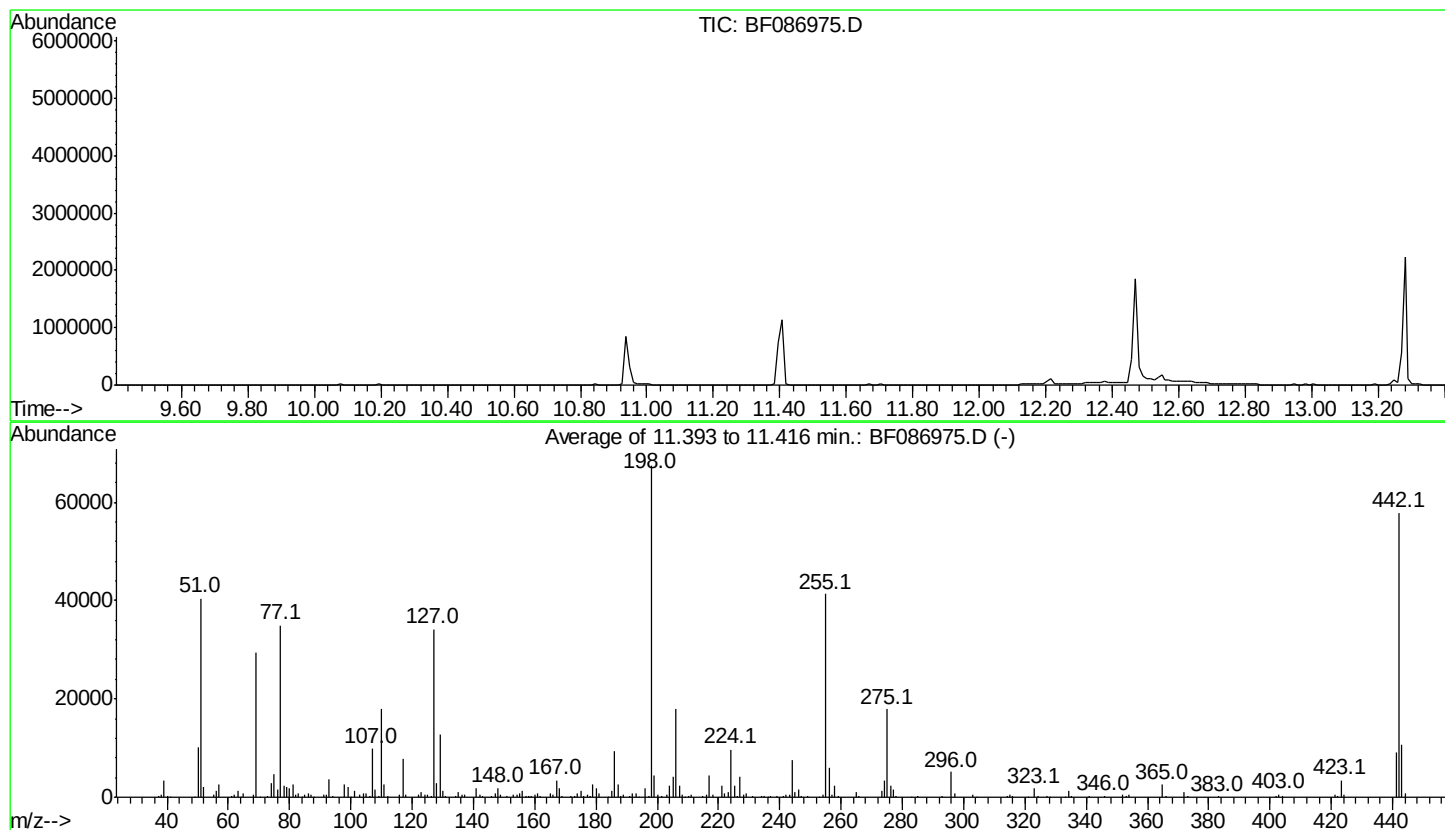

AutoFind: Scans 858, 859, 860; Background Corrected with Scan 854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.0	40481	PASS
68	69	0.00	2	1.9	549	PASS
69	198	0.00	100	43.5	29343	PASS
70	69	0.00	2	0.4	122	PASS
127	198	10	80	50.7	34177	PASS
197	198	0.00	2	0.3	203	PASS
198	198	100	100	100.0	67442	PASS
199	198	5	9	6.7	4544	PASS
275	198	10	60	26.5	17896	PASS
365	198	1	100	3.7	2494	PASS
441	442	0.01	24	15.9	9199	PASS
442	198	50	100	85.8	57857	PASS
443	442	15	24	18.4	10645	PASS