


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF051319\
 Data File : BF114220.D
 Acq On : 13 May 2019 11:14
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF051019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 10 15:56:46 2019

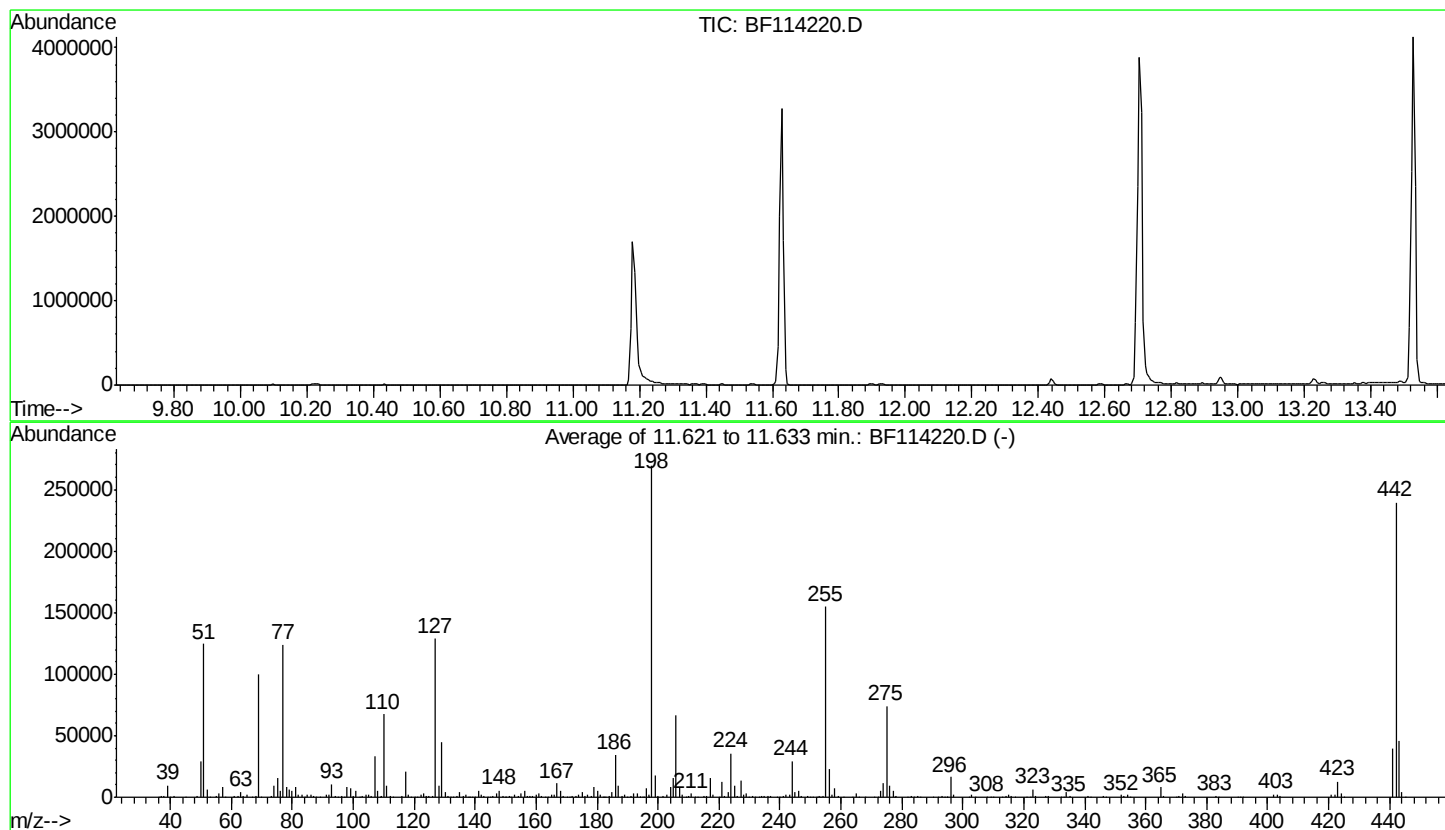

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.3	124738	PASS
68	69	0.00	2	1.5	1525	PASS
69	198	0.00	100	37.0	99672	PASS
70	69	0.00	2	0.5	529	PASS
127	198	10	80	47.7	128562	PASS
197	198	0.00	2	0.7	1818	PASS
198	198	100	100	100.0	269290	PASS
199	198	5	9	6.6	17645	PASS
275	198	10	60	27.6	74240	PASS
365	198	1	100	3.1	8230	PASS
441	198	0.01	100	14.6	39333	PASS
442	198	50	100	89.0	239592	PASS
443	442	15	24	19.2	45930	PASS