


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF051319\  
 Data File : BF114245.D  
 Acq On : 13 May 2019 23:14  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF051019.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri May 10 15:56:46 2019

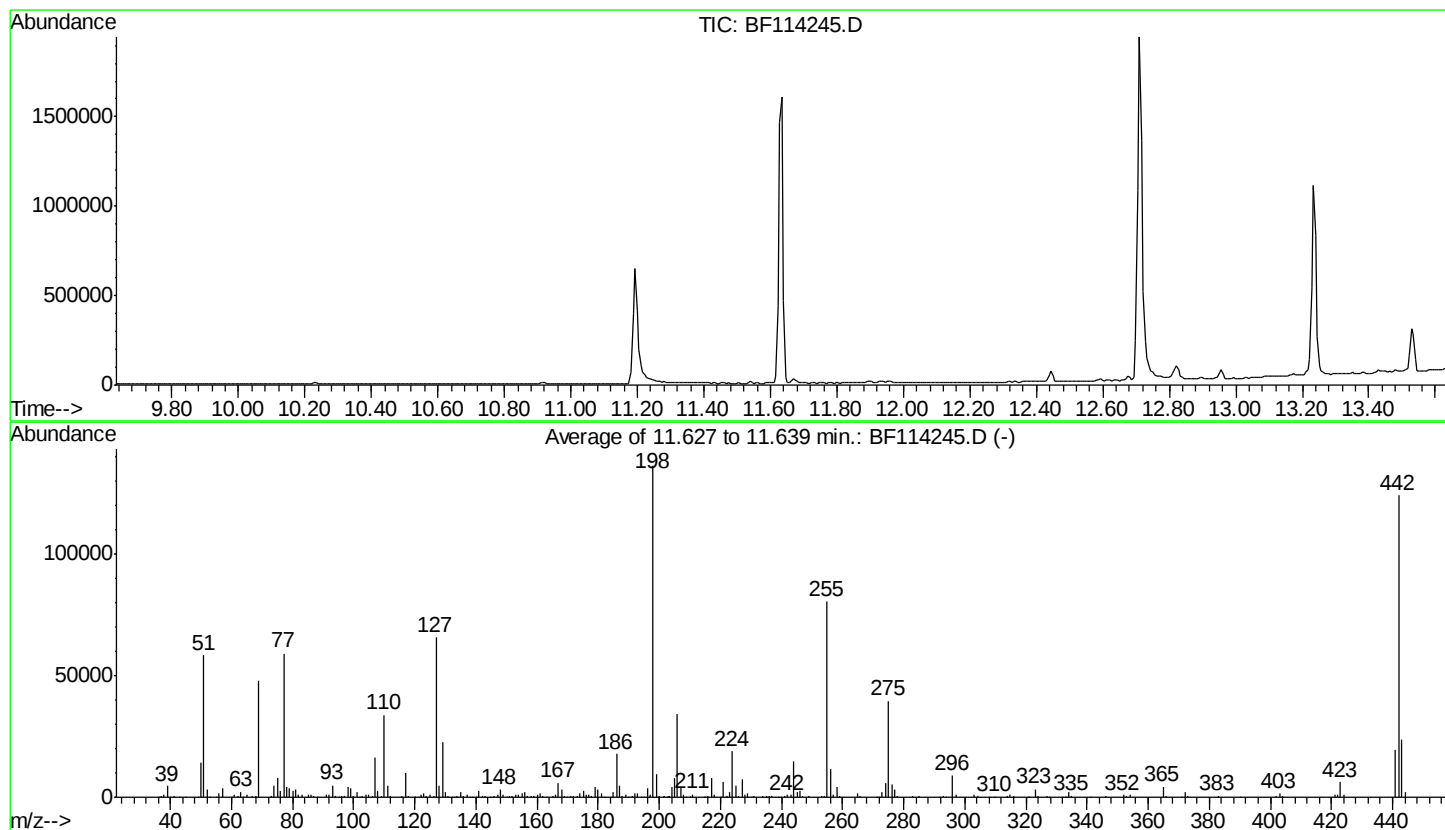

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 42.7      | 58199   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.7       | 789     | PASS             |
| 69          | 198          | 0.00         | 100          | 35.1      | 47779   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 48.1      | 65549   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.6       | 856     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 136272  | PASS             |
| 199         | 198          | 5            | 9            | 6.9       | 9395    | PASS             |
| 275         | 198          | 10           | 60           | 29.0      | 39469   | PASS             |
| 365         | 198          | 1            | 100          | 3.2       | 4314    | PASS             |
| 441         | 198          | 0.01         | 100          | 14.4      | 19574   | PASS             |
| 442         | 198          | 50           | 100          | 91.0      | 124048  | PASS             |
| 443         | 442          | 15           | 24           | 19.3      | 23901   | PASS             |